



Automation

Autoimmune diagnostics

Infection diagnostics

Allergy diagnostics

Antigen detection

Molecular genetic diagnostics

# Product Catalog



## Table of contents

<b>About us</b> .....	<b>4</b>
The EUROIMMUN Academy.....	8
The Institute for Quality Assurance.....	8
The Institute for Experimental Immunology.....	9
The Clinical Immunological Laboratory.....	9
Germany.....	12
Global business.....	13
Research and development.....	14
Scientific publications.....	14
Patents.....	16
<b>Detection methods</b> .....	<b>18</b>
Sample collection & Preatalytics.....	20
Dried Blood Spots (DBS): Sample collection at home – analysis in the lab.....	20
Indirect immunofluorescence.....	22
EUROIMMUN IFT: unrivalled quality and diversity.....	22
Microtiter ELISA.....	24
EUROIMMUN ELISA: quantitative and precise.....	24
Chemiluminescence immunoassays (ChLIA).....	26
EUROIMMUN ChLIA: Random access with chemiluminescence immunoassays.....	26
EUROASSAY.....	28
Line blots in chip format.....	28
EUROLINE.....	30
Multiparameter line blots for comprehensive antibody profiles.....	30
Westernblot/EUROLINE-WB.....	32
Reliable differentiation with Westernblots.....	32
EUROArray.....	34
Molecular genetic diagnostics with EUROArrays.....	34
EURORealTime.....	36
EUROIMMUN's expert solution for real-time PCR diagnostics.....	36
RIA.....	38
EUROIMMUN RIA: high-performance classic.....	38
<b>Automation</b> .....	<b>40</b>
Indirect immunofluorescence.....	42
MERGITE!.....	42
Sprinter.....	44
EUROLabWorkstation IFA.....	46
UNIQO 160.....	48
EUROStar III Plus.....	50
EUROPattern Microscope Live.....	52
EUROPattern.....	54
Microtiter ELISA.....	56
EUROIMMUN Analyzer.....	56
EUROLabWorkstation ELISA.....	58
Dried Blood Spots (DBS).....	60
Chemiluminescence.....	62
IDS-i10 and IDS-iSYS.....	62
Immunoblots.....	64
EUROBlotMaster.....	64
EUROLineScan.....	66
EUROBlotOne.....	68
Microwell Imager.....	70
Liquid handling.....	72
Pre-NAT II.....	72
EUROArray.....	74
EUROArrayProcessor.....	74
EUROArrayScanner.....	76
EUROArray.....	78
Eonis™ Q96.....	78
EURORealTime Analysis.....	80
Laboratory management.....	82
EUROLabOffice 4.0.....	82
EUROIMMUN CSF Software.....	84
<b>Special test kits and reagents for automation</b> .....	<b>86</b>
<b>Autoimmune diagnostics</b> .....	<b>98</b>
Rheumatology.....	100
Connective tissue diseases.....	100
Systemic lupus erythematosus.....	102
Vasculitis.....	104
Rheumatoid arthritis.....	106
Anti-phospholipid syndrome.....	108
Hepatology.....	110
Autoimmune hepatitis.....	110
Primary biliary cholangitis.....	112



Gastroenterology .....	114
Coeliac disease.....	114
Chronic inflammatory bowel diseases.....	116
Autoimmune gastritis/Pernicious anaemia.....	118
Endocrinology .....	120
Diabetes .....	120
Thyroid diseases .....	122
Neurology.....	124
Paraneoplastic neurological syndromes.....	124
Autoimmune encephalitis .....	126
Other diseases of the central and peripheral nervous system.....	128
Nephrology.....	130
Primary membranous nephropathy .....	130
Goodpasture's syndrome.....	132
Dermatology.....	134
Autoimmune dermatoses.....	134
<b>Products for autoimmune diagnostics .....</b>	<b>136</b>
<b>Infection diagnostics .....</b>	<b>166</b>
Bacteria.....	168
Bordetella.....	168
Borrelia.....	170
Treponema pallidum .....	172
Chlamydia.....	174
Viruses .....	176
SARS-CoV-2.....	176
Epstein-Barr virus.....	178
Hepatitis E virus .....	180
Fungi.....	182
Aspergillus.....	182
Special infection diagnostics .....	184
CSF diagnostics.....	184
TORCH.....	186
Tropical infections and emerging diseases.....	188
<b>Products for infection diagnostics .....</b>	<b>190</b>
<b>Allergy diagnostics .....</b>	<b>216</b>
Allergy profiles.....	218
Inhalation .....	218
Food .....	220
Atopy.....	222
Anti-CCD absorbent.....	224
Molecular allergy diagnostics.....	226
DPA-Dx (Defined partial allergen diagnostics).....	226
Insect venoms .....	228
<b>Products for allergy diagnostics .....</b>	<b>230</b>
<b>Antigen detection .....</b>	<b>242</b>
Neurodegenerative diseases.....	244
Beta-amyloid, tau proteins.....	244
Neurofilaments.....	246
Kidney markers .....	248
Uromodulin .....	248
Soluble CD163 (sCD163).....	250
Inflammatory bowel diseases.....	252
Calprotectin .....	252
IDS Products.....	254
Bone turnover markers.....	254
IDS Products.....	256
Calcium metabolism .....	256
<b>Products for antigen detection .....</b>	<b>258</b>
<b>Molecular genetic diagnostics .....</b>	<b>266</b>
Molecular genetics.....	268
ApoE.....	268
Factor V / Factor II / MTHFR.....	270
HLA-B27 .....	272
HLA-B57:01 .....	274
HLA-Cw6 .....	276
HLA-DQ2/DQ8.....	278
HFE gene (haemochromatosis).....	280
Lactose intolerance (LCT gene) and hereditary fructose intolerance .....	282
Molecular infection diagnostics.....	284
Dermatomycosis .....	284
Human papillomavirus .....	286
GynTect® – cervical cancer test .....	288
STI – Sexually transmitted infections .....	290
SARS-CoV-2.....	292
Zika Virus.....	294
Tuberculosis .....	296
<b>Products for molecular genetic diagnostics .....</b>	<b>298</b>
<b>Additional reagents and material .....</b>	<b>304</b>
<b>Index .....</b>	<b>308</b>



# About us








EUROIMMUN meets its needs for qualified personnel not only through its presence at recruitment or trade fairs and via advertisements, but also through its own training and dual degree programs. In addition to vocational school, the trainees undergo a comprehensive practical and theoretical program and receive intensive support in their everyday work life. At present, the company has more than 3200 employees, of which 112 are apprentices and students. 1685 employees have an academic qualification and 217 a doctoral degree. The percentage of female employees is around 60 percent.

The atmosphere at the company is productive and characterised by openness and respect. New employees at EUROIMMUN are given permanent contracts. All employees receive company pension benefits and premium payments for outstanding achievements. They also have the possibility of regular further training. The excellent company restaurant offers a variety of freshlycooked meals every day. The children are lovingly looked after in the company-owned crèche, kindergarten and after-school care, while their parents are working in the vicinity.

## EUROIMMUN in figures

<b>1987</b>	founded in Lübeck, Germany	<b>7</b>	offices in Germany
<b>USD 465 M</b>	annual group turnover in 2020	<b>16</b>	subsidiaries in other countries
<b>3233</b>	employees worldwide	<b>543</b>	own/in-licensed IP rights
<b>1685</b>	university graduates	<b>3<sup>rd</sup></b>	in the ranking of the most innovative small and medium-sized enterprises in Germany <i>(WirtschaftsWoche, April 2014)</i>
<b>217</b>	employees with doctoral degree		
<b>112</b>	apprentices		





## EUROIMMUN AG

The company · Global business



## The EUROIMMUN Academy

At the EUROIMMUN Academy qualified experts in medical laboratory diagnostics provide intensive theoretical and practical training at a high scientific level. The trainings comprise all topics from clinical pictures to diagnostic strategies, reagents, automation solutions and workflow generation based on laboratory software. The training content is optimally matched to meet the requirements and knowledge of the participants. Moreover, the courses are offered in different languages, e.g. German, English, French, Arabic, Swedish and Hungarian.

Every year, more than 1000 guests from over 100 countries, including customers, technicians, field staff and employees from all EUROIMMUN subsidiaries and distributors benefit from the trainings provided by the EUROIMMUN Academy. The trainings are certified according to ISO 9001:2008.

## The Institute for Quality Assurance

The Institute for Quality Assessment (IfQ) was founded in 2005 as an institution of EUROIMMUN Medizinische Labordiagnostika AG. It received accreditation in December 2008. The IfQ is responsible for organising, managing and evaluating quality assessment schemes. These are used to assess the capabilities of participating laboratories and provide an objective means to determine the reliability of measured data. After successful completion, participants are awarded a certificate. The assessment is performed using reference values, which are determined based on the consensus of the qualitative evaluations from external reference laboratories. These laboratories use reagents from different manufacturers for their analyses and share their test results.

Since recently, registered participants also have the possibility to carry out an evaluation of electronically provided immunofluorescence pictures or answer special exercise questions. At completion, they receive a certificate of participation. Together with the new literature area, the IfQ offers a complete package to enable participants to master their daily laboratory challenges in a competent, safe and reliable way. Moreover, the IfQ Lübeck is always happy to support laboratories with expert scientific advice.



## The Institute for Experimental Immunology

The Institute for Experimental Immunology was founded in 2005 to combine the scientific activities of researching new antigens and developing innovative methods. Highly qualified scientists work hand in hand on various projects. The institute creates the basis for the development of new test systems using state-of-the-art laboratory equipment, such as a mass spectrometer. The most outstanding achievements of the institute include the following:

- the cloning and expression of numerous recombinant antigens used in EUROIMMUN test systems, e.g. VlsE from *Borrelia* or glycolprotein G from HSV-2
- the development of so-called designer antigens, which consist of natural molecules that have been genetically optimised for antibody detection, e.g. PR3-hn-hr, GAF-3X, BP180-NC16A-4X or OspCadV
- RC-IFT (recombinant cell IFT) – cells transfected with diagnostically relevant antigens, which are used particularly in neurology and dermatology, e.g. NDMAR, aquaporin 4 and desmoglein 1 and 3
- the identification of previously unknown neuronal autoantigens using histo-immunoprecipitation, e.g. neuronal Na<sup>+</sup>/K<sup>+</sup>-ATPase (ATP1A3), inositol-1,4,5-trisphosphate receptor type 1 (ITPR1) and neurochondrin (NCDN)

## The Clinical Immunological Laboratory

EUROIMMUN and the Clinical Immunological Laboratory of Prof. Dr. med. Winfried Stöcker have a close research cooperation. The diagnostic spectrum of the clinical immunological laboratory encompasses the areas of autoimmune, infection and allergy diagnostics as well as molecular diagnostics.


Techniques used by the laboratory are mainly indirect immunofluorescence, enzyme immunoassays, chemiluminescence immunoassays, radioimmunoassays (RIA) and microarrays. Each day the laboratory receives several hundreds of patient samples from different countries for clarification of unusual or difficult result constellations. Here, EUROIMMUN customers can also obtain confirmation of their test results as a special service.




## EUROIMMUN AG

The company · Global business

About  
us

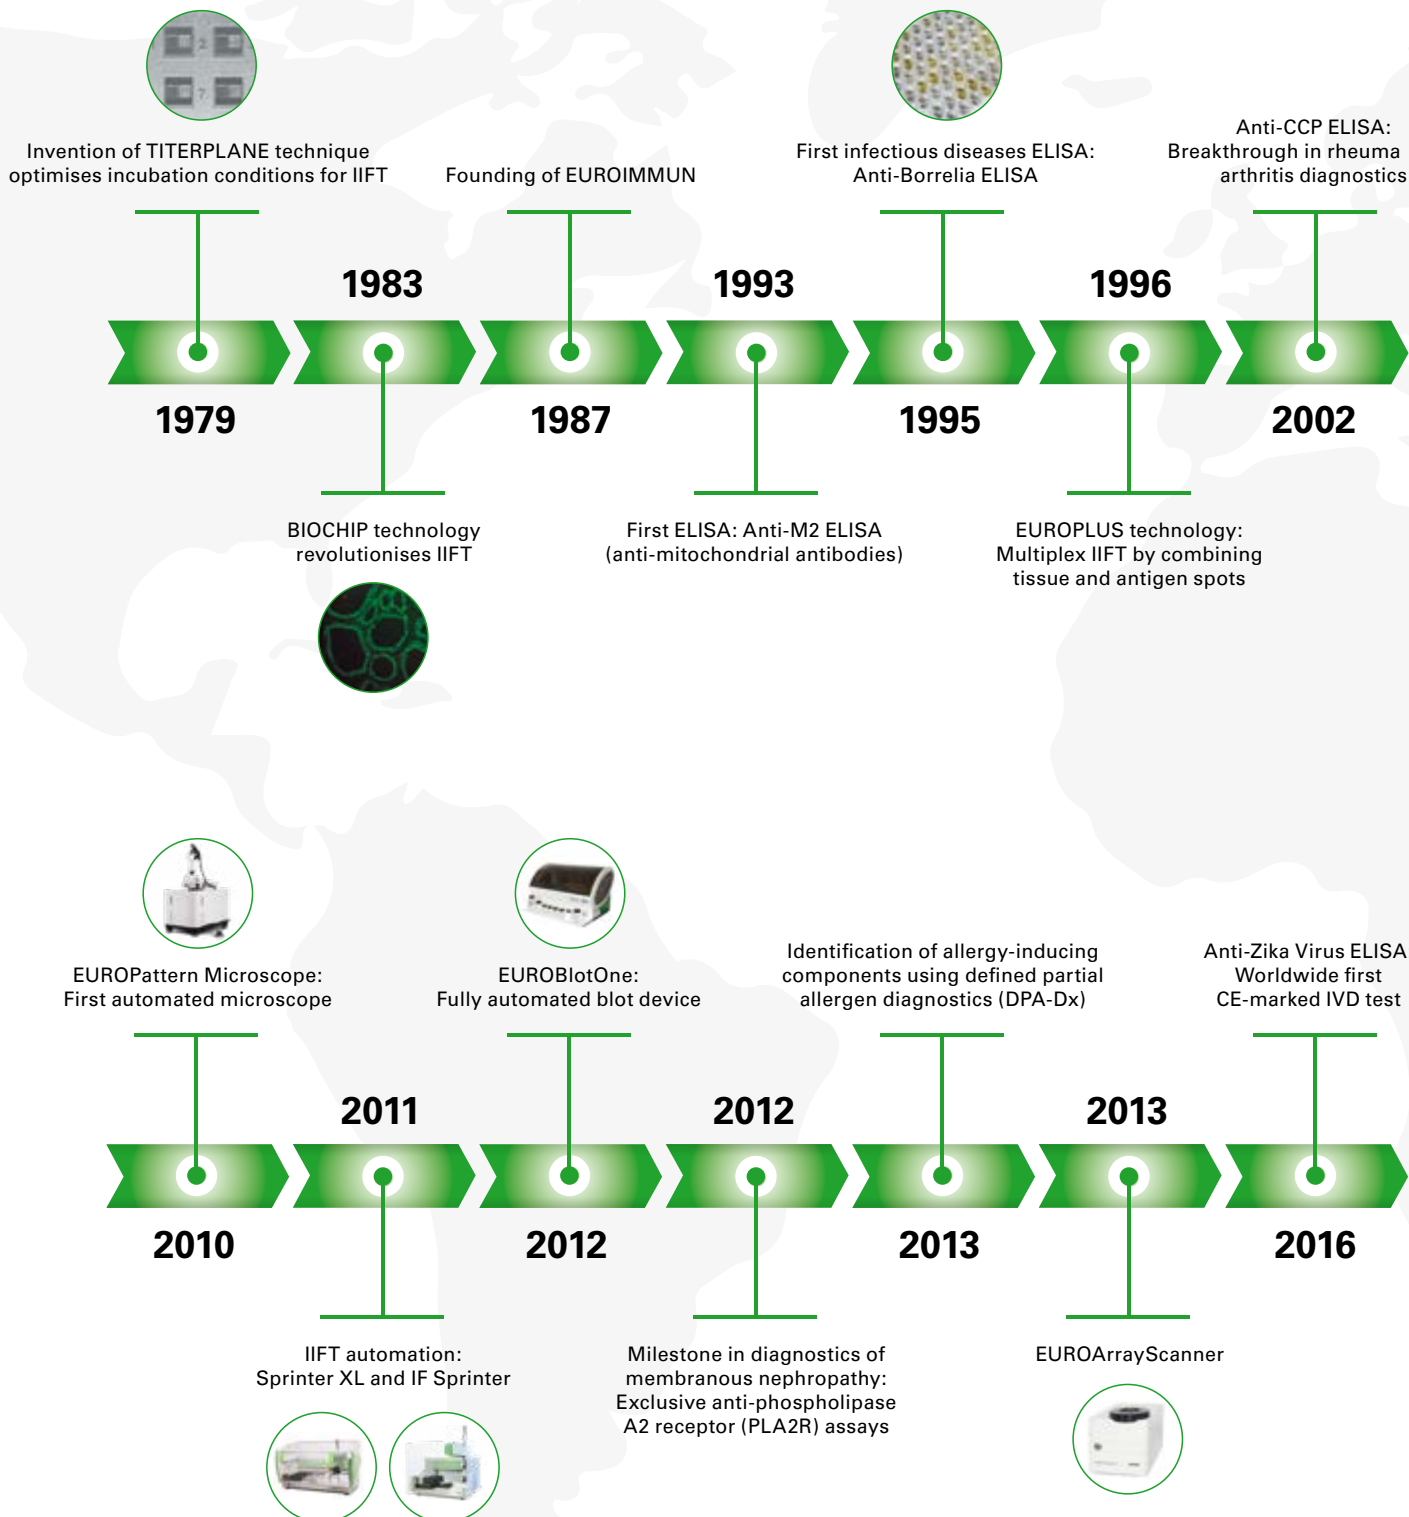

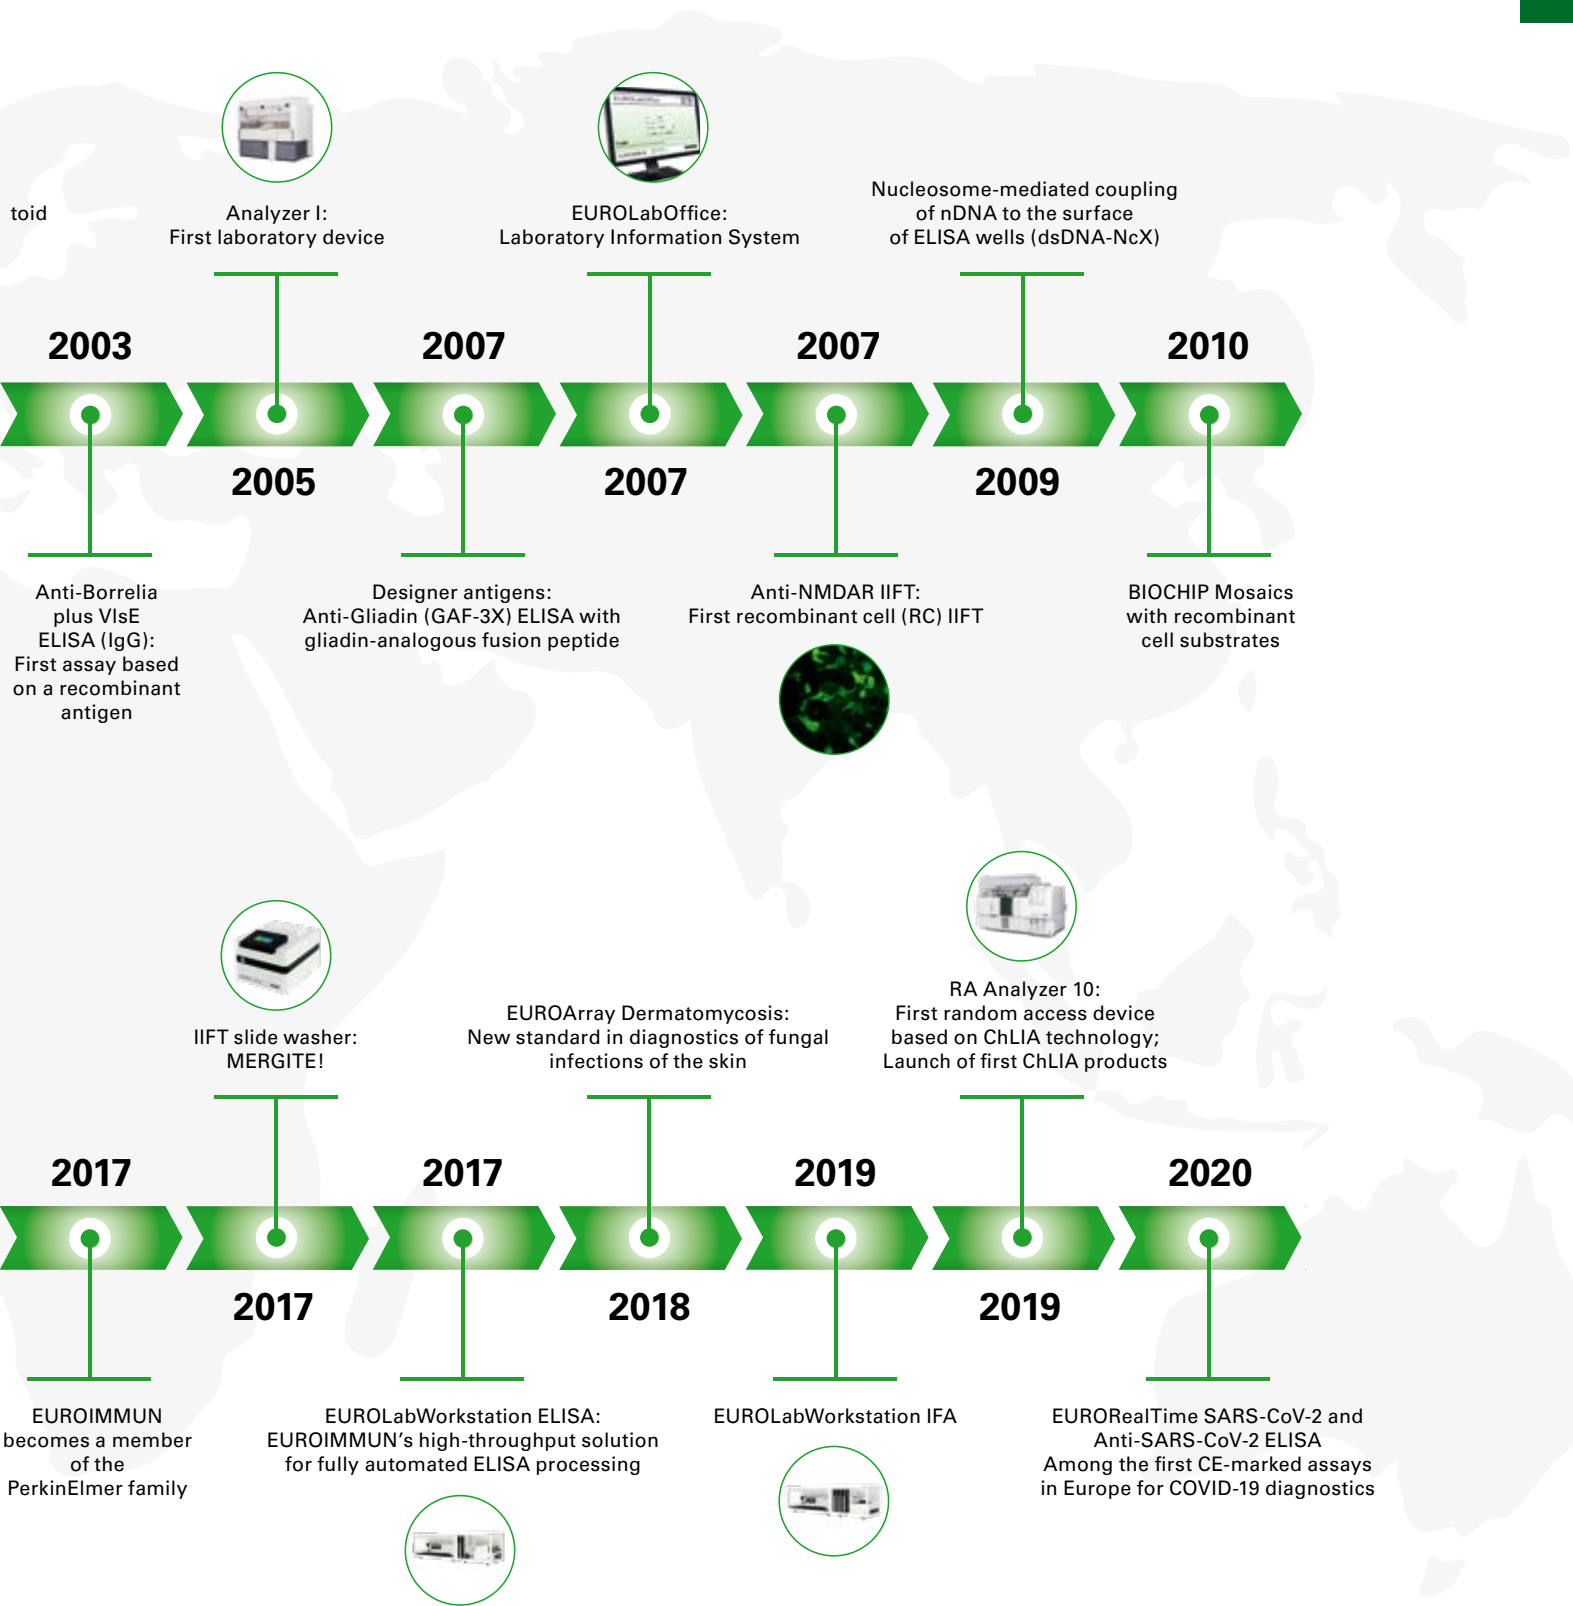





# EUROIMMUN AG

The company · Global business



About  
us


## Germany





For more information on this subject scan the QR code or enter the Quick Link code **q163** at [www.euroimmun.com](http://www.euroimmun.com)

## Global business

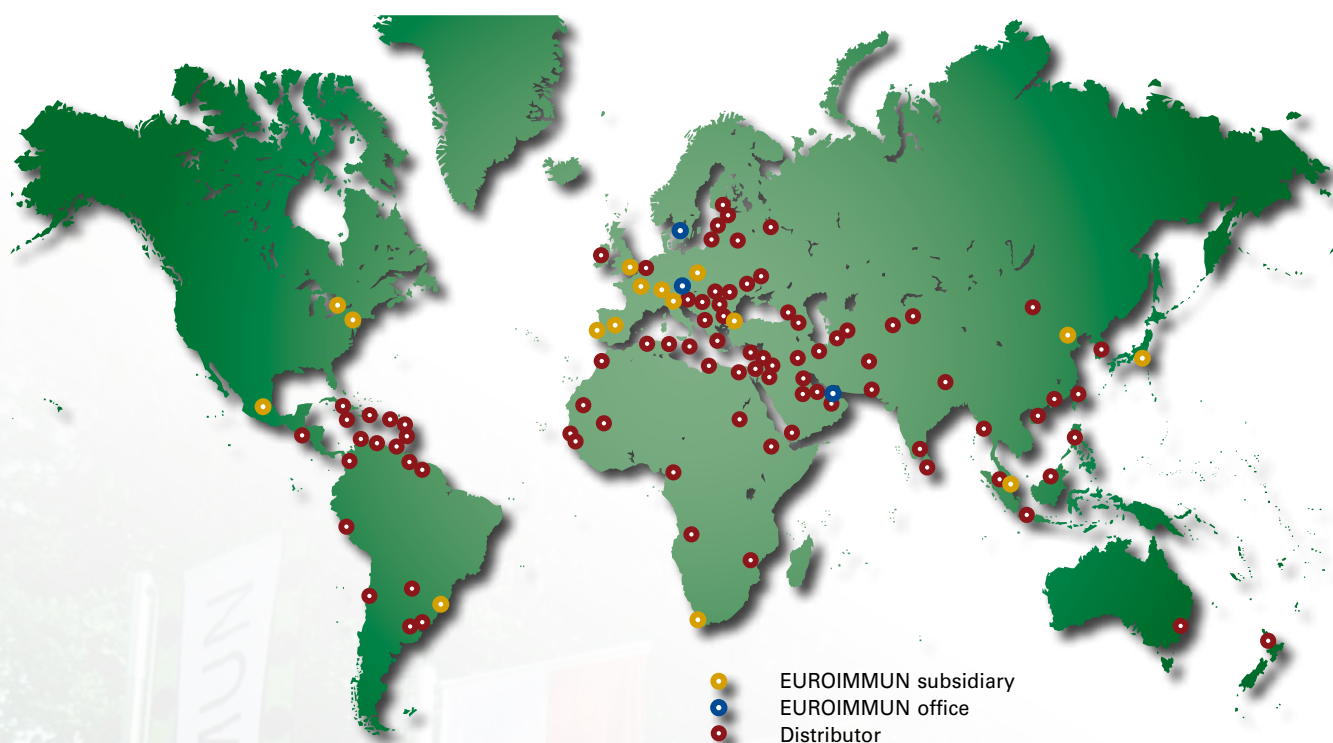

The main country to manufacture EUROIMMUN products is Germany. From there the products – reagents, automated analysis systems and evaluation software – are delivered to over 150 countries worldwide. Other production sites are Hangzhou/China and Singapore. Both subsidiaries produce EUROIMMUN products for their own markets.

All other subsidiaries are distribution companies, which also mostly have their own laboratories for training.



# Research and development

Scientific publications · Patents



For more information on this subject scan the QR code or enter the Quick Link code **q113** at [www.euroimmun.com](http://www.euroimmun.com)

## Scientific publications

### Publications 2020/2021

- Abu-Dayyeh I, Abu-Kwaik J, Weimann A, Abdelnour A. Prevalence of IgE-mediated sensitization in patients with suspected food allergic reactions in Jordan. *Immun Inflamm Dis*. 8(3):384-392 (2020).
- Álvarez I, Díez-Fairén M, Aguilar M, González JM, Ysamat M, Tartari JP, Carcel M, Alonso A, Brix B, Arendt P, Pastor P. Added value of cerebrospinal fluid multimarker analysis in diagnosis and progression of dementia. *Eur J Neurol*. Online ahead of print. (2021).
- Aubreville M, Bertram CA, Donovan TA, Marzali C, Maier A, Klopffleisch R. A completely annotated whole slide image dataset of canine breast cancer to aid human breast cancer research. *Sci Data* 7:417 (2020).
- Aubreville M, Bertram CA, Marzali C, Gurtner C, Dettwiler M, Schmidt A, Bartschlagger F, Mierz S, Fragoso M, Kerschaw O, Klopffleisch R, Maier A. Deep learning auto-perform veterinary pathologists in detecting the microscopically most active tumor region. *Sci Rep* 10:16447 (2020).
- Bossuyt X, Dillaerts D, Mahler M, Roggenbuck D, Leinfelder U, Hammar F, Schlumberger W, Otschowska N, Demouiseaux J. Standardisation of PR3-ANCA and MPO-ANCA: evaluation of certified reference materials. *Ann Rheum Dis*. 79:1520-1522 (2020).
- Boulo S, Kuhlmann J, Andreasson U, Brix B, Venkataraman I, Herbst V, Rutz S, Manuilova E, Vandjick M, Dekeyser F, Björke M, Pannese J, Charouf-Got J, Aucaric G, Mazrou S, Pinski G, Trappmann S, Schimmel H, Emms H, Quaglia M, Portalius E, Kercka M, Shaw LM, Lame M, Chambers V, Vanderschelle H, Stoops E, Leinenbach A, Bittner T, Jenkins RG, Kostanjekovic V, Lewczuk P, Gombom J, Zetterberg H, Zegers I, Blennow K. First amyloid  $\beta$ -42 certified reference material for re-calibrating commercial immunoassays. *Alzheimers Dement*. 16(11):1493-1503 (2020).
- Braasch J, Ostermann S, Mackiewicz M, Bardot C, Pagnoux C, Borchardt-Löhöfner V, Latwain E. *Trichinella spiralis* - New method for sample preparation and objective detection of specific antigens using chemiluminescence immunoassay. *Veterinary Parasitology* 4, 4:100033 (2020).
- Corman VM, Nagy P, Ostermann S, Arlojt J, Liljander A, Barua R, Gupta AD, Haki-Mudin F, Juhasz J, Wernery U, Drosten C. Hepatitis E virus genotype 7 RNA and antibody kinetics in naturally infected dromedary camels, United Arab Emirates. *Emerg. Inf. Dis*. 26(9):2214-2217 (2020).
- Dährnich C, Saschenbrecker S, Gunnarsson I, Schlumberger W, Ronco P, Debic H. Development of a standardized chemiluminescence immunoassay for the detection of autoantibodies against human M-type phospholipase A2 receptor in primary membranous nephropathy. *Kidney Int Rep*. 5(2):182-188 (2020).
- Derer S, Bresthack AK, Pletsch C, Jendrek ST, Nitsche T, Bokemeyer A, Hov JR, Schäffler H, Bettenworth D, Grassl GA, Sina C. Inflammatory Bowel Disease-associated GP2 Autoantibodies Inhibit Mucosal Immune Response to Adherent-Invasive Bacteria. *Inflamm Bowel Dis*. 26(12): 1856-1868 (2020).
- Dubey D, Honorat JA, Shelly S, Klein CJ, Komorowski L, Mills JR, Brakopp S, Probst C, Lennon VA, Pittcock SJ, McKeon A. Contactin-1 autoimmunity: Serologic, neurologic, and pathologic correlates. *Neuroimmunol Neuroinflamm*. 7(4): e771 (2020).
- Eftymiou G, Liaskos C, Simopoulou T, Marou E, Patrikiou E, Schepfer T, Meyer W, Daoussi D, Sakkas LI, Bogdanos DP. Antigen-specific humoral responses against Helicobacter pylori in patients with systemic sclerosis. *Immunol Res*. 68(1):39-47 (2020).
- Ehlers AM, Otten HG, Wierzbica E, Flügge U, Le TM, Knulst AC, Suer W. Detection of specific IgE against linear epitopes from Gal 1 has additional value in diagnosing hen's egg allergy in adults. *Clin Exp Allergy*. 50:1415-1423 (2020).
- Ehlers AM, Rohwer S, Otten HG, Brix B, Le TM, Suer W, Knulst AC. IgE-binding to vicilin-like antimicrobial peptides is associated with systemic reactions to macadamia nut. *Clin Transl Allergy* 10:55 (2020).
- Hall S, Janelidze S, Zetterberg H, Brix B, Mattsson N, Surova Y, Blennow K, Hansson O. Cerebrospinal fluid levels of neurogranin in Parkinsonism disorders. *Mov Disord*. 35(3):513-518 (2020).
- Marzali C, Aubreville M, Bertram CA, Stavyt J, Jasensky AK, Bartschlagger F, Fragoso-Garcia M, Barton AK, Elsemann S, Jabari S, Krauth J, Madhu P, Voigt J, Hill J, Klopffleisch R, Maier A. Deep Learning-Based Quantification of Pulmonary Hemosiderophages in Cytology Slides. *Sci Rep*. 10:3755 (2020).
- Mastroianni-Kirzajta J, Homig N, Schlumberger W. **Corrigendum: Autoantibodies in renal diseases - clinical significance and recent developments in serological detection.** *Front Immunol*. 11(11):424 (2020).
- Naides SJ, Genzen JR, Abel G, Bashlenseh C, Ansari MQ. **Antinuclear Antibodies (ANA) testing method variability: a survey of participants in the College of American Pathologists' (CAP) Proficiency Testing Program.** *J Rheumatol*. Mar 15;19(3):1903-1903 (2020).
- Naides SJ. **Correctly Interpreting SARS-CoV-2 Serologic Assays.** *Clin Chem*. 66(9):1244-1245 (2020).
- Pan H, Steixner-Kumar AA, Seelbach A, Deutsch N, Ronnenberg A, Tapken D, von Ahsen N, Mitjans M, Worthmann H, Trippel R, Klein-Schmidt C, Schopf N, Rentsch K, Begemann M, Wienands J, Stöcker W, Weisenborn K, Hollmann M, Nave KM, Lühder F, Ehrenreich H. **Multiple inducers and novel roles of autoantibodies against the obligatory NMDAR subunit NR1: a translational study from chronic life stress to brain injury.** *Mol Psychiatry*. <https://doi.org/10.1038/s41380-020-0672-1> (2020).
- Raulf M, Jordan D, Auer H, Warnecke J, Lepenius B, Strube C. **A new ELISA and western blot technique based on recombinant TES antigen and/or larval antigen for the detection of toxocarasis in humans.** *Parasitology*. 1-8 (2020).
- Reichert S, Jurianz E, Pütz N, Schlumberger W, Dährnich C, Johannsen N, Altermann W, Schlaf G, Keyßer G, Schaefer C, Schaller HG, Schulz S. **E. peridontitis a prognostic factor in order to indicate antibodies against citrullinated peptides in patients with rheumatoid arthritis?** *Clin Exp Rheumat* 38:227-238 (2020).
- Reindl M, Schanda K, Woodhall M, Tea F, Ramanathan S, Sagen J, Fryer JP, Mills J, Teegen B, Mindorf S, Ritter N, Krumrei U, Stöcker W, Eggert J, Flanagan EP, Ramberger M, Hegen H, Rostasy K, Berger T, Leite MI, Palaca J, Irani SR, Dale RC, Probst C, Probst M, Briot F, Pittcock SJ, Waters P. **International multicenter examination of MOG antibody assays.** *Neuroimmunol Neuroinflamm*. 7(2): e674 (2020).
- Richter CD. **Response to „Continental Drift? Do European clinical genetic testing laboratories have a patent problem?“. Eur J Hum Genet.** 28(5):535-536 (2020).
- Tsouris Z, Liaskos C, Dardiotis E, Schepfer T, Tsimourtoiu V, Meyer W, Hadjiorgioiu G, Bogdanos DP. **A comprehensive analysis of antigen-specific autoimmune liver disease related autoantibodies in patients with multiple sclerosis.** *Auto Immun Highlts*. 11(1):7 (2020).
- Schmidt E, Steinhagen K, Rupp J. **Heavy exposure of children aged 9 to 12 years with SARS-CoV-2 did not lead to infection.** *J Pediatric Infect Dis Soc*. 9(5): 620-621 (2020).
- Van Beek N, Krüger S, Fuhrmann T, Lemcke S, Goletz S, Probst C, Komorowski L, Di Zenzo G, Dmochowski M, Drenovska K, Horn M, Jedlickova H, Kowalewski C, Medemica L, Murrell D, Patsatsi A, Geller S, Uzun S, Vassileva S, Zhu X, Fechner K, Zillikens D, Stöcker W, Schmidt E, Rentsch K. **Multicenter prospective study on multiantigenic diagnostics of autoimmune bullous dermatoses using the BIO-CHIP technology.** *J Am Acad Dermatol* 83(5): 1315-1322 (2020).
- Venkataraman I, Naides SJ. **The development of new diagnostic tests for neurologic disorders in the commercial laboratory environment.** *Clin Lab Med*. Sep;40(3):331-339 (2020).
- Warnecke JM, Pollmann M, Borchardt-Löhöfner V, Moreira-Soto A, Kaya S, Gamze Sener A, Gómez-Guzmán E, Figueroa-Hernández L, Li W, Li F, Buska K, Zakazewska K, Ziolkowska K, Jantz J, Ott A, Schepfer T, and Meyer W. **Seroprevalence of antibodies against ToRCR infectious pathogens in women of childbearing age residing in Brazil, Mexico, Germany, Poland, Turkey and China.** *Epidemiology and Infection*. 148:E271 (2020).
- Weisser H, Steinhagen K, Höcker R, Borchardt-Löhöfner V, Anvari Ö, Kern PM. **Evaluation of dried blood spots as alternative sampling material for serological detection of anti-SARS-CoV-2 antibodies using established ELISAs.** *Clin Chem Lab Med*. In press (2020).
- Zelini P, Fornara C, Furione M, Sarasini A, Klemens J, Arossa A, Spinillo A, Gerna G, Lillini D. **Determination of anti-pS2 IgM and anti-IgG IgG by ELISA as a novel diagnostic tool for detection of early and late phase of primary human cytomegalovirus infections during pregnancy.** *J Clin Virol*. 120:348-352 (2020).
- Álvarez I, Díez-Fairén M, Aguilar M, González JM, Ysamat M, Tartari JP, Carcel M, Alonso A, Brix B, Arendt P, Pastor P. **Added value of cerebrospinal fluid multimarker analysis in diagnosis and progression of dementia.** *Eur J Neurol* 28(4):1142-1152 (2021).
- Bogdanos DP, Gkoutzouras A, Papadopoulos V, Liaskos C, Patrikiou E, Tsigalou C, Sarantziotis A, Hagiouannou J, Schepfer T, Meyer W, Sakkas LI, Papandreou C. **Anti-Ro52 antibody is highly prevalent and a marker of better prognosis in patients with ovarian cancer.** *Clin Chim Acta* 521:199-205 (2021).
- Brändle SM, Cerina M, Weber S, Held K, Menke AF, Alcalá C, Gebert D, Herrmann AM, Peliköfer H, Gerdies LA, Bittner S, Leyradt F, Teegen B, Komorowski L, Kümpfel T, Hähnel R, Meuth SG, Casassini S, Meuser N, Betzler E, Dornheim K. **Cross-reactivity of a pathogenic autoantibody to a tumor antigen in GABA receptor encephalitis.** *Proc Natl Acad Sci USA* 118(9):e1916337118 (2021).
- Braasch J, Beck-Jendroschek V, Voss K, Achenbach A, Berger HG, Harder M, Gräser Y, Schwarz T. **Arthroderma crassum auf menschlicher Haut.** *Hautartz* 3 (2021).
- Dolscheid-Pommerich R, Bartok E, Renn M, Kümmerer BM, Schulte B, Schmitthausen RM, Stollhoff-Wagner B, Strecek H, Saschenbrecker S, Steinhagen K, Hartmann G. **Correlation between a quantitative anti-SARS-CoV-2 IgG ELISA and neutralization activity.** *J Med Virol* doi: 10.1002/jmv.27287 (2021).
- Emmerich P, von Possel R, Descherner C, Ahmeti S, Berisha L, Halli B, Jakupi X, Sherri F, Messing C, Borchardt-Löhöfner V. **Comparison of diagnostic performances of ten different immunoassays detecting anti-CHRV IgM and IgG antibodies from acute to subsided phases of Crimean-Congo hemorrhagic fever.** *PLoS Negl Trop Dis* 15(3):e0008280 (2021).
- Emmerich P, von Possel R, Hemmer CJ, Fritzsche C, Geerdes-Fenge H, Menge B, Messing C, Borchardt-Löhöfner V, Descherner C, Steinhagen K. **Longitudinal detection of SARS-CoV-2-specific antibody responses with different serological methods.** *J Med Virol* 93(10):5816-5824 (2021).
- Emtani S, Ghorbanipoor S, Mayer-Hain S, Kridin K, Komorowski L, Probst C, Hashimoto T, Pas HH, Męcińska-Jurzdził K, Czajkowski R, Recke A, Sunderkötter C, Schneider SW, Hundt JE, Zillikens D, Schmidt E, Ludwig RJ, Hammes CM. **Pathogenic Activation and Therapeutic Blockage of Fc  $\alpha$  Receptor-Expressing Polymorphonuclear Leukocytes in IgA Pemphigus.** *J Invest Dermatol* S0022-202X(21)01412-3 (2021).
- Hansson O, Batrla R, Brix B, Carrillo MC, Corradini V, Edelmayer RM, Esquivel RN, Hall C, Lawson J, Bastard NL, Molinuevo JJ, Nissenbaum LK, Rutz S, Salomone SJ, Teunissen CE, Travnichan C, Unek RM, Vanderschelle H, Vandjick M, Wahl S, Weber CJ, Zetterberg H, Blennow K. **The Alzheimer's Association International guidelines for handling of cerebrospinal fluid for routine clinical measurements of amyloid  $\beta$  and tau.** *Alzheimers Dement* 17(9):1575-1582 (2021).
- Haubold B, Klötzl F, Hellberg L, Thompson D, Cavalari M. **Fur: Find Unique Genomic Regions for Serological PCR.** *Bioinformatics* btab059 (2021).
- Hoxha E, Stahl RAK, Reinhard L, Kühn A, Schlumberger W, Dährnich C. **A new chemiluminescence immunoassay for phospholipase A2 receptor 1 autoantibodies allows early identification of autoantibody recurrence in patients with membranous nephropathy.** *Kidney Int Rep* 6(4):928-935 (2021).
- Jarius S, Wilken D, Haas J, Ruprecht K, Komorowski L, Wildemann B. **Parvovirus B19 and mumps virus antibodies are major constituents of the intrathecal immune response in European patients with MS and increase the diagnostic sensitivity and discriminatory power of the MRZ reaction.** *J Neurol* 268(10):3759-3765 (2021).
- Knight V, Askar MZ, Ntrivalas E, Nandiwada SL, Peterson LK, Tebo AE, Kadkhoda K, Schmitz JL, Naides SJ, Snyder MR, Sridhish Akhis AA. **Highlights of the 33rd annual scientific meeting of the Association of Medical Laboratory Immunologists (AMLI).** *J Immunol Methods* 492:112994 (2021).
- Markowitz R, Pauli D, Dargavaniene E, Steinhagen K, Engel S, Herbst V, Zapf D, Krüger C, Sharifzadeh S, Schomburg B, Leyboldt F, Rupp J, Görg S, Junker R, Wandinger KP. **The temporal course of T- and B-cell-responses to vaccination with BNT162b2 and mRNA-1273.** *Clin Microbiol Infect* S1198-743X(21)00496-1 (2021).
- Marzali C, Aubreville M, Bertram CA, Maier J, Bergler C, Krüger C, Voigt J, Breininger K, Klopffleisch R, Maier A. **EXACT: a collaboration toolset for algorithm-aided annotation of images with annotation version control.** *Sci Rep* 11(1):4343 (2021).
- Miske R. **What do we know about autoantibodies against the novel Purkinje cell antigen DAGLA7?** *AACC Academy Scientific Shorts*. May 18, 2021.
- Miske R, Scharf M, Stark P, Dietzel H, Bien CI, Borchers C, Kermer P, Ott A, Denno Y, Rochow N, Borowski K, Finke C, Teegen B, Probst C, Komorowski L. **Autoantibodies against the Purkinje cell protein RGSS in paraneoplastic cerebellar syndrome.** *Neuroimmunol Neuroinflamm* 9(5):e87 (2021).
- Naides SJ. **D. Naides reply.** *J Rheumatol* 48(7):1190 (2021).
- Niederhauser C, Tinguely C, Dreier J, Vollmer T, Marti HP, Nickel B, Klemens JM, Warnecke JM, Gowland P. **Comparison of a new IgE-EIA for the detection of anti-Plasmodium antibodies with two currently used assays.** *Transfus Med Hemother* 48:265-271 (2021).
- Raulf M, Jordan D, Auer H, Warnecke J, Lepenius B, Strube C. **A new ELISA and western blot technique based on recombinant TES antigen and/or larval antigen for the detection of toxocarasis in humans.** *Parasitology* 149(3):333-340 (2021).
- Reinhard L, Thomas C, Machalitz M, Latwain E, Weiss LS, Vitu J, Wiewch T, Stahl RAK, Hoxha E. **Characterization of THSD7A-antibodies not binding to glomerular THSD7A in a patient with diabetes mellitus but no membranous nephropathy.** *Sci Rep* 11(1):16188 (2021).
- Rietveld A, Wienko J, Visser E, Vree Egbertus W, Schlumberger W, van Engelen B, van Royen-Kerkhof A, Lu H, Wedderburn L, Saris C, Tansley S, Pruin G. **Juvenile Dermatomyositis Research Group and Dutch Myositis Consortium. Anti-cytosolic 5-nucleotidase 1A autoantibodies are absent in juvenile dermatomyositis.** *Arthritis Rheumatol* 73(7):1323-1333 (2021).
- Schanda K, Peschl P, Lerch M, Seebacher B, Mindorf S, Ritter N, Probst M, Hegen H, Di Pauli F, Wenzel EM, Lechner C, Baumann M, Mariotto S, Ferrari S, Saiz A, Ferrali M, Leite MIS, Irani SR, Palaca J, Lutterotti A, Kümpfel T, Valkovic S, Marignier R, Waters P, Rostasy K, Berger T, Probst C, Höttinger R, Reindl M. **Differential Binding of Autoantibodies to MOG Isoforms in Inflammatory Demyelinating Diseases.** *Neuroimmunol Neuroinflamm* 9(5):e1027 (2021).
- Steinhagen K, Borchardt-Löhöfner V, Siba K, Klemens JM, Latwain E, Saschenbrecker S, Schlumberger W. **Serological detection of specific IgA autoantibodies against Zika virus nonstructural protein 1 contributes to diagnosis of acute Zika virus infections.** *In: Martin CR et al. (Hrsg.): Zika virus impact, diagnosis, control, and models.* The Neuroscience of Zika virus. Elsevier Academic Press, Volume 2:293-302 (2021).
- Van Anh Pham C, Rademacher F, Hinrichs H, Beck-Jendroschek V, Harder M, Brasch J, Gläser R, Harder J. **Expression of epidermal antimicrobial peptides is increased in tinea pedis.** *Mycoses* 64(7):763-770 (2021).
- Weisser H, Steinhagen K, Höcker R, Borchardt-Löhöfner V, Anvari Ö, Kern PM. **Evaluation of dried blood spots as alternative sampling material for serological detection of anti-SARS-CoV-2 antibodies using established ELISAs.** *Clin Chem Lab Med* 59(5):978-985 (2021).
- Wilke JH, Hindermand M, Berghoff SA, Zehsler S, Arinrad S, Ronnenberg A, Barnkothke N, Steiner-Kumar AA, Röglin S, Stöcker W, Hollmann M, Nave KA, Lühder F, Ehrenreich H. **Autoantibodies against NMDA receptor 1 modify rather than cause encephalitis.** *Mol Psychiatry* doi: 10.1038/s41380-021-01238-3 (2021).





## Scientific presentations (abstracts/posters) 2020/2021

- Aubreville M, Bertram CA, Jabari S, Marzahi C, Klopfeisch R, Maier A. **Inter-Species, Inter-Tissue Domain Adaptation for Mitotic Figure Assessment - Learning New Tricks from Old Dogs.** Bildverarbeitung für die Medizin, virtueller Kongress (2020).
- Bertram CA, Aubreville M, Marzahi C, Maier A, Klopfeisch R. **How Big is Big Enough? A Large-Scale Histological Dataset of Mitotic Figures.** Bildverarbeitung für die Medizin, virtueller Kongress (2020).
- Bertram CA, Veta M, Marzahi C, Stathonikos N, Maier A, Klopfeisch R, Aubreville M. **Are Pathologist-Defined Labels Reproducible? Comparison of the TUPAC16 Mitotic Figure Dataset with an Alternative Set of Labels.** 22. International Conference on Medical Image Computing & Computer Assisted Intervention, virtueller Kongress (2020).
- Braasch J, Ostermann S, Mackiewicz M, Liljander A, Borchardt-Lohöfner V, Lattwein E, Schlumberger W. **New approach for the detection of Trichinella spiralis in slaughtered pigs.** 6. World One Health Congress, virtuelle Konferenz (2020).
- Ehlers AM, Rohwer S, Otten HG, Brix B, Le TM, Suer W, Knulst AC. **Vicilin-like antimicrobial peptides from macadamia nut are clinically relevant allergens.** European Academy of Allergy & Clinical Immunology (EAACI), virtueller Kongress (2020).
- Gebhardt AK, Klemens O, Sabalza M, Stiba K, Saschenbrecker S, Steinhagen K. **Comparison of enzyme-linked immunosorbent assays for the diagnosis of dengue virus infections.** 3. International Conference on Zika Virus and Aedes Related Infections, Washington DC, USA (2020).
- Hoffmann K, Rosenstock P, Borchardt-Lohöfner V, Dichtl K, Seybold U, Ormanns S, Horns H, Wagener J, Herbst V. **Diagnostic performance of a novel Aspergillus Antigen ELISA.** 30. European Congress of Clinical Microbiology & Infectious Diseases, Paris, France (2020).
- Marzahi C, Bertram CA, Aubreville M, Petrick A, Wailer K, Gläsel AC, Frago M, Merz S, Bartschlagger F, Hoppe J, Langenhanen A, Jasensky AK, Voigt J, Klopfeisch R, Maier A. **Are fast labeling methods reliable? A case study of computer-aided expert annotations on microscopy slides.** 23. International Conference on Medical Image Computing and Computer-Assisted Intervention (MICCAI), virtueller Kongress (2020).
- Marzahi C, Aubreville M, Bertram CA, Gerlach S, Maier J, Voigt J, Hill J, Klopfeisch R, Maier A. **Is crowd-algorithm collaboration an advanced alternative to crowd-sourcing on cytology slides?** International workshop on Algorithms - Systeme - Anwendungen, virtueller Workshop (2020).
- Marzahi C, Aubreville M, Voigt J, Maier A. **Classification of leukemic B-lymphoblast cells from blood smear microscopic images with an attention-based deep learning method and advanced augmentation techniques.** IEEE International Symposium on Biomedical Imaging (ISBI), virtueller Kongress (2020).
- Menge B, Klemens O, Klemens JM, Sabalza M, Jittmitrathap A, Leauangwuthong P, and Steinhagen K. **Testing for specific serum IgA in addition to IgM has an added value in acute secondary dengue virus infections.** 2. Polythematic Autoimmunity Congress, virtueller Kongress (2020).
- Miske R, Scharf M, Jäger D, Hahn S, Denno Y, Benkhadra F, Rochow N, Probst C, Teegen B, Stöcker W, Komorowski L. **Identification of DAGLA as an autoantibody target in cerebellar or hippocampal degeneration.** 2. Polythematic Autoimmunity Congress, virtueller Kongress (2020).
- Moraes Soane M, Freitas Henriques D, Abreu Lima J, Caricio Martins L, Muligg N, Sabalza M, Klemens O, Steinhagen K. **Novel screening ELISA for sensitive detection of Mayaro virus-infected patients.** 3. International Conference on Zika Virus and Aedes Related Infections, Washington DC, USA (2020).
- Pollmann M, Borchardt-Lohöfner V, Moreira-Soto A, Kaya S, Gamze Sener A, Gómez-Guzmán E, Figueroa-Hernández L, Li W, Li F, Buska K, Zakaszewska, Ziolkowska K, Janz J, Ott A, Scheper T, Meyer W. **Seroprevalence of ten TORCH infectious pathogens in women residing in Europe, Latin America and China.** 30. European Congress of Clinical Microbiology & Infectious Diseases, Paris, France (2020).
- Weisser H, Steinhagen K, Höcker R, Borchardt-Lohöfner V, Anvari Ö, Kern PM. **Evaluation of dried blood spots as alternative sampling material for serological detection of anti-SARS-CoV-2 antibodies using established ELISA.** ECCMID Conference on Coronavirus Disease (ECCVID), virtuelle Konferenz (2020).
- Alessio MG, Previtali G, Agatea L, Favaro E, de Gaspari P, Novel P, Confettura A, Diberger B, Wenderoth A, Herbst V. **A new chemiluminescence immunoassay for the detection of faecal calprotectin.** 15th Dresden Symposium on Autoantibodies, Dresden, Germany (2021).
- Braasch J, Ostermann S, Mackiewicz M, Borchardt-Lohöfner V, Lattwein E, Schlumberger W. **New approach for the detection of Trichinella spiralis in slaughtered pigs.** 29th Annual Meeting of the German Society for Parasitology, virtueller Kongress (2021).
- Diekmann K, Menge B, Klemens O, Klemens JM, Saschenbrecker S, Jittmitrathap A, Leauangwuthong P, Steinhagen K. **Added value of testing for specific serum IgA additionally to IgM in acute secondary dengue virus infections.** 31st European Congress of Clinical Microbiology & Infectious Diseases (ECCMID), virtueller Kongress (2021).
- Diberger B, Sabalza M, Schlumberger W, Dähnrich C. **Increased sensitivity for detection of IgA autoantibodies against tissue transglutaminase using a new chemiluminescence immunoassay.** 34th Meeting of Medical Laboratory Immunologists (AMLI), Austin, USA (2021).
- Diberger B, Sabalza M, Schlumberger W, Dähnrich C. **Increased sensitivity for detection of IgA autoantibodies against tissue transglutaminase using a new chemiluminescence immunoassay.** AACC Annual Scientific Meeting & Clinical Lab Expo, Atlanta, USA (2021).
- Diberger B, Schlumberger W, Dähnrich C. **Increased sensitivity for detection of IgA autoantibodies against tissue transglutaminase using a new chemiluminescence immunoassay.** 12th International Congress on Autoimmunity (ICA), virtueller Kongress (2021).
- Feng X, Liu Y, Karl I, Ott A, Scheper T, Meyer W, Yan HP. **Diagnostic value of autoantibodies against D-3-phosphoglycerate dehydrogenase (PGDH) among patients with liver diseases.** 12th International Congress on Autoimmunity (ICA), virtueller Kongress (2021).
- Filippis C, Binder F, Lickfeld M, Schröder AK, Klemens JM, Saschenbrecker S, Steller U. **Novel PCR test to differentiate between SARS-CoV-2, Influenza A and B.** 31st European Congress of Clinical Microbiology & Infectious Diseases (ECCMID), virtueller Kongress (2021).
- Filippis C, Binder F, Lickfeld M, Schröder AK, Klemens JM, Saschenbrecker S, Steller U. **Novel PCR test to differentiate between SARS-CoV-2, Influenza A and B.** 8th International Meeting on Emerging Diseases and Surveillance (IMED), virtueller Kongress (2021).
- Goletz S, Karl I, Probst C, Komorowski L, Schlumberger W, Zillikens D, Stöcker W, Schmidt E. **Cell-based immunofluorescence test applying recombinant laminin 332 for the serological diagnosis of pemphigoid.** 12th International Congress on Autoimmunity (ICA), virtueller Kongress (2021).
- Goletz S, Probst C, Komorowski L, Schlumberger W, Zillikens D, Stöcker W, Schmidt E. **Cell-based immunofluorescence test applying recombinant laminin 332 for the serological diagnosis of pemphigoid.** 15th Dresden Symposium on Autoantibodies, Dresden, Germany (2021).
- Goletz S, Venkataraman I, Karl I, Probst C, Komorowski L, Schlumberger W, Zillikens D, Stöcker W, Schmidt E. **Cell-based immunofluorescence test applying recombinant laminin 332 for the serological diagnosis of pemphigoid.** 34th Meeting of Medical Laboratory Immunologists (AMLI), Austin, USA (2021).
- Goletz S, Venkataraman I, Karl I, Probst C, Komorowski L, Schlumberger W, Zillikens D, Stöcker W, Schmidt E. **Cell-based immunofluorescence test applying recombinant laminin 332 for the serological diagnosis of pemphigoid.** AACC Annual Scientific Meeting & Clinical Lab Expo, Atlanta, USA (2021).
- Hoffmann K, Diekmann K, Klemens JM, Saschenbrecker S, Herbst V. **Novel antigen assay for acute diagnostics of COVID-19 in the laboratory.** 31st Annual Congress of Clinical Microbiology & Infectious Diseases (ECCMID), virtueller Kongress (2021).
- Hoffmann K, Diekmann K, Klemens JM, Saschenbrecker S, Herbst V, Sabalza M. **Novel antigen assay for acute diagnostics of COVID-19 in the laboratory.** AACC Annual Scientific Meeting & Clinical Lab Expo, Atlanta, USA (2021).
- Honorat JA, Lopez-Chiriboga AS, Kryzer TJ, Lennaova VA, Komorowski L, Scharf M, Stöcker W, Hinson SR, Pittock SJ, Klein CJ, McKeon A. **Autoimmune gait disturbance accompanying adaptor protein 382-IgG.** 12th International Congress on Autoimmunity (ICA), virtueller Kongress (2021).
- Honorat JA, Lopez-Chiriboga AS, Kryzer TJ, Lennaova VA, Komorowski L, Venkataraman I, Scharf M, Stöcker W, Hinson SR, Pittock SJ, Klein CJ, McKeon A. **Autoimmune gait disturbance accompanying adaptor protein 382-IgG.** 34th Meeting of Medical Laboratory Immunologists (AMLI), Austin, USA (2021).
- Honorat JA, Lopez-Chiriboga AS, Kryzer TJ, Lennaova VA, Komorowski L, Venkataraman I, Scharf M, Stöcker W, Hinson SR, Pittock SJ, Klein CJ, McKeon A. **Autoimmune gait disturbance accompanying adaptor protein 382-IgG.** AACC Annual Scientific Meeting & Clinical Lab Expo, Atlanta, USA (2021).
- Hoxha E, Stahl RAK, Brix SR, Venkataraman I, Witte T, Brock J, Schlumberger W, Dähnrich C. **Increased sensitivity for PR3-ANCA using a novel chemiluminescence immunoassay.** AACC Annual Scientific Meeting & Clinical Lab Expo, Atlanta, USA (2021).
- Hoxha E, Stahl RAK, Brix SR, Witte T, Brock J, Schlumberger W, Dähnrich C. **Increased sensitivity for PR3-ANCA using a novel chemiluminescence immunoassay.** 12th International Congress on Autoimmunity (ICA), virtueller Kongress (2021).
- Hoxha E, Stahl RAK, Reinhard L, Kühnl A, Burmeister Y, Saschenbrecker S, Schlumberger W, Dähnrich C. **A new chemiluminescence immunoassay for phospholipase A2 receptor 1 autoantibodies allows earlier identification of relapses in patients with membranous nephropathy.** 12th International Congress on Autoimmunity (ICA), virtueller Kongress (2021).
- Hoxha E, Stahl RAK, Reinhard L, Kühnl A, Burmeister Y, Saschenbrecker S, Schlumberger W, Dähnrich C. **A new chemiluminescence immunoassay for phospholipase A2 receptor 1 autoantibodies allows earlier identification of relapses in patients with membranous nephropathy.** 13. Jahrestagung der Deutschen Gesellschaft für Nephrologie (DGfN), Rostock, Germany (2021).
- Hoxha E, Stahl RAK, Reinhard L, Sabalza M, Kühnl A, Burmeister Y, Saschenbrecker S, Schlumberger W, Dähnrich C. **A new chemiluminescence immunoassay for phospholipase A2 receptor 1 autoantibodies allows earlier identification of relapses in patients with membranous nephropathy.** 34th Meeting of Medical Laboratory Immunologists (AMLI), Austin, USA (2021).
- Janz J, Ott A, Lindae A, Scheper T, Schlumberger W, Meyer W. **Multiparameter assay for the detection of IgA antibodies in autoimmune gastrointestinal disease.** 12th International Congress on Autoimmunity (ICA), virtueller Kongress (2021).
- Janz J, Ott A, Lindae A, Scheper T, Schlumberger W, Meyer W. **Multiparameter assay for the detection of IgG antibodies in autoimmune gastrointestinal disease.** 12th International Congress on Autoimmunity (ICA), virtueller Kongress (2021).
- Janz J, Ott A, Richter M, Scheper T, Schlumberger W, Meyer W. **Addition of cN1A as a target for detection of autoantibodies associated with Inclusion Body Myositis to a multiparameter line blot immunoassay for autoimmune inflammatory myopathies.** 12th International Congress on Autoimmunity (ICA), virtueller Kongress (2021).
- Janz J, Ott A, Richter M, Scheper T, Schlumberger W, Meyer W. **Addition of cN-1A as a target for detection of autoantibodies associated with Inclusion Body Myositis to a multiparameter line blot immunoassay for autoimmune inflammatory myopathies.** AACC Annual Scientific Meeting & Clinical Lab Expo, Atlanta, USA (2021).
- Kühnl A, Burmeister Y, Sabalza M, Saschenbrecker S, Komorowski L, Probst C, Pesce G, Schlumberger W, Dähnrich C. **Novel Anti-ATP4B ELISA to aid the diagnosis of autoimmune gastritis.** 34th Meeting of Medical Laboratory Immunologists (AMLI), Austin, USA (2021).
- Kühnl A, Burmeister Y, Sabalza M, Saschenbrecker S, Komorowski L, Probst C, Pesce G, Schlumberger W, Dähnrich C. **Novel Anti-ATP4B ELISA to aid the diagnosis of autoimmune gastritis.** AACC Annual Scientific Meeting & Clinical Lab Expo, Atlanta, USA (2021).
- Kühnl A, Burmeister Y, Saschenbrecker S, Komorowski L, Probst C, Pesce G, Schlumberger W, Dähnrich C. **Novel Anti-ATP4B ELISA to aid the diagnosis of autoimmune gastritis.** 12th International Congress on Autoimmunity (ICA), virtueller Kongress (2021).
- Langner N, Wilken D, Klemens O, Doltschaid-Pommerich R, Renn M, Streck H, Kümmerer BM, Schulte B, Frank K, Karl A, Klemens JM, Saschenbrecker S, Hartmann G, Steinhagen K. **Correlation between quantitative anti-SARS-CoV-2 IgG ELISA and neutralization tests.** 31st European Congress of Clinical Microbiology & Infectious Diseases (ECCMID), virtueller Kongress (2021).
- Markewitz R, Pauli D, Dargavainiene J, Steinhagen K, Engel S, Herbst V, Zapf D, Krüger C, Shehadeh S, Schomburg B, Leyppoldt F, Rupp J, Görg S, Junker R, Wandinger KP. **No evidence for short-term induction of antinuclear antibodies by vaccination with BNT162b2 and mRNA-1273.** 15th Dresden Symposium on Autoantibodies, Dresden, Germany (2021).
- Menge B, Klemens JM, Mentz J, Diekmann K, Saschenbrecker S, Tran KH, Hetherington M, Steinhagen K. **Sensitive detection of antibodies in patients with acute Coxiella burnetii infection.** World Microbe Forum, Congress of the American Society for Microbiology (ASM) and the Federation of European Microbiological Societies (FEMS), virtueller Kongress (2021).
- Menge B, Klemens JM, Mentz J, Diekmann K, Saschenbrecker S, Tran KH, Hetherington M, Steinhagen K. **Sensitive detection of antibodies in patients with acute Coxiella burnetii infection.** 8th International Meeting on Emerging Diseases and Surveillance (IMED), virtueller Kongress (2021).
- Miske R, Mindorf S, Ott A, Borowski K, Jäger D, Honorat J, McKeon A, Teegen B, Probst C, Komorowski L. **Detection of anti-AKS autoantibodies in patients with limbic encephalitis by indirect immunofluorescence assay and line blot.** 15th Dresden Symposium on Autoantibodies, Dresden, Germany (2021).
- Miske R, Scharf M, Hahn S, Denno Y, Benkhadra F, Rochow N, Probst C, Teegen B, Stöcker W, Komorowski L. **Identification of DAGLA as an autoantibody target in cerebellar or hippocampal degeneration.** 12th International Congress on Autoimmunity (ICA), virtueller Kongress (2021).
- Miske R, Venkataraman I, Scharf M, Hahn S, Denno Y, Benkhadra F, Rochow N, Probst C, Teegen B, Stöcker W, Komorowski L. **Identification of DAGLA as an autoantibody target in cerebellar or hippocampal degeneration.** 34th Meeting of Medical Laboratory Immunologists (AMLI), Austin, USA (2021).
- Miske R, Venkataraman I, Scharf M, Hahn S, Denno Y, Benkhadra F, Rochow N, Probst C, Teegen B, Stöcker W, Komorowski L. **Identification of DAGLA as an autoantibody target in cerebellar or hippocampal degeneration.** AACC Annual Scientific Meeting & Clinical Lab Expo, Atlanta, USA (2021).
- Ott A, Scharf M, Miske R, Jäger D, Honorat J, Komorowski L, Scheper T, Meyer W. **Parallel detection of antibodies against CD22L and CD29L increases the diagnostic specificity in serological diagnostics of paraneoplastic cerebellar degeneration.** 15th Dresden Symposium on Autoantibodies, Dresden, Germany (2021).
- Pollmann M, Klemens O, Klemens JM, Saschenbrecker S, Steinhagen K. **Development of a novel NS1-based ELISA for the detection of specific IgG antibodies against Japanese encephalitis virus.** 23rd Annual Meeting of the European Society for Clinical Virology (ESCV), virtueller Kongress (2021).
- Pollmann M, Ott A, Liefeld M, Borchardt-Lohöfner V, Scheper T, Meyer W. **Novel line blot differentiates between IgG antibodies against three SARS-CoV-2 antigens and against further seasonal coronaviruses.** 22nd Annual Meeting of the European Society for Clinical Virology (ESCV), virtueller Kongress (2021).
- Schäfer J, Menge B, Dibbern J, Borchardt-Lohöfner V, Steinhagen K, Schlumberger W. **Novel ELISA based on purified and recombinant antigens from Toxocara canis exhibits a high diagnostic sensitivity.** 29th Annual Meeting of the German Society for Parasitology, virtueller Kongress (2021).
- Schäfer J, Menge B, Stiba K, Dibbern J, Borchardt-Lohöfner V, Steinhagen K, Schlumberger W. **Novel ELISA based on purified and recombinant antigens from Toxocara canis exhibits a high diagnostic sensitivity.** 8th International Meeting on Emerging Diseases and Surveillance (IMED), virtueller Kongress (2021).
- Scharf M, Miske R, Denno Y, Probst C, Jäger D, Borowski K, Teegen B, Komorowski L. **Strategy for the detection of anti-septin antibodies by indirect immunofluorescence assay.** 15th Dresden Symposium on Autoantibodies, Dresden, Germany (2021).
- Stiba K, Menge B, Klemens O, Klemens JM, Saschenbrecker S, Jittmitrathap A, Leauangwuthong P, Steinhagen K. **Added value of testing for specific serum IgA additionally to IgM in acute secondary dengue virus infections.** 23rd Annual Meeting of the European Society for Clinical Virology (ESCV), virtueller Kongress (2021).
- Stiba K, Klemens O, Pollmann M, Klemens JM, Saschenbrecker S, Steinhagen K. **Development of a novel NS1-based ELISA for the detection of specific IgG antibodies against Japanese encephalitis virus.** 31st European Congress of Clinical Microbiology & Infectious Diseases (ECCMID), virtueller Kongress (2021).
- Van Beers J, Damoiseaux J, Jobsen M, Dähnrich C, Kühnl A, Schlumberger W. **Routine application of PR3- and MPO-ANCA chemiluminescence immunoassays demonstrates enhanced detection rates.** 15th Dresden Symposium on Autoantibodies, Dresden, Germany (2021).
- Venkataraman I, Pollmann M, Ott A, Liefeld M, Borchardt-Lohöfner V, Scheper T, Meyer W. **Novel line blot differentiates between IgG antibodies against three SARS-CoV-2 antigens and against further seasonal coronaviruses.** AACC Annual Scientific Meeting & Clinical Lab Expo, Atlanta, USA (2021).
- Villalta D, Alessio MG, Previtali G, Infantino M, Manfredi M, Agatea L, Favaro E, Kühnl A, Dähnrich C, Schlumberger W. **Novel chemiluminescence immunoassays for serological diagnosis of coeliac disease.** 15th Dresden Symposium on Autoantibodies, Dresden, Germany (2021).
- Vink C, van de Logt AE, Kühnl A, Dähnrich C, Schlumberger W, Wetzel J. **Relevance of anti-PLAZR levels in therapy decision and prediction of therapy outcome using cyclophosphamide and steroids treatment in patients with membranous nephropathy.** 15th Dresden Symposium on Autoantibodies, Dresden, Germany (2021).
- Weisser H, Steinhagen K, Höcker R, Borchardt-Lohöfner V, Anvari Ö, Kern PM. **Dried blood spots: a robust sample material for detection of anti-SARS-CoV-2 antibodies.** Valuable tool in the context of seroprevalence and vaccination studies. 31st European Congress of Clinical Microbiology & Infectious Diseases (ECCMID), virtueller Kongress (2021).
- Weisser H, Steinhagen K, Höcker R, Borchardt-Lohöfner V, Anvari Ö, Kern PM. **Dried blood spots are an alternative sampling material for detection of anti-SARS-CoV-2 antibodies.** 30th Annual Meeting of the Society for Virology (GV), virtueller Kongress (2021).
- Wolf J, Rockstroh A, Kalbitz S, Pollmann M, Rosenstock P, Steinhagen K, Borte S. **Correlation between binding and neutralising antibodies against SARS-CoV-2 with respect to the severity and phase of COVID-19.** 23rd Annual Meeting of the European Society for Clinical Virology (ESCV), virtueller Kongress (2021).
- Zeng Z, Miske R, Scharf M, Denno Y, Probst C, Teegen B, Ott A, Komorowski L. **Identification of NVL as a novel ANA target in systemic sclerosis.** 15th Dresden Symposium on Autoantibodies, Dresden, Germany (2021).



# Research and development

Scientific publications · Patents




For more information on this subject scan the QR code or enter the Quick Link code **q114** at [www.euroimmun.com](http://www.euroimmun.com)

## Patents

To ensure investments in research and development, EUROIMMUN again filed numerous patent applications for inventions by employees in 2021.

For patents from previous years, the patent protection was maintained and expanded through follow-up applications in the respective priority year. The applications concern developments in instrument and process engineering as well as new antigens for the diagnosis of autoimmune and infectious diseases. In addition, the trademark portfolio was supplemented by national and international trademark applications.





## Published Patent Applications 2021

1. Becker A, Schoch McGovern S. **Detection of an autoantibody**. European and US patent applications EP3786641 (filed in 2020) and US2021/0063393A1 (filed in 2020).
2. Bernitt E, Feirer C, Rateike M, Stöcker W, Schwab S. **Device and method for identification of cover glass areas of a slide**. European and International patent applications EP3839596 (filed in 2019) and WO2021/122888 (filed in 2020).
3. Dähnrich C, Konitzer S. **An improved autoantibody detection assay**. International patent application WO2021/023836 (filed in 2020).
4. Dettmann IM, Stegelmann C, Probst C, Radzimski C, Mindorf S. **Method for the detection of autoantibody to acetylcholine receptor**. European and Singaporean patent applications EP3842802 (filed in 2020) and 10202012737T (filed in 2020).
5. Filippis C, Steller U, Schilling F. **Method for qualitative evaluation of real-time PCR data**. European and international patent applications EP3839958 (filed in 2019) and WO2021/123171 (filed in 2020).
6. Hagen-Eggert M, Sumpf TJ. **Method and microscopy system for acquisition of a microscopic fluorescence image of a sample region with a biological sample**. Brazilian patent application BR102019026948-0 (filed 2019).
7. Harder M, Gräser Y, Kupsch C, Cavalari M. **Assay for the diagnosis of dermatophytosis**. Australian and US patent applications 2018202209 (filed 2018) and US2021/0254184A1 (filed 2021).
8. Krauth J, Krause C, Voigt J, Hahn M, Marzahl C, Gerlach S. **Detection of the presence of different antinuclear antibody fluorescence pattern types and device for same**. European, Chinese and US patent applications EP3767587 (filed in 2019), CN112240878A (filed in 2020) and US2021/0019883A1 (filed in 2020).
9. Marzahl C, Gerlach S, Voigt J, Kröger C. **Image processing method for displaying cells of multiple overall images**. European and US patent applications EP3876193 (filed in 2020) and US2021/0272279 (filed in 2021).
10. Miske R, Scharf M, Komorowski L, Denno Y, Hahn S, Radzimski C, Unger M, Mayo Clinic. **Diagnosis of neurological disease**. European and US patent applications EP3839511 (filed in 2020) and US2021/0181196A1 (filed in 2020).
11. Morgenroth K, Viertel V, Steller U, Gerlach S, Marzahl C, Voigt J, Stöcker W. **Method for automated detection of antibodies in a liquid biological sample using an antigen chip, and antigen chip therefore**. Chinese, Brazilian and US patent applications CN112334775A (filed in 2019), BR112020023867-8 (filed in 2019) and US2021/0245152A1 (filed in 2019).
12. Menge B, Steinhagen K, Schaefer J, Probst C, Deerberg A, Unger M, Messing C. **A novel assay for the diagnosis of nematode infections**. European, Chinese and US patent application EP3761029 (filed in 2020), CN112180096A (filed in 2020) and US2021/0003591A1 (filed in 2020).
13. Probst C, Mindorf S, Dettmann IM. **Improved detection of NMDA receptor autoantibodies**. International patent application WO2021/048263 (filed in 2020).
14. Rolf A, Stahl K, Hoxha E, Eisenmann J, Reinhard L. **A method and reagents for the diagnosis of MN**. International patent application WO2021/023816 (filed in 2020).
15. Steinhagen K, Deerberg A, Lattwein E, Radzimski C, Böthfür J. **An immunoassay for the diagnosis of viral infections**. US patent application US2021/0033609A1 (filed in 2017).
16. Steinhagen K, Messing C, Lattwein E, Stiba K, Lindhorst F, Neugebauer E, Charité - Universitätsmedizin Berlin. **Methods and reagents for diagnosis of SARS-CoV-2 infection**. European, Belgian, British, German, French, Italian, Dutch, Austrian, Polish, Swiss, Spanish, Czech patent applications 3809137 (filed 2021).
17. Steinhagen K, Messing C, Lattwein E, Stiba K, Lindhorst F, Neugebauer E, Müller M, Corman V. **Methods and reagents for diagnosis of SARS-CoV-2 infection**. European, German, Spanish, International, Chinese, Japanese, Canadian and US patent applications EP3869199 (filed in 2020), EP3869200 (filed in 2020), EP3809137A1 (filed in 2021), DE21158065T1 (filed in 2021), ES21158065T1 (filed in 2021), WO2021/165448A1 (filed in 2021), CN113557431A (filed in 2021), JP2021167805A (filed in 2021), CA3109607A1 (filed in 2021) and US2021/0190797A1 (filed in 2021).
18. Stöcker W, Komorowski L, Steinhagen K. **A method for determining the efficacy of a vaccine**. European patent application EP3855186 (filed in 2021).
19. Not yet known. **Assessing and treating autoimmune ataxia**. European patent application EP3819156 (filed in 2019).





# Detection methods





# Sample collection & Preanalytics

## Dried blood spots (DBS)








For more information on this subject scan the QR code or enter the Quick Link code **q172** at [www.euroimmun.com](http://www.euroimmun.com)

## Dried Blood Spots (DBS): Sample collection at home – analysis in the lab

Dried blood has been used as a sample material for *in vitro* diagnostic analysis since the mid 1960s, especially in newborn screening and, over the past decades, has become a standard in this field. Moreover, dried blood is applied in drug screenings, doping controls and in therapeutic drug monitoring. It is also more and more used in antibody and antigen diagnostics. Therefore, EUROIMMUN developed **the first CE-labelled blood collection set**. It contains all materials that are required for collection and sending of dried capillary blood samples. Patients can collect the sample themselves from their fingertip by using the set, or the collection can be performed by medical professionals. The dried capillary blood samples are an excellent alternative to venous blood samples and can be analysed subsequently in the lab, e.g. for antibodies against SARS-CoV-2.

- **Sample collection at home by the patient possible**, no medical staff required
- **Simple handling**: Capillary blood is collected by a prick in the finger, dropped onto the EUROIMMUN blood collection card and air-dried.
- **Minimally invasive method**, a simple alternative to venous blood sampling
- **Reduction / elimination of biological risks**: According to the US Department of Transportation (DOT), the International Air Transporter Association (IATA) and the World Health Organisation (WHO), dried blood spots are released medical specimens which do not require any special protective measures.
- **Samples can be shipped by post without any additional cooling**. **High stability** demonstrated for a large number of analytes
- **Quantification possible**, punches with a defined diameter allow exact determination of the collected blood volume
- **Complete automation of all process steps possible** (see page 60)
- **Application** of DBS samples **validated** in combination with the ELISAs for the detection of IgG antibodies against SARS-CoV-2 (see page 176)
- **Feasibility studies performed for the determination of a large number of analytes**, e.g. vitamin D, antibodies against CCP, gliadin, Borrelia, measles virus, mumps virus, Rubella virus, TBE virus and Zika virus, as well as all allergens of the Atopy screen test (allergy)





# Indirect immunofluorescence

EUROIMMUN IFT: unrivalled quality and diversity



For more information on this subject scan the QR code or enter the Quick Link code **q115** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROIMMUN IFT: unrivalled quality and diversity

**Immunofluorescence tests from EUROIMMUN: high-tech, not old-fashioned!** Numerous innovations contribute to the standardisation and modernisation of indirect immunofluorescence:


■ **Activation technique:** Physically or chemically activated cover glasses are coated with cultured cells or tissue sections. Frozen tissue sections are fixed to the glass surface by covalent bonding. This increases the adhesion by more than 100 fold, preventing detachment of the sections.

■ **BIOCHIP Technology:** Cover glasses coated with biological substrates are cut mechanically into millimetre-sized fragments (BIOCHIPS). Ten or more first-class preparations of consistent quality can be obtained per tissue section, for cultured cell substrates even several thousands.


■ **BIOCHIP Mosaics:** When multiple BIOCHIPS coated with different substrates are arranged in one reaction field, antibodies against various organs or infectious agents can be investigated simultaneously. Comprehensive antibody profiles can be easily established (multiplex) and the results are verified reciprocally on different substrates.

■ **TITERPLANE Technique:** The samples or reagents are first pipetted onto the reaction fields of a reagent tray. The slides are then placed into recesses of the reagent tray, where all BIOCHIPS come into contact with the liquids, and the individual reactions begin simultaneously. As the fluids are confined in a closed space, there is no need for a conventional humidity chamber.

■ **Automation:** EUROIMMUN offers a range of IFT automation options for both low and high throughput, from sample dilution to fully automated evaluation of fluorescence images, including archiving.

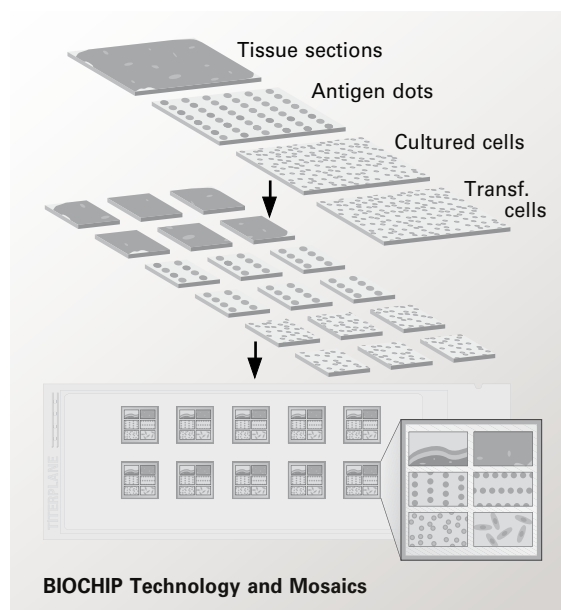





Indirect immunofluorescence: one substrate (here: HEP-2 cells) – many antibodies to investigate







# Microtiter ELISA

EUROIMMUN ELISA: quantitative and precise



For more information on this subject scan the QR code or enter the Quick Link code **q116** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROIMMUN ELISA: quantitative and precise

**When precision is needed:** Antibody detection using ELISA provides quantitative results – ideally suited for monitoring disease courses and interpreting borderline results.

- **Optimised for fully automated processing**
- **Simple handling:**
  - Break-off microplate wells
  - Ready-to-use reagents (no mixing or diluting necessary)
  - Bar- and colour-coded reagents, largely exchangeable between different lots and between different parameters
  - Standardised incubation conditions for the majority of parameters
- **RF absorbent** included in sample buffer (IgM tests) – no extra costs
- **Incubation protocols** for all tests integrated in EUROIMMUN Analyzers:  
no additional programming necessary
- **Comprehensive validation** of test systems for EUROIMMUN Analyzers
- **Detailed validation documents** available for virtually all parameters
- **Over 800 parameters** – all test systems from one manufacturer:
  - > 70 autoantibody parameters
  - > 120 infectious parameters
  - > 650 allergy parameters





# Chemiluminescence immunoassays (ChLIA)

EUROIMMUN ChLIA: Random access with chemiluminescence immunoassays



For more information on this subject scan the QR code or enter the Quick Link code **q116** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROIMMUN ChLIA: Random access with chemiluminescence immunoassays

Immunoassays for autoimmune, infection and allergy diagnostics and antigen detection

- **Bead technology:** Antigens are immobilised on the surface of magnetic particles. The detection of the immunological reaction between antigen and specific antibodies in patient serum is based on a chemical reaction which leads to a quantitative emission of light, the so-called chemiluminescence.
- **Fast analyses:** The ChLIA technology allows even shorter reaction times compared to immunoenzymatic methods, so that the total duration of the analysis amounts to less than 30 minutes.
- **Optimised for fully automated processing:** The patient samples can be processed fully automatically, from pipetting to result evaluation – also in connection with a sample line.
- **Simple and safe handling:** Ready-for-use reagent cartridges and calibrators and automated transmission of quality control data via RFID chips enable error-free and quick loading with little manual effort.
- **Efficient workflows:** Optimal processing on random access instruments, with continuous loading of samples and processing of emergency (STAT) samples. EUROIMMUN ChLIA tests enable quantification of test results based on a calibration curve which is stable over several weeks, so that capacities and reagents are saved.
- **Broad dynamic analysis range:** Owing to the high signal intensity at high sensitivity and specificity, the EUROIMMUN ChLIA tests allow quantification of antibodies from very low to very high concentrations based on the saved calibration curve.





# EUROASSAY

Line blots in chip format




For more information on this subject scan the QR code or enter the Quick Link code **q117** at [www.euroimmun.com](http://www.euroimmun.com)


## Line blots in chip format

**Easy handling** through incubation using the TITERPLANE Technique, **reliable and simple evaluation**:

- **Several patient samples** can be analysed next to each other and simultaneously **on one slide**.
- **Quick results**: The total time for analysis is 100 minutes. During washing the reagents are pipetted onto the reagent tray for the next incubation step. All incubation steps are carried out at room temperature. Shaking of the slides and reagent tray on a rotary shaker provides optimal sensitivity.
- **Low consumption of reagents**: 50 µl of diluted serum or reagent solution per application is sufficient.
- **At a glance**: Results are evaluated visually, thus there are no investment costs for photometers or similar devices. The antigen lines are located at precisely defined positions. Correct performance of the individual incubation steps is indicated by staining of the control band. Positive and negative results can be distinguished from each other reliably and easily. The intensity of bands generally correlates with the antibody titer.
- **Monospecific**: The antigens used are purified antigens which are mostly isolated by affinity chromatography. The membrane strips do not contain any superfluous proteins that might lead to unspecific positive results.
- **Archivable**: Incubated EUROASSAY slides can be stored for long periods, with easy documentation of results.











# EUROLINE

Line blots for comprehensive antibody profiles




For more information on this subject scan the QR code or enter the Quick Link code **q118** at [www.euroimmun.com](http://www.euroimmun.com)

## Multiparameter line blots for comprehensive antibody profiles

Uncomplicated test performance, reliable and simple evaluation:

- **Quick:** The total time for analysis is 105 minutes. All incubation steps are carried out at room temperature.
- **Automatable incubation:** with EUROBlotOne or EUROBlotMaster.
- **Secure:** The antigen lines are located at precisely defined positions. Correct performance of the individual incubation steps is indicated by staining of the control band contained on each EUROLINE test strip. Positive and negative results can be distinguished from each other reliably and easily. The intensity of bands correlates with the antibody titer.
- **Monospecific:** The antigens used are purified antigens, mostly isolated by affinity chromatography, or antigen extracts. The membrane strips do not contain superfluous proteins that may lead to unspecific positive results.
- **Multiparameter analysis:** The use of an antigen spectrum that is specifically tailored to the diagnostic requirements increases the serological detection rate.
- **Evaluation:** The EUROLineScan program developed by EUROIMMUN allows standardised evaluation of EUROLINE test strips, easy data management and detailed documentation of results. First, the incubated EUROLINE test strips are scanned by a flatbed scanner or photographed by a camera system. EUROLineScan recognises the position of the strips, even if they have been placed inexactly, identifies the bands, and measures their intensity. Finally, the results are saved together with the image data and a separate results sheet can be issued for each patient. EUROLineScan can be integrated easily into EUROLabOffice or any other LIMS for optimal data communication.





Detection  
methods



# Westernblot/EUROLINE-WB

Reliable differentiation with Westernblots





For more information on this subject scan the QR code or enter the Quick Link code **q119** at [www.euroimmun.com](http://www.euroimmun.com)

## Reliable differentiation with Westernblots

### High diagnostic value:

- **Quick:** Total time for analysis is around 115 minutes. All incubation steps are carried out at room temperature.
- **Automatable incubation:** with EUROBlotOne or EUROBlotMaster.
- **Precise evaluation:** The bands are identified by means of a lot-specific evaluation template provided with each test kit. Each electrophoresis gel has a unique lot number. Thus, mix-up between bands is prevented.
- **Secure:** Each test kit comes with a positive blot strip from the same strip lot, which has been incubated with a reference serum. The incubation of a positive control serum can thus be omitted. The blot strips are numbered to avoid mix-ups. No extra labelling is needed. Correct performance of the individual incubation steps is indicated by staining of a control band on the lower end of the strip.
- **Qualitative:** Positive und negative reactions can be distinguished from each other reliably and easily. The intensity of the bands generally correlates with the antibody titer.
- **Method of choice:** in cases in which positive results from a screening test (indirect immunofluorescence or microplate ELISA) need confirmation or differentiation.
- **EUROLINE-WB is a combination of Westernblot and line blot:** Proteins from a whole-antigen extract are separated by gel electrophoresis according to molecular mass and transferred onto a nitrocellulose membrane (Westernblot). Highly purified native or recombinant antigens are then applied as lines to the Westernblot strips (EUROLINE membrane chips).
- **Evaluation:** The EUROLineScan program developed by EUROIMMUN allows standardised evaluation of Westernblot-based test strips, easy data management and detailed documentation of results. First, the incubated Westernblot and EUROLINE-WB test strips are scanned by a flatbed scanner or photographed by a camera system. EUROLineScan recognises the position of the strips, even if they have been placed inexactly, identifies the bands, and measures their intensity. Finally, the results are saved together with the image data and a separate results sheet can be issued for each patient. EUROLineScan can be integrated easily in EUROLabOffice or any other LIMS for optimal data communication.

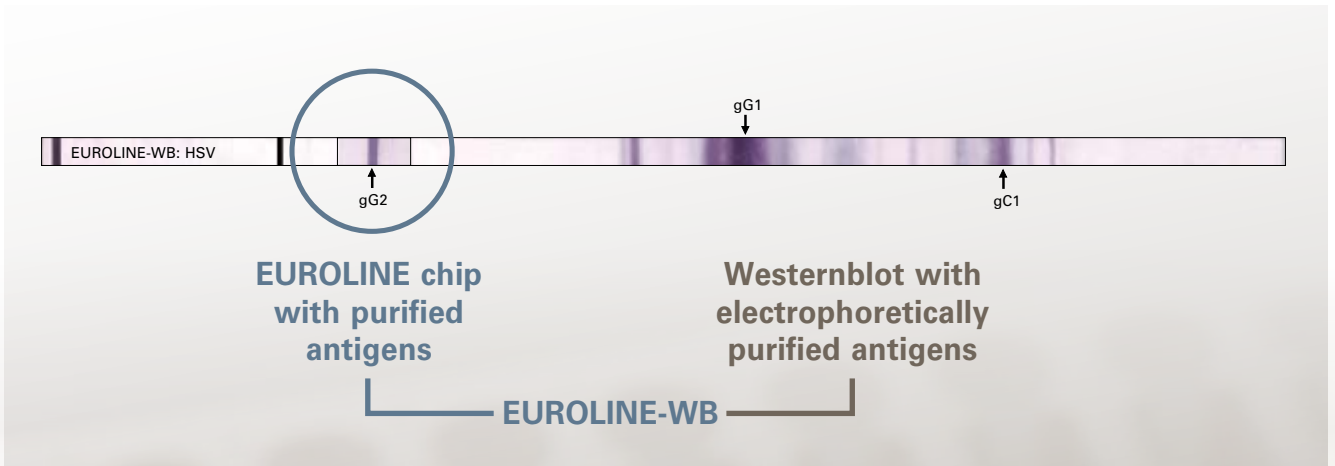



# EUROArray

Molecular diagnostics with EUROArrays




For more information on this subject scan the QR code or enter the Quick Link code **q120** at [www.euroimmun.com](http://www.euroimmun.com)

## Molecular genetic diagnostics with EUROArrays

Simple test performance, correct results:

- **EUROArrays are based on BIOCHIP technology:** Quality-controlled batch production of EUROArrays guarantees faultless arrays for exact and reliable diagnostics.
- **DNA isolation – quicker using the direct method:** Genomic DNA can be extracted with the direct method in a very time- and cost-saving manner. The sample is simply mixed with two extraction reagents provided in the test kit and can then be used directly in the PCR.
- **Ready-for-use PCR components:** All required reagents are contained in the test kit. No extra components must be purchased. The minimised number of pipetting steps allows quick, efficient and error-free test performance.
- **EUROArray hybridisation – simple and robust:** The established TITERPLANE Technique allows standardised and simple hybridisation of PCR products with the EUROArray.
- **Fully automated, standardised evaluation, generation of results and archiving:** Incubated EUROArrays can be automatically evaluated in a very short time using the EUROArrayScan evaluation system. Only around 5 seconds are required per sample. The evaluation is standardised and correct – results are not dependent on subjective interpretation.
- **Integrated controls ensure correct test performance:** Many integrated controls ensure the correct test performance for each individual analysis and help to monitor e.g. the sample quality, the rigour of the hybridisation reaction and the absence of cross contamination.
- **Complete process validated in accordance with IVD directive and CE label:** From sample preparation to issuing of results – DNA extraction, test reagents, EUROArrays, EUROArrayScan evaluation system – the complete process, including evaluation, is validated.
- **One platform for all applications:** Single-parameter, low-multiplex and high-multiplex analyses are reliable and precise with the EUROArray system.
- **LIMS connection available:** The EUROArrayScan software is equipped for simple import and export of data and test results.







# EURORealTime

EUROIMMUN's expert solution for real-time PCR diagnostics




For more information on this subject scan the QR code or enter the Quick Link code **q154** at [www.euroimmun.com](http://www.euroimmun.com)


## EUROIMMUN's expert solution for real-time PCR diagnostics

Simple performance and evaluation with highest result reliability


- **Fully automated, standardised evaluation, reporting and documentation:** The EURORealTime Analysis Software provides fast, fully automated and objective evaluation of all raw data, including all internal and external controls. Subjective definitions of cut-offs or calculations for the quantification of pathogens are not required.
- **Convenient guidance through the entire procedure:** Pipetting schemes which are automatically generated by the EURORealTime Analysis Software help to prevent mistakes.
- **Specific detection of infectious pathogens by Real-Time PCR:** Pathogen-specific primers and probes guarantee exact and reliable direct detection of infectious pathogens based on their gene sequence (DNA/RNA). In addition to the purely qualitative determination, also pathogen quantification in the raw material is possible in selected parameters.
- **Complete determination in one reaction vessel also for RNA viruses:** With viruses with RNA genome, the required reverse transcription and the real-time PCR detection take place in the same preparation.
- **Minimised number of pipetting steps owing to ready-for-use PCR components:** All required reagents are included, no extra components must be purchased.
- **Integrated controls ensure the reliability of the results:** Inhibition and extraction controls to check the efficiency of the nucleic acid isolation and PCR in every preparation and external positive and negative controls to confirm the validity of the entire run.
- **Complete procedure validated according to IVD directive, CE-labelled:** All steps of the procedure and evaluation are validated (test reagents, EURORealTime Analysis Software).
- **Prepared LIMS connectivity:** The EURORealTime Analysis Software is set up for simple import and export of data and test results.



RNA/DNA sample



Real-time PCR



Fully automated  
evaluation and  
documentation



## RIA

EUROIMMUN RIA: high-performance classic



For more information on this subject scan the QR code or enter the Quick Link code **q121** at [www.euroimmun.com](http://www.euroimmun.com)

# EUROIMMUN RIA: high-performance classic

Radioimmunoassays (RIA/IRMA) from EUROIMMUN are robust and reliable:

- **Fast, simplified test performance** with short incubation times, few wash steps and mostly ready-for-use reagents.
- **Highly specific** through use of optimal antigens and highly suited, established antibodies.
- **Secure quality management** through supplied controls (including kit-specific reference range) for evaluation of the test.
- **Large measurement ranges** with very good calibration reduces the need for repeat measurements with other sample dilutions and increases result retrieval.
- **Comprehensive range of separation methods:** coated tubes (CT), precipitation (P), magnetic separation (MS), polyethylene glycol precipitation (PEG).
- **Excellent correlation** with comparable test systems using the same analytical specifications.







# Automation





# Indirect immunofluorescence

MERGITE! · Sprinter · ELW IFA · UNIQO 160 · EUROStar · EUROPattern Microscope Live · EUROPattern



For more information on this subject scan the QR code or enter the Quick Link code **q144** at [www.euroimmun.com](http://www.euroimmun.com)

## MERGITE!

MERGITE! enables fully automated, standardised washing of IIFT slides. The compact table-top device utilises a directed but gentle liquid flow, which washes up to 50 substrate fields with consistent quality and without damage to the substrates. The use of carriers allows convenient switching between incubation and wash stations with just one hand maneuver and without the slides drying out. MERGITE! is equipped with an integrated touch screen and does not require an additional PC.

- **No risk of cross contamination** between substrate fields due to field-by-field washing with directed and controlled liquid flows



- **High reproducibility** due to the standardised, gentle MERGITE! washing procedure with defined wash programs

- **Easy and efficient handling** of slides, reagent racks and cover glasses through use of carriers

- **Reduction of required working steps** – no beakers, cuvettes and drying of slides required

- **Compact tabletop device** with integrated touch screen

- **Convenient operation** and minimal familiarisation time due to intuitive and user-friendly interface

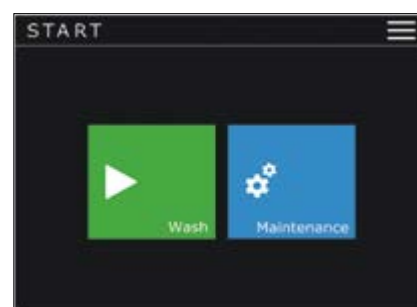



## Product overview

Device	Description	Order number
MERGITE! 10	For up to 5 slides each with 10 reaction fields	YG 0064-0101-1
MERGITE! 50	For 1 slide with 50 reaction fields	YG 0064-0101-2



# Indirect immunofluorescence

MERGITE! ·  · ELW IFA · UNIQO 160 · EUROStar · EUROPattern Microscope Live · EUROPattern



For more information on this subject scan the QR code or enter the Quick Link code **q040** at [www.euroimmun.com](http://www.euroimmun.com)

## Sprinter

With the IF Sprinter and the Sprinter XL, EUROIMMUN offers flexible solutions for fully automated processing of immunofluorescence tests. The devices perform identification, dilution and transfer of samples, as well as all washing and incubation steps.

Both instruments are available in different configurations depending on the requirements of the laboratory. They can also be used as combination devices for processing of ELISAs.

- **Flexible systems** for fully automated processing of ELISA and immunofluorescence tests on one device
- **Reliability and traceability** due to standard integrated barcode reader for sample identification and the fully automated identification of slides via matrix codes (optional)
- **Efficient pipetting without carryover** using one (IF Sprinter) or four (Sprinter XL) washable pipetting needles
- **Simplification of work processes** in routine laboratories due to user-friendly data communication with an LIS or EUROLabOffice 4.0
- **Variable instrument configuration** for different laboratory requirements with up to 96, 160 or 240 samples and up to 30 slides or six microplates (Sprinter XL), or 15 slides or two microplates (IF Sprinter) in one run







## Product overview

Device	Description	Order number
IF Sprinter IIFT	IIFT automation for up to 96 samples, up to 15 slides	YG 0032-0101
IF Sprinter IIFT/ELISA	IIFT/ELISA automation for up to 96 samples, up to 15 slides/2 microplates	YG 0032-0101-3
Sprinter XL 160 IIFT	IIFT automation for up to 160 samples, up to 30 slides, 4 washable needles	YG 0033-0101-5
Sprinter XL 160 IIFT/ELISA	IIFT/ELISA automation for up to 160 samples, up to 30 slides/6 microplates, 4 washable needles, with incubator	YG 0033-0101-3
Sprinter XL 240 IIFT	IIFT automation for up to 240 samples, up to 30 slides, 4 washable needles	YG 0033-0101-25
Sprinter XL 240 IIFT/ELISA	IIFT/ELISA automation for up to 240 samples, up to 30 slides/6 microplates, 4 washable needles, with incubator	YG 0033-0101-23



# Indirect immunofluorescence

MERGITE! · Sprinter · ELW IFA · UNIQO 160 · EUROStar · EUROPattern Microscope Live · EUROPattern




For more information on this subject scan the QR code or enter the Quick Link code **q151** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROLabWorkstation IFA

The EUROLabWorkstation IFA provides fully automated and standardised processing of EUROIMMUN immunofluorescence tests with the highest capacity and efficiency for laboratories with a high sample throughput. Up to 750 substrate fields and more than 700 samples can be analysed at high throughput with just one worklist. In the slide washing process, the established TITERPLANE Technique is complemented by the MERGITE! washing technology. This ensures brilliant fluorescence signals without background for the automatically mounted slides. The software can be operated conveniently and intuitively via touch screen and guides the user through the entire process. Complete traceability is guaranteed at all times, since the matrix codes of the slides and the barcodes of samples, reagents and accessories are automatically detected in each step of the process.

- **Fully automated processing** of EUROIMMUN immunofluorescence tests from primary sample to mounted slide
- **Highest capacity** of up to 750 substrate fields and more than 700 samples in a single worklist
- **Highest efficiency** due to 10 washable pipetting needles and complementary accessories, as well as separation of pipetting and transport steps for flexible time management
- **Flexible workflows** owing to freely selectable loading of the 45 tracks with samples, reagents and dilution plates
- **Brilliant fluorescence signals** with the unique MERGITE! washing technology – each substrate field is washed without the risk of cross contamination using directed liquid flow in a standardised and gentle procedure





## Product overview

Device	Description	Order number
EUROLabWorkstation IFA	Fully automated IIFT processing from primary sample to mounted slide for up to 750 substrate fields and more than 700 samples	YG 0852-0101



# Indirect immunofluorescence

MERGITE! · Sprinter · ELW IFA · UNIQO 160 · EUROStar · EUROPattern Microscope Live · EUROPattern



For more information on this subject scan the QR code or enter the Quick Link code **q175** at [www.euroimmun.com](http://www.euroimmun.com)

## UNIQO 160

The UNIQO 160 provides full IIFT automation of the next generation – from the primary sample to the microscopy result with only one instrument. This all-in-one solution maximises the efficiency of the entire IIFT process, encompassing sample preparation, incubation, washing and mounting of slides as well as image acquisition and analysis. Via the interface to the EUROLabOffice 4.0 middleware, the indirect immunofluorescence with the UNIQO 160 can integrate seamlessly into the efficient workflows of diagnostic laboratories.

Up to 160 primary samples and 18 slides can be processed in one run on the compact benchtop device. During loading, samples, reagents and slides are automatically identified and assigned by their barcodes. As the slides are protected from drying out by automated mounting after incubation, brilliant fluorescence images are produced from the first to the last sample, even with large worklists. The integrated high-quality microscope with automatically changing objectives (4x, 10x, 20x) ensures optimal recording parameters for each product. This enables reliable result and titer proposals from the automated evaluation based on artificial intelligence.

- **Fully automated processing system** from primary sample to evaluated fluorescence image for up to 160 samples and 18 slides
- **Flexible loading** as well as complete traceability of samples, reagents and slides through automated barcode registration
- **Brilliant fluorescence images** due to automatically mounted slides and the integrated high-quality microscope unit with automatically changing objectives (4x, 10x, 20x)
- **Automatically generated result proposals** based on state-of-the-art artificial intelligence methods and convenient evaluation in EUROLabOffice 4.0





## Product overview

Device	Description	Order number
UNIQO 160	Fully automated IIFT processing from primary sample to evaluated fluorescence image for up to 160 samples and 18 slides per run	YG 2900-0101





# Indirect immunofluorescence

MERGITE! · Sprinter · ELW IFA · UNIQO 160 · EUROStar · EUROPattern Microscope Live · EUROPattern




For more information on this subject scan the QR code or enter the Quick Link code **q025** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROStar III Plus

The LED fluorescence microscope EUROStar III Plus has been precisely tailored to the requirements of indirect immunofluorescence – superfluous, and in some cases expensive components have been intentionally dispensed with. A camera can be attached directly to the integrated photo tube for capturing digital images. Switching between the ocular and the camera is no longer necessary owing to the convenient 50/50 beam splitter. EUROIMMUN also offers the highly functional EUROPicture software for the displaying and handling of the digital images. The EUROStar III Plus includes a halogen lamp as standard equipment for normal transmitted light microscopy in bright and dark field and can be upgraded for phase contrast work.

- **Constant fluorescence excitation** due to regulated LED for reliable and reproducible results
- **Long life span** of over 50,000 hours, low current consumption and full light intensity immediately after being switched on
- **Environmentally friendly** without mercury
- **cLED available as separate module** for equipping various other microscopes
- **Screen diagnostics and digital image acquisition** using optional camera with EUROPicture software
- **50/50 beam splitter** for microscopy without switching between the oculars and the optional camera





## Product overview

Device	Description	Order number
EUROStar III Plus	Fluorescence LED microscope with constant, controlled light intensity, convenient 50/50 beam splitter, transmitted light microscopy, optional camera and image recording software EUROPicture, optional dark field and phase contrast	YG 0306-0101-3
EUROIMMUN cLED	Fluorescence LED light source with constant, controlled light intensity, suitable for most Zeiss microscopes with an HBO fixture	YG 0331-0101



# Indirect immunofluorescence

MERGITE! · Sprinter · ELW IFA · UNIQO 160 · EUROStar · EUROPattern Microscope Live · EUROPattern




For more information on this subject scan the QR code or enter the Quick Link code **q159** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROPattern Microscope Live

The EUROPattern Microscope Live is a fully automated immunofluorescence system which only needs two seconds to process an image. This enormous speed is supplemented by greatest convenience in the operation of EUROLabOffice 4.0 for the evaluation of immunofluorescence images directly at the computer screen. The intuitive touch screen user interface allows the user to directly zoom in on the image or to change the position during live microscopy. Moreover, it is possible for several users to view the images simultaneously at the screen – no discussion bridge is required. Up to 50 reaction fields are loaded into the microscope at once. Using the 20x objective, a high-resolution camera and high-quality optic components, a large number of substrates can be automatically viewed at the microscope, e.g. tissues, HEp-2 cells, Crithidia, granulocytes and antigen-expressing cells. Focusing is performed fully automatically by a new laser focusing technology. A self-regulating long-life LED as excitation source and the automated microscope calibration based on an integrated fluorescence standard ensure consistent immunofluorescence signal intensity.

- **Fully automated image recording and advanced on-screen reporting** – no darkroom required
- **Ultra-fast processing in only 2 seconds per image**
- **Convenient control of the EUROPattern Microscope Live as well as efficient input of results** directly in EURO-LabOffice 4.0
- **Automated result proposals** based on state-of-the-art artificial intelligence methods
- **Easy live microscopy** with on-screen multi-touch navigation and zooming
- **Reliability and traceability** owing to automatic identification of slides via matrix codes





## Product overview

Device / software	Description	Order number
EUROPattern Microscope Live	Fast, automated live microscopy with LIS connection and convenient result input	YG 0371-0101



# Indirect immunofluorescence

MERGITE! · Sprinter · ELW IFA · UNIQO 160 · EUROStar · EUROPattern Microscope Live · EUROPattern




For more information on this subject scan the QR code or enter the Quick Link code **q023** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROPattern

The EUROPattern Suite automates immunofluorescence microscopy (slide transport, image recording and archiving and interpretation of immunofluorescence images), providing support and improvement in diagnostic result reporting. As a module of the laboratory management software EUROLabOffice 4.0, EUROPattern can be flexibly integrated into any laboratory environment. The high speed of the system and the minimisation of manual handling enable EUROPattern to be employed for standardised IIFT diagnostics even at the highest of throughput requirements. The EUROPattern Suite consists of a fully automated microscope with a slide magazine (500 reaction fields per loading) together with a sophisticated pattern recognition software, which not only provides classification in terms of “positive” and “negative” for a large variety of substrates, but also reliably recognises the different ANA and ANCA patterns.

- **Automated microscopy and advanced on-screen reporting** for a multitude of EUROIMMUN IIFT products – no darkroom required
- **Automatically generated result proposals** based on state-of-the-art artificial methods for or ANA (including mixed patterns), ANCA, tissues, *Crithidia* and antigen-expressing cells
- **Long walk-away time** due to high loading capacity and automated processing of up to 500 reaction fields in one run
- **High-throughput immunofluorescence microscopy** – over 250 fluorescence images can be recorded and automatically evaluated in just one hour
- **Reliability and traceability** due to automatic identification of slides via matrix codes







## Product overview

Device / software	Description	Order number
EUROPattern	Complete system for computer-aided immunofluorescence microscopy (CAIFM); fast automated microscopy, image acquisition and pattern recognition incl. mixed patterns and corresponding titers	YG 0075-0101-1



# Microtiter ELISA

EUROIMMUN Analyzer · EUROLabWorkstation ELISA · Dried Blood Spots (DBS)



For more information on this subject scan the QR code or enter the Quick Link code **q017** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROIMMUN Analyzer

The EUROIMMUN Analyzer I and EUROIMMUN Analyzer I-2P are systems for fully automated ELISA processing and ensure an optimal routine operation. The combination of EUROIMMUN ELISAs and the EUROIMMUN Analyzer I or I-2P enables a quick and simple, but also secure start of the worklist, owing to the automatic recognition and assignment of reagents. The EUROIMMUN Analyzer I-2P is designed for small to medium sample throughput and the EUROIMMUN Analyzer I for medium to high sample throughput.

- **Fully automated ELISA processing** for various sample volumes with minimal hands-on time
- **Flexible open system** also for ELISA kits from different manufacturers
- **High reliability and traceability** due to automatic identification of barcodes of patient samples and ready-to-use reagents
- **Fast processing** on the EUROIMMUN Analyzer I of up to 70 tests per hour (up to 7 plates and 180 samples per run) and on the EUROIMMUN Analyzer I-2P of up to 50 tests per hour (up to 3 plates and 144 samples per run) possible
- **Convenient operation** of the software, including scanning of QC certificates using a 2D-hand barcode scanner





## Product overview

Device	Description	Order number
EUROIMMUN Analyzer I-2P	Fully automated ELISA processing for up to 3 microplates	YG 0015-0101
EUROIMMUN Analyzer I	Fully automated ELISA processing for up to 7 microplates	YG 0014-0101



# Microtiter ELISA

EUROIMMUN Analyzer · EUROLabWorkstation ELISA · Dried Blood Spots (DBS)



For more information on this subject scan the QR code or enter the Quick Link code **q141** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROLabWorkstation ELISA

The EUROLabWorkstation ELISA is a fully automated complete solution for processing ELISA kits in laboratories with high sample throughput. The system was developed by EUROIMMUN with a focus on efficiency and flexibility, in order to accommodate the ever increasing sample numbers and changing dynamics in the routine laboratory.

Ten washable needles and complementary consumables as well as a separate robotic arm for handling of the ELISA plates enable unparalleled sample throughput. The state-of-the-art, intuitive software guides the user graphically through all work steps.

- **Fully automated processing of ELISA** from primary sample to result
- **Highest capacity** of up to 15 ELISA plates and more than 700 samples in a single worklist
- **High throughput** of more than 200 tests per hour possible
- **Flexible open system** also for ELISA kits from different manufacturers
- **Minimal hands-on time and complete traceability of results** due to recognition of barcodes and matrix codes of samples, reagents, consumables and ELISA plates





## Product overview

Device	Description	Order number
EUROLabWorkstation ELISA	Fully automated high-throughput ELISA processing (over 700 samples and 15 ELISA plates possible)	YG 0851-0101



# Microtiter ELISA

EUROIMMUN Analyzer · EUROLabWorkstation ELISA · Dried Blood Spots (DBS)





For more information on this subject scan the QR code or enter the Quick Link code **q171** at [www.euroimmun.com](http://www.euroimmun.com)

## Dried Blood Spots (DBS)


EUROIMMUN's product portfolio in combination with Revvity instruments enables fully automated processing of serological tests based on dried blood spots (DBS) as sample material. Capillary blood, collected from the fingertip, is applied onto barcoded blood collection cards which allow complete traceability of the sample over the entire process. There are various automation solutions available, both for punching out the DBS (e.g. Revvity DBS Puncher® or Panthera-Puncher™ 9) and automated test processing, which are suitable for every laboratory size and sample throughput.

The analysis of DBS extracts with EUROIMMUN ELISAs can be performed conveniently and safely using, for instance, the EUROLabWorkstation ELISA, the EUROIMMUN Analyzer I or I-2P or the Sprinter XL, thanks to optimised workflows and consumables. For automated processing of immunoblot strips, the EUROBlotMaster and EUROBlotOne instruments are available. The communication with the LIS is established either directly via the respective instrument software, or conveniently via the EUROLabOffice middleware, which allows optimal channelling and display of all information.

- **Complete traceability** from the sample card to the final result
- **Flexible and scalable automation solutions** for all laboratory sizes and sample throughputs
- **Clear result overview** including documentation and archiving of all relevant patient information by the optional middleware EUROLabOffice 4.0

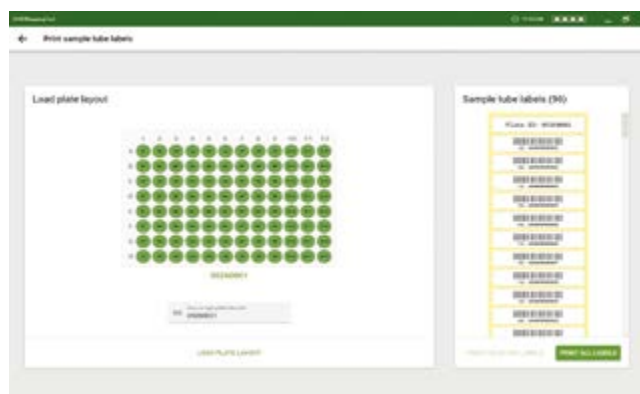



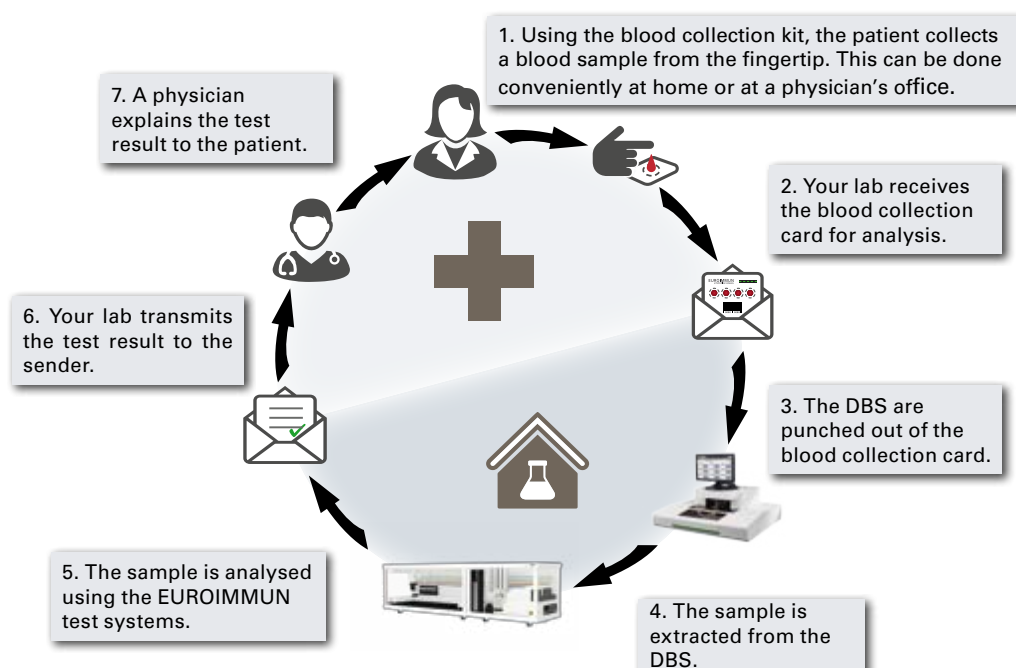

## Product overview

Device	Description	Order number
EUROLabWorkstation ELISA	Fully automated high-throughput ELISA (more than 700 samples and up to 15 ELISA plates possible)	YG 0851-0101
EUROMappingTool	Translation of plate barcodes into sample tube barcodes	YG 9730-0101
EUROIMMUN Analyzer I-2P	Fully automated ELISA processing for up to three microplates	YG 0015-0101
EUROIMMUN Analyzer I	Fully automated ELISA processing for up to seven microplates	YG 0014-0101
Sprinter XL 160 IIFT/ELISA Sprinter XL 240 IIFT/ELISA	IIFT/ELISA automation for up to 160/240 samples, up to 30 slides/six microplates, four washable needles, with incubator	YG 0033-0101-3 YG 0033-0101-23
EUROBlotMaster EUROBlotMaster 44	Blot processor for up to 30/44 EUROIMMUN blot strips	YG 0151-0101 YG 0151-0101-1
EUROBlotOne	Fully automated blot processing, up to 44 samples or strips for autoimmune, infection and allergy parameters	YG 0153-0101



# Chemiluminescence

IDS-i10 and IDS-iSYS



For more information on this subject scan the QR code or enter the Quick Link code **q152** at [www.euroimmun.com](http://www.euroimmun.com)

## IDS-i10 and IDS-iSYS

The random access instruments IDS-i10 and IDS-iSYS are compact solutions for automated processing of chemiluminescence immunoassays (ChLIA) for autoimmune, allergy and infection diagnostics as well as antigen detection. The possibility of loading the samples continuously – with the IDS-i10 also via connection to a lab track system – means that each patient sample can be processed as a single determination with minimal effort and short reaction times. In addition, the preferred processing of emergency (STAT) samples gives laboratories with different requirements and sample volumes unparalleled flexibility in their laboratory routine.

- **Random access instruments** for batch, continuous and STAT loading
- **Minimal calibration effort** owing to stored master curves
- **Connection to a laboratory track system** possible for the IDS-i10
- **Autoimmune, allergy and infection parameters as well as antigen detection** on one instrument
- **Short reaction times** for fast and reliable results in just 25 minutes (depending on the test)
- **High throughput** of up to 120 samples per hour
- **Convenient and reliable operation** due to barcode recognition of samples and test and lot-specific information including stored standard curve





## Product overview

Device	Description	Order number
IDS-i10	Random access instrument for chemiluminescence immunoassays (ChLIA) for the analysis of up to 60 samples and 10 parameters	IS-810400
IDS-iSYS	Random access instrument for chemiluminescence immunoassays (ChLIA) for the analysis of up to 120 samples and 15 parameters	IS-310400



# Immunoblots

EUROBlotMaster · EUROLineScan · EUROBlotOne · Microwell Imager




For more information on this subject scan the QR code or enter the Quick Link code **q015** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROBlotMaster

The EUROBlotMaster and the EUROBlotMaster 44 are compact benchtop devices for processing EUROIMMUN blot strips (EUROLINE, EUROLINE-WB, Westernblot). Following the software-guided loading of reagents, blot strips and samples, the devices perform all incubation and wash steps of the work protocol, as well as the dispensing of buffers, conjugates and substrate and stop solutions. Different conjugates and tests for autoimmune, infection and allergy diagnostics can be combined in one run. EUROBlotMaster devices have an integrated display with a membrane keyboard and do not require an additional PC. They are convenient and simple to operate using six keys and require minimal daily maintenance of five minutes at most.

- **Flexible automation for all EUROIMMUN blot strips** (EUROLINE, EUROLINE-WB, Westernblot)
- **Standardised processing** for better precision and reproducibility
- **Combination** of autoimmune, infection and allergy diagnostics on one device
- **Two models available:** up to 30 or up to 44 strips per run
- **Easy operation** using menu navigation on the integrated display
- **Combination** of different conjugates/tests in one run
- **Compact benchtop device** with low space requirement






## Product overview

Device	Description	Order number
EUROBlotMaster	Blot processor for up to 30 EUROIMMUN blot strips	YG 0151-0101
EUROBlotMaster 44	Blot processor for up to 44 EUROIMMUN blot strips	YG 0151-0101-1





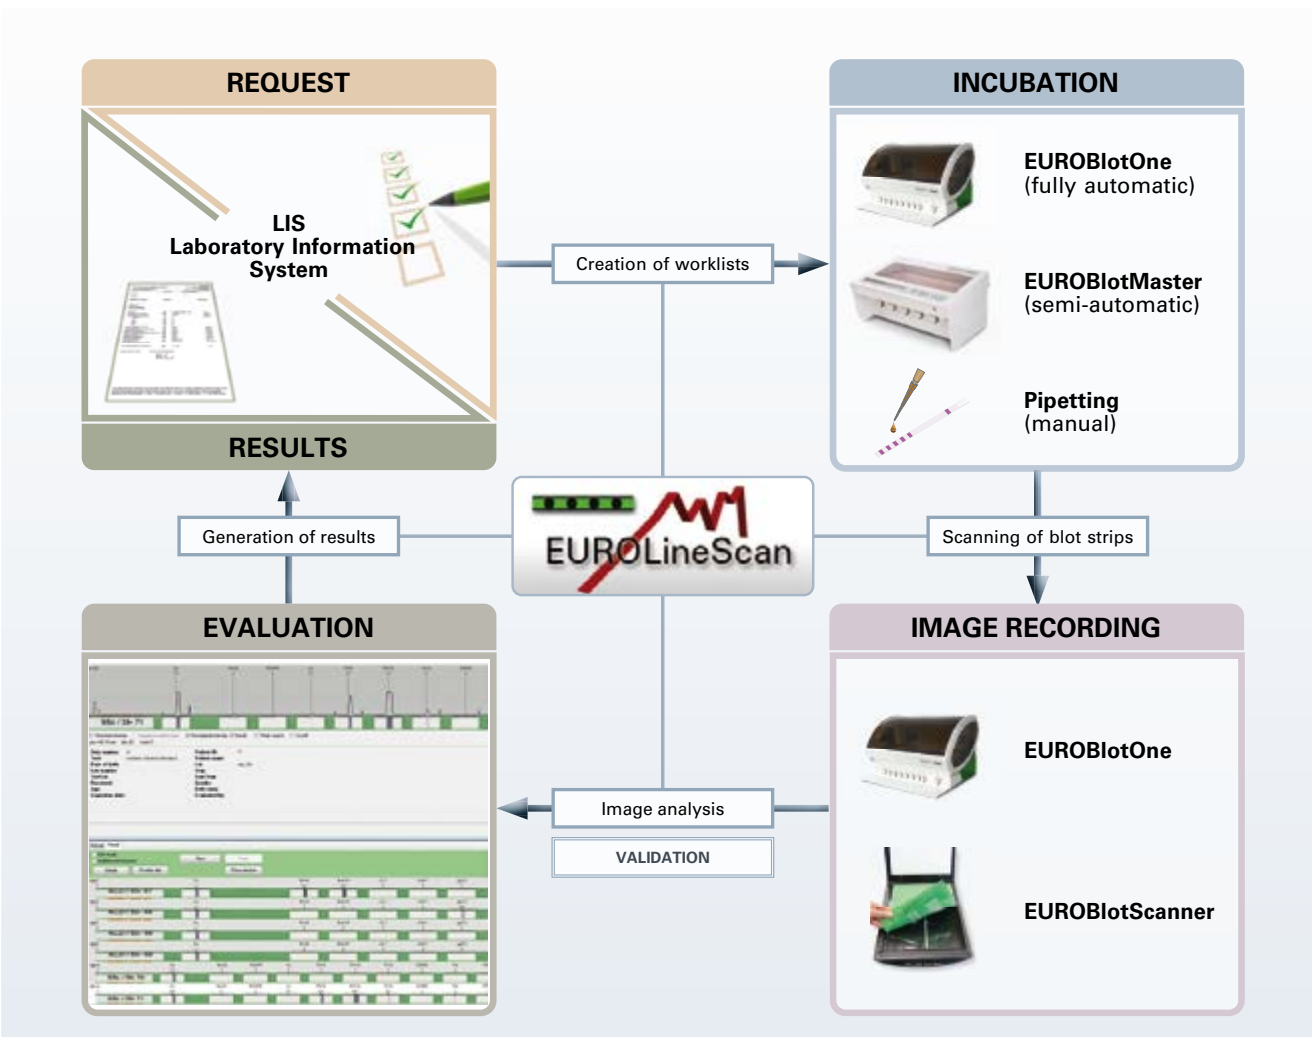

Automation

## Product overview

Device / software	Description	Order number
EUROLineScan	Fully automated identification, quantification, evaluation and archiving of incubated blot strips, support for protocol generation	YG 0006-0101
EUROBlotScanner	Fast digitisation using flatbed scanner	YG 0102-0101



# Immunoblots

EUROBlotMaster · EUROLineScan · EUROBlotOne · Microwell Imager





For more information on this subject scan the QR code or enter the Quick Link code **q016** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROBlotOne

The EUROBlotOne is a compact benchtop device for complete processing of immunoblots. Following the fast and convenient software-guided loading, the system performs the identification and dilution of samples as well as all incubation and wash steps. Eight reagent channels allow the combination of tests from autoimmune and infection diagnostics in one run. The incubated strips are then automatically dried, photographed and evaluated using the EUROLineScan software. The test requests and results can be communicated bidirectionally via LIS or EUROLabOffice 4.0.

- **Fully automated system** for the processing of up to 44 immunoblots in one run – from sample identification to the final result
- **Integrated drying unit** for fast evaluation of strips and high reproducibility of results
- **Highest security** through automatic barcode identification of samples
- **Flexible combination** of autoimmune and infection parameters in one run and autoimmune, infection and allergy diagnostics on one device
- **Intuitive software** for secure and convenient operation
- **Reliable automated evaluation** of blot strips with the EUROLineScan software





## Product overview

Device	Description	Order number
EUROBlotOne	Fully automated blot processing, up to 44 samples or strips for autoimmune, infection and allergy parameters	YG 0153-0101



# Immunoblots

EUROBlotMaster · EUROLineScan · EUROBlotOne · Microwell Imager



For more information on this subject scan the QR code or enter the Quick Link code **q177** at [www.euroimmun.com](http://www.euroimmun.com)

## Microwell Imager

The Microwell Imager is a compact benchtop device for automated image recording in EUROMicroblot analyses. As part of the workflow, the Microwell Imager provides acquisition of images of the wells. The EUROMicroblots, miniaturised immunoblots in microplate format, combine the advantages of blot and ELISA technologies in one product and are processed in exactly the same way as classical ELISAs. In fully automated high-throughput diagnostics, depending on the parameter tested, both screening by ELISA and confirmation by EUROMicroblot can be carried out with just one automated incubation system.

The EUROMicroblots are incubated with the patient samples using an ELISA processor, for example the EUROLab-Workstation ELISA or the EUROIMMUN Analyzer I or I-2P, depending on the sample throughput. The microplates with the incubated EUROMicroblots are then placed in the Microwell Imager. The automated recognition of microplate barcodes ensures correct assignment of results. In the subsequent image recording, the integrated camera of the Microwell Imager delivers high-quality images of each individual EUROMicroblot well in the shortest possible time. The intuitive EUROLineScan software then automatically evaluates these images and generates a result proposal.

- **Automated reading and evaluation** due to the combination of Microwell Imager and EUROLineScan
- **Compact benchtop device** for easy integration into any laboratory
- **Suitable combination** with the established automated ELISA systems EUROIMMUN Analyzer I or I-2P or EUROLabWorkstation ELISA
- **Traceability and reliable assignment** of results throughout the entire process due to harmonised products





## Product overview

Device	Description	Order number
Microwell Imager	Digitisation and evaluation of EUROMicroblots in 96-well format	YG 0191-0101



# DNA/RNA extraction and processing

Automation

Pre-NAT II



For more information on this subject scan the QR code or enter the Quick Link code **q166** at [www.euroimmun.com](http://www.euroimmun.com)

## Pre-NAT II

The Pre-NAT II allows fully automated high-throughput sample preparation for molecular genetic diagnostics, consisting of nucleic acid extraction and subsequent pipetting of the PCRs. In this way, up to 96 primary samples from various source materials are prepared efficiently, safely and without any manual intermediate steps for subsequent PCR-based tests.

After automated barcode identification of the sample tubes, the cell material is lysed and the nucleic acids are extracted by means of magnetic particles. These are subsequently transferred one after another into the automatically dispensed reagents by magnetisable metal rods. Afterwards, the liquid-handling module of the Pre-NAT II automatically pipettes the prompted PCRs using the extracted nucleic acids and the PCR reagents, which are stored refrigerated in the instrument.

- **Fully automated instrument for nucleic acid extraction and PCR preparation** for up to 96 primary samples and up to 288 PCRs per run
- **Further applications of the PCRs possible** for a variety of diagnostic analyses
- **Established nucleic acid extraction system** based on magnetic particles
- **Precise pipetting** with disposable filter tips, as well as an efficient and resource-saving dispensing system for extraction reagents
- **User-friendly instrument software** with clear graphic visualisation of all process and run times







## Product overview

Device	Description	Order number
Pre-NAT II	Fully automated instrument for nucleic acid extraction and preparation of PCRs for up to 96 samples	YG 9102-0101



# EUROArray

EUROArrayProcessor · EUROArrayScanner




For more information on this subject scan the QR code or enter the Quick Link code **q173** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROArrayProcessor

The EUROArrayProcessor enables automated processing of EUROArray slides. In the pre-PCR area, the software automatically generates a worklist based on the registered primary samples and the requested analyses and supports the user in the manual preparation of PCRs by providing information on the pipetting layout and the required reagent and sample volumes. Alternatively, for a higher degree of automation, the Pre-NAT II can be included in the workflow for automated preparation of the PCRs. In this case, run information and PCR layout are transferred from the Pre-NAT II to the EUROArrayProcessor. In the post-PCR area, the EUROArrayProcessor provides dilution of the PCRs with hybridisation buffer, the transfer of the hybridisation preparations to reagent trays and the incubation, washing and drying of the EUROArray slides. These can then be read out with the EUROArrayScanner. The integrity of the data is ensured by digital transmission between LIS, Pre-NAT II, EUROArrayProcessor and EUROArrayScan software throughout the entire process.

- **Automated post-PCR processing** of up to 192 PCR preparations and 40 EUROArray slides per run using proven TITERPLANE technology
- **Standardised and reproducible washing** of EUROArray slides based on MERGITE! washing technology and automated drying for best quality of results
- **Safety and traceability** through barcode identification of EUROArray slides, reagent tray boxes and reagents
- **Interfaces to Pre-NAT II and EUROArrayScan software** for secure data transfer throughout the process





## Product overview

Device / software	Description	Order number
EUROArrayProcessor	Automated processing of EUROArray slides: pipetting, hybridisation, washing and drying on one instrument	YG 0671-0101-1



# EUROArray

EUROArrayProcessor · EUROArrayScanner



For more information on this subject scan the QR code or enter the Quick Link code **q014** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROArrayScanner

After hybridisation, the EUROArrays are read by the EUROArrayScanner. The EUROArrayScan software automatically recognises the position of the arrays and quantifies the spot signals for each DNA probe. In just a few seconds, the software calculates the test results from the signal intensity for all samples and documents the findings. The extensive, integrated controls are automatically taken into account in the process. Manual evaluation and interpretation of the signals is not necessary. The EUROArrayScan software generates a clearly laid out work protocol for every run, which helps to make processing of the samples simple and secure.

With the report output, the user has the possibility to obtain an overview of the results for all samples and/or a detailed individual report with all partial results together with the associated array image in order to verify the suggested findings. Furthermore, the user can add individual comments. The results are automatically saved together with the image data, therefore archiving of the incubated EUROArray slides can be dispensed with. It is possible to connect the EUROArrayScan software to an LIS.

■ **Analysis and evaluation system** for molecular genetic diagnostics by means of EUROArrays

■ **Fully automatic digital evaluation, result output and data archiving**

■ **Rapid evaluation** – one EUROArray slide for five samples in under 20 seconds

■ **Result output** in the form of an overview or a detailed individual result

■ **Possibility to add comments to the result**

■ **LIS connection and networkability** for optimal data communication and integration

Patienten ID: 0      Test: HLA-DQ2/DQ8  
 Ergebnis vom: 09.07.2013      Protokoll: 130529DH\_20\_Demo07  
 Charge: 521003AS      Druckdatum: 20.08.2013 10:18:01  
 Patientenname: 0

**EUROIMMUN** Medizinische Labordiagnostik AG      Automatische Auswertung mit der EUROArrayScan-Software


Teilergebnis	Ergebnis
Kontroll-Kontrollsubstanzkontrolle	positiv
Hybridisierungs-/Spezifikationskontrolle	positiv
Profilkontrolle I	positiv
Profilkontrolle II	positiv
Analysel HLA-DQ2 2	negativ
Analysel HLA-DQ2 5	negativ
Analysel HLA-DQ8	negativ
Substanz HLA-DQ2 2/DQ2 5	positiv
Substanz HLA-DQ8	negativ

**Testergebnis**

HLA-DQ2	Ergebnis
HLA-DQ2 I	negativ
HLA-DQ2 II	negativ

\*In den europäischen Leitlinien zur Zöliakie-Diagnostik wird ausschließlich der Subtyp HLA-DQ2.5 als HLA-DQ2-assoziiert aufgeführt (Husby et al., J. Pediatr. Gastroenterol. Nutr. 2012;Jan;54(1):136-42). Andere Studien zeigen, dass mit HLA-DQ2 2 ein untypischer Subtyp ebenfalls mit der Zöliakie assoziiert sein kann, wenn auch verbunden mit einem niedrigeren Verdacht der Erkrankung (Matsuda et al., J. Pediatr. Gastroenterol. Nutr. 2013;Oct 16; [Epub ahead of print] - Stand 11. März 2013)

Unterschrift: \_\_\_\_\_



## Product overview

Device / software	Description	Order number
EUROArrayScanner	EUROArrayScanner incl. EUROArrayScan software for fully automated recording, evaluation, interpretation of findings and archiving of EUROArrays	YG 0602-0101



# EURORealTime

Eonis™ Q96 · EURORealTime-Analysis



For more information on this subject scan the QR code or enter the Quick Link code **q176** at [www.euroimmun.com](http://www.euroimmun.com)

## Eonis™ Q96

The Eonis™ Q96 is a quantitative real-time PCR thermal cycler for analyses in 96-well format with accurate real-time results.

The 96-well PCR plate with a sample volume between 5 and 100 µL can be conveniently inserted into the easily accessible sample drawer. The heating block made of silver with gold coating ensures fast heating and cooling cycles as well as highest temperature homogeneity over all 96 wells due to its thermal conductivity properties. The motorised heated lid with precise contact pressure prevents condensation, thus avoiding losses of sample volume. The fibre-optic system with 4 long-life LEDs and the high-performance optics enable homogeneous excitation of the fluorescent dyes in all individual samples for the best possible quantum yield. The signals are received by the detection module with 6 different colour filter modules, so that multiplex PCRs with different probes can be analysed with the Eonis™ Q96.

The Eonis™ Q96 is operated with an intuitive control software that can also be connected to the EURORealTime Analysis software for secure and convenient evaluation.

- **Convenient insertion and removal** of the 96-well PCR plate due to the freely accessible sample drawer
- **Fast heating and cooling cycles** and **ideal temperature homogeneity** over the entire heating block
- **Homogeneous excitation** without edge effects and readout of 96 samples in only 6 seconds
- **Bidirectional connection to EURORealTime Analysis software** for secure data transfer





## Product overview

Device / software	Description	Order number
Eonis™ Q96	Quantitative real-time PCR cyclers	YG 1092-0101



# EURORealTime

Eonis™ Q96 · EURORealTime-Analysis



For more information on this subject scan the QR code or enter the Quick Link code **q153** at [www.euroimmun.com](http://www.euroimmun.com)

## EURORealTime Analysis

The EURORealTime Analysis software provides guided preparation and fully automated evaluation of EURORealTime tests. It automatically calculates pipetting schemes and master mix preparations to support the subsequent pipetting of PCRs and performs standardised evaluation of raw data for selected PCR cyclers, including generation of result suggestions. All internal and external controls are automatically taken into account. Manual definition of cut-offs and subjective interpretation of results are no longer required. Moreover, the software provides the possibility of printing an overview of all test results, optionally including the respective amplification curves.

An interface enables digital data transfer between the EURORealTime Analysis software and the Pre-NAT II, as well as a laboratory information system (LIS) for a convenient and secure workflow.

- Software-supported preparation and automated evaluation of EURORealTime tests
- Generation of pipetting schemes and PCR layouts, including all required controls
- Result documentation and issuing of result suggestions for patient samples as well as all internal and external controls
- Economical **reusability of standard curves** for quantification
- **Result output** in a clearly arranged list of individual results, optionally including amplification curves
- Digital data communication possible between EURORealTime Analysis software, Pre-NAT II and LIS


EUROIMMUN Worldwide Laboratory 45 Speziallabor Densow  
Werkstraße 2-22 Densow

**EURORealTime Resultist**

Protocol: Zika\_example  
print date: 13.09.2017 14:27:07

Local Device ID: LC\_Da\_EVA 121272  
Performed tests: • Zika virus (LOT: 1170120AE) EUROIMMUN

Test:	Zika virus					
Sample ID (Laboratory ID)	Param.	Result	Cp	Copies/ml Sample	Comment	
NC	Zika	valid				
	IC	valid	31.01			
PC	Zika	valid	31.59			
	IC	valid	30.96			
170413001 36	Zika	detected	33.98			
	IC	valid	31.14			
170413001 35	Zika	detected	34.16			
	IC	valid	31.03			
170413001 34	Zika	detected	33.68			
	IC	valid	31.35			







# Laboratory management

EUROLabOffice 4.0 · EUROLab CSF software



For more information on this subject scan the QR code or enter the Quick Link code **q021** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROLabOffice 4.0

The laboratory management system EUROLabOffice 4.0 simplifies and speeds up the daily routine in the diagnostic laboratory and increases security through organisation of the entire laboratory procedure and traceable documentation of all data and processes. EUROLabOffice 4.0 offers many advantages both for small laboratories with mainly manual workstations as well as for high-throughput laboratories with a variety of connected automated systems and workstations.

- **Efficient consolidation of laboratory results** obtained with EUROIMMUN products for autoimmune, infection and allergy diagnostics as well as antigen detection
- **Central interface** between all EUROIMMUN instruments and the LIS for maximal automation and minimisation of manual working steps
- **Increase in the efficiency and reproducibility of all working steps:** Completely paperless work procedures in accordance with automated protocols – from easy management of analysis requests, (cost-) optimised test performance, IIFT result input at the computer screen, archiving of IIFT and blot images
- **Security and comprehensive data processing** via automated and complete data communication between the LIS and all workstations
- **Flexible and open system** for individual adaptation to existing laboratory processes due to various setting options and expansion modules





## Product overview

Software	Description	Order number
EUROLabOffice 4.0	Laboratory management software of the latest generation for optimisation of workflows in the diagnostic laboratory	YG 0250-0101-7
Module Quality Control Management, EUROLabOffice 4.0	Optional module for automated lot management and quality management evaluation of controls	YG 0250-0101-70
Module Sample Archive, EUROLabOffice 4.0	Optional module for efficient sample archiving	YG 0250-0101-71
Module Manual Sample Registration, EUROLabOffice 4.0	Optional module for convenient manual sample registration and assignment to different workstations	YG 0250-0101-72



# Laboratory management

EUROLabOffice 4.0 · EUROLab CSF software



For more information on this subject scan the QR code or enter the Quick Link code **q128** at [www.euroimmun.com](http://www.euroimmun.com)

## EUROIMMUN CSF Software

The EUROIMMUN CSF Software provides automated calculation of CSF/serum quotients ( $CSQ_{alb.}$ ,  $CSQ_{total}$  IgA/G/M,  $CSQ_{path.-spec.}$ ,  $CSQ_{lim.}$  and  $CSQ_{rel.}$  or antibody index AI). The  $CSQ_{rel.}$  allows a statement to be made on the intrathecal pathogen-specific antibody synthesis.

The albumin and antibody concentrations measured by means of e.g. a nephelometer and the EUROIMMUN Analyzer or the EUROLabWorkstation ELISA can be transferred online into the EUROIMMUN CSF Software so that time-consuming and error-prone manual data transfer is no longer required. Manual input of the values or quotients into the software is also possible. For manual transfer a photometer can be connected.

Optionally, a storable standard curve can be used so that only one recalibrator needs to be included instead of 4 to 6 calibrators per run. This saves reaction wells on the ELISA plate. The recalibration, validity check and calculation of the antibody concentration are fully automated in the EUROIMMUN CSF Software. For internal quality control, the values of the recalibrator or the serum/CSF controls from different runs for one lot are clearly presented.



In the detailed patient view, all findings and a suggested final result are shown. The CSF/serum quotients  $CSQ_{alb.}$  and  $CSQ_{total}$  IgA/G/M are additionally displayed graphically in quotient diagrams according to Reiber and Lange and can be interpreted using the legend.

■ **Automatic calculation of CSF/serum quotients** from pathogen-specific antibody, albumin and total IgA/G/M concentrations


■ **Safe and quick data transfer due to automated, bidirectional data communication** between the EUROIMMUN Analyzer I or I-2P or EUROLabWorkstation ELISA and photometer, LIS or nephelometer

■ **Clear graphic display** in quotient diagrams according to Reiber and Lange

■ **Optional use of a storable standard curve** for highest economic efficiency with simultaneous result security

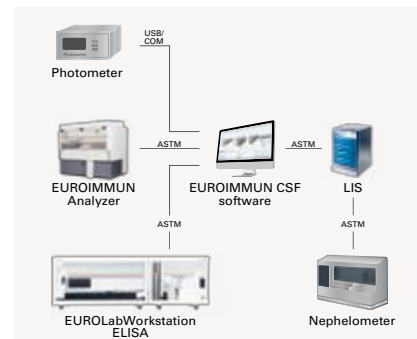





## Product overview

Software	Description	Order number
EUROIMMUN CSF Software	Software for automated calculation of CSF/serum quotients ( $CSQ_{alb.}$ , $CSQ_{total}$ , IgA/G/M, $CSQ_{path.-spec.}$ , $CSQ_{lim.}$ and $CSQ_{rel.}$ or antibody index AI)	YG 0259-0101-1



# Special test kits and reagents for automation



### Format

- 1005: 10 slides with 5 fields each
- 2005: 20 slides with 5 fields each
- 1010: 10 slides with 10 fields each
- 1050: 10 slides with 50 fields each

**FC** **1512** - **1010** **-1**

### Product code

### Product classification

- DL: EUROLINE autoantibodies (test system with preequipped incubation tray) ..... page 88
- DN: EUROLINE infectious serology (test system with preequipped incubation tray) ..... page 89
- Further reagents for **ids** chemiluminescence tests ..... page 89
- FC: Test system for indirect immunfluorescence (EUROPattern): Autoantibodies..... page 90
- FW: Single slides for indirect immunfluorescence (EUROPattern): Autoantibodies..... page 90
- FR: Test system for indirect immunfluorescence (EUROPattern): Infectious serology ..... page 94
- FS: Single slides for indirect immunfluorescence (EUROPattern): Infectious serology ..... page 94
- FA: Test system for indirect immunfluorescence (EUROLabLiquidHandler)..... page 96
- FC: Test system for indirect immunfluorescence (EUROPattern&EUROLabLiquidHandler) .. page 96

For product orders the amount, product code and test name are required. **Test kits** comprise all reagents needed to perform the serological investigation. For diagnostics in indirect immunofluorescence, for example, these include slides, FITC-labelled antibodies against human immunoglobulin, positive and negative control sera (not available for some products) as well as embedding medium, cover glasses, sachets of PBS and Tween 20.

Substrates consisting of cell cultures and tissues which do not appear in this catalogue can be made to specification. In addition, BIOCHIP mosaics can be produced according to individual requirements. Apart from the customary package sizes and slide formats, special sizes are available as well. Quotations can be provided upon request.



## EUROLINE for the Determination of Autoantibodies (Test Systems with preequipped incubation trays)

Order No.	Antibodies against	Ig Class	Substrate	Format
DL 0160-5001 G	EUROLINE validation	IgG	EUROLINE	50 strips Immunoblot-PreQ
DL 1111-5001-7 G	Paraneoplastic Neurologic Syndromes - 12 Ag (amphiphysin, CV2, PNMA2 (Ma-2/Ta), Ri, Yo, Hu, recoverin, SOX1, titin, Zic4, GAD65, Tr (DNER) separately)	IgG	EUROLINE	50 strips Immunoblot-PreQ
DL 1300-5001-4 G	Autoimmune Liver Diseases (AMA M2, M2-3E, Sp100, PML, gp210, LKM-1, LC-1, SLA/LP, Ro-52 separately)	IgG	EUROLINE	50 strips Immunoblot-PreQ
DL 1360-0510 A	Autoimmune Gastrointestinal Diseases IgA (tissue transglutaminase (endomysium), gliadin-analogue fusion peptide (GAF-3X), mannan (ASCA))	IgA	EUROLINE	50 strips Immunoblot-PreQ
DL 1360-5001 G	Autoimmune Gastrointestinal Diseases IgG (tissue transglutaminase (endomysium), gliadin-analogue fusion peptide (GAF-3X), parietal cell antigen (PCA) separately Intrinsic factor, mannan (ASCA))	IgG	EUROLINE	50 strips Immunoblot-PreQ
DL 1530-5001-4 G	Autoimmune Inflammatory Myopathies 16 Ag (Mi-2 alpha, Mi-2 beta, TIF1g, MDA5, NXP2, SAE1, Ku, PM-Scl100, PM-Scl75, Jo-1, SRP, PL-7, PL-12, EJ, OJ, Ro-52 separately)	IgG	EUROLINE	50 strips Immunoblot-PreQ
DL 1530-5001-7 G	Autoimmune Inflammatory Myopathies 16 Ag et cN-1A (Mi-2 alpha, Mi-2 beta, TIF1g, MDA5, NXP2, SAE1, Ku, PM-Scl100, PM-Scl75, Jo-1, SRP, PL-7, PL-12, EJ, OJ, Ro-52, cN-1A separately)	IgG	EUROLINE	50 strips Immunoblot-PreQ
DL 1532-5001 G	Systemic Sclerosis Profile (Nucleoli) (Scl-70, CENP A, CENP B, RP11, RP155, fibrillarin, NOR90, Th/To, PM-Scl100, PM-Scl75, Ku, PDGFR, Ro-52 separately)	IgG	EUROLINE	50 strips Immunoblot-PreQ
DL 1590-5001-3 G	ANA Profile 3 (nRNP/Sm, Sm, SS-A, Ro-52, SS-B, Scl-70, PM-Scl, Jo-1, CENP B, PCNA, dsDNA, nucleosomes, histones, ribosomal P-proteins, AMA M2 separately)	IgG	EUROLINE	50 strips Immunoblot-PreQ
DL 1590-5001-8 G	ANA Profile 1 (nRNP/Sm, Sm, SS-A, Ro-52, SS-B, Scl-70, Jo-1, CENP B, dsDNA, nucleosomes, histones, ribosomal P-proteins separately)	IgG	EUROLINE	50 strips Immunoblot-PreQ
DL 1590-5001-23 G	ANA Profile 23 (nucleosomes, dsDNA, histones, SS-A, Ro-52, SS-B, nRNP/Sm, Sm, Mi-2 alpha, Mi-2 beta, Ku, CENP A, CENP B, Sp100, PML, Scl-70, PM-Scl100, PM-Scl75, RP11, RP155, gp210, PCNA, DFS70 separately)	IgG	EUROLINE	50 strips Immunoblot-PreQ
DL 1590-5001-30 G	ANA Profile 3 plus DFS70 (nRNP/Sm, Sm, SS-A, Ro-52, SS-B, Scl-70, PM-Scl, Jo-1, CENP B, PCNA, dsDNA, nucleosomes, histones, ribosomal P-proteins, AMA M2, DFS70 separately)	IgG	EUROLINE	50 strips Immunoblot-PreQ
DL 1590-5001-32 G	dsDNA, nucleosomes, histones, DFS70	IgG	EUROLINE	50 strips Immunoblot-PreQ
DL 1590-5001-33 G	ANA Profile et Mi-2, Ku, DFS70 (Mi-2, Ku, nRNP/Sm, Sm, SS-A, Ro-52, SS-B, Scl-70, PM-Scl100, Jo-1, CENP B, PCNA, dsDNA, nucleosomes, histones, ribosomal P-proteins, AMA M2, DFS70 separately)	IgG	EUROLINE	50 strips Immunoblot-PreQ



## EUROLINE for the Determination of Autoantibodies (Test Systems with preequipped incubation trays)

Order No.	Antibodies against	Ig Class	Substrate	Format
DL 1590-5001-35 G	Cytoplasm profile (AMA M2, M2-3E, ribosomal P-proteins, Jo-1 SRP, PL-7, PL-12, EJ, OJ, Ro-52 separately)	IgG	EUROLINE	50 strips Immunoblot-PreQ
DL 159z-5001 G	EUROLINE Anti-DFS70	IgG	EUROLINE	50 strips for Immunoblot PreQ

## EUROLINE for Infectious Serology (Test Systems with preequipped incubation trays)

Order No.	Antibodies against	Ig Class	Substrate	Format
DL 0160-5001 G	EUROLINE validation	IgG	EUROLINE	50 strips Immunoblot-PreQ
DN2131-0510 G	EUROLINE Borrelia-RN-AT (p18, p19, p20, p21, p58, OspC (p25), p39, p83, LBb, LBA, VlsE Bg, VlsE Bb, VlsE Ba separately)	IgG	EUROLINE	50 strips Immunoblot-PreQ
DN2131-0510 M	EUROLINE Borrelia-RN-AT (OspC Bg native, OspC Bb native, OspC Ba native, p39, VlsE Bb separately)	IgM	EUROLINE	50 strips Immunoblot-PreQ
DN2131-0510-2 M	EUROLINE Borrelia-RN-AT-adv (OspC-adv Bsp, OspC-adv Bg, OspC-adv Bb, OspC-adv Ba, p39, VlsE Bb separately)	IgM	EUROLINE	50 strips Immunoblot-PreQ
DN2525-0510 A	EUROLINE Hepatitis E Virus (separat: GT1 ORF2, GT2 ORF2, GT3 ORF2, GT4 ORF2)	IgA	EUROLINE	50 stripes Immunoblot-PreQ
DN2525-0510 G	EUROLINE Hepatitis E Virus (separat: GT1 ORF2, GT2 ORF2, GT3 ORF2, GT4 ORF2)	IgG	EUROLINE	50 stripes Immunoblot-PreQ
DN2525-0510 M	EUROLINE Hepatitis E Virus (separat: GT1 ORF2, GT2 ORF2, GT3 ORF2, GT4 ORF2)	IgM	EUROLINE	50 stripes Immunoblot-PreQ
DN2606-0510-1 G	EUROLINE Anti-SARS-CoV-2 Profile ( IgG)	IgG	EUROLINE	50 strips Immunoblot-PreQ
DN2790-0510-2 G	EBV Profile 2 (VCA gp125, VCA p19, EBNA-1, p22, EA-D separately)	IgG	EUROLINE	50 strips Immunoblot-PreQ
DN2790-0510-2 M	EBV Profile 2 (VCA gp125, VCA p19, EBNA-1, p22, EA-D separately)	IgM	EUROLINE	50 strips Immunoblot-PreQ

## Further Reagents for IDS Chemiluminescence Tests

IDS Order No.	Reagent	Format
IS-CAP300	IDS Top Cap Set	
IS-CT100	IDS-iSYS Trigger Set	2 x 250 ml
IS-CS100	IDS-iSYS System Liquid (Syst.I)	5 l
IS-CSC105	Sample Cups (500 µL)	1000 pieces
IS-CW100	IDS-iSYS Wash Solution (Wash S)	10 l
IS-DS200	IDS-iSYS D-SORB Solution	2 x 1 L
IS-IM100	IDS Immunocleaner	3 cartridges with 2 tanks of 27 mL each
IS-CC100	IDS-iSYS Cuvettes	960 pieces
IS-6010	IDS-iSYS Cartridge Checking System CCS	1 piece







## Diagnostics for Indirect Immunofluorescence: EUROPattern, Autoantibodies

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FC 1020-2005 FC 1020-2010	islet cells antibodies (PM) EUROPattern pancreas islets	IgG	1 BIOCHIP per field: pancreas	monkey	20 x 05 (test system) 20 x 10 (test system)
FC 1050-1005 FC 1050-1010 FC 1050-2005 FC 1050-2010	Endocrinology Screen (AM) EUROPattern adrenal cortex	IgG	1 BIOCHIP per field: adrenal gland	monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FC 1111-1005-1 FC 1111-1010-1	Neurology Mosaic 1 EUROPattern Yo, Hu, Ri, CV2, Ma, amphiphysin medullated nerves non-medullated nerves	IgG	3 BIOCHIPS per field: cerebellum nerves intestinal tissue	monkey monkey monkey	10 x 05 (test system) 10 x 10 (test system)
FC 1111-1005-8 FC 1111-1010-8	Neurology Mosaic 8 EUROPattern Yo, Hu, Ri, CV2, Ma, amphiphysin medullated nerves non-medullated nerves pancreas islets	IgG	4 BIOCHIPS per field: cerebellum nerves intestinal tissue pancreas	monkey monkey monkey monkey	10 x 05 (test system) 10 x 10 (test system)
FC 1111-12010-14	Neurology Mosaic 14 EUROPattern cerebellum antigens medullated nerves	IgG	2 BIOCHIPS per field cerebellum intestinal tissue	monkey monkey	120 x 10 (test system)
FC 1128-2005-1	NMOSD Screen 1 EUROPattern aquaporin-4 (AQP-4) Myelin-oligodendrocyte glycoprotein (MOG)	IgG PI	3 BIOCHIPS per field: transfected cells transfected cells control transfection	EU 90 EU 90 EU 90	20 x 05 (test system)
FC 1128-1005-50 FC 1128-1010-50 FC 1128-2005-50 FC 1128-2010-50	aquaporin-4 EUROPattern	IgG PI	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FC 112d-1005-6 FC 112d-1010-6 FC 112d-2005-6 FC 112d-2010-6	Autoimmune Encephalitis Mosaic 6 EUROPattern glutamate receptor (type NMDA) contactin-associated protein 2 (CASPR2) glutamate receptors (type AMPA1/2) leucine-rich glioma-inactivated protein 1 (LGI1) dipeptidyl aminopeptidase-like protein 6 (DPPX) GABA B receptor	IgG PI	6 BIOCHIPS per field: transfected cells transfected cells transfected cells transfected cells transfected cells transfected cells	EU 90 EU 90 EU 90 EU 90 EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FC 112d-1005-51 FC 112d-1010-51 FC 112d-2005-51 FC 112d-2010-51 FC 112d-12010-51	glutamate receptor (type NMDA) EUROPattern	IgG PI	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system)
FC 112m-2005-50	dipeptidyl aminopeptidase-like protein 6 (DPPX) EUROPattern	IgG PI	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	20 x 05 (test system)
FC 1156-2005-50	Myelin-Oligodendrocyte-Glycoprotein (MOG) EUROPattern	IgG PI	transfected cells control transfection	EU 90 EU 90	20 x 05 (test system)
FC 1200-1005 FC 1200-1010 FC 1200-2005 FC 1200-2010 FC 1200-12010	cytoplasm of granulocytes (cANCA, pANCA), nuclei of granulocytes (GS-ANA) EUROPattern	IgG EB	granulocytes, ethanol-fixed	human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system)
FC 1201-1005 FC 1201-1010 FC 1201-2005	granulocytes (cANCA, pANCA) EUROPattern	IgG EB	granulocytes, formaldehyde-fixed	human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system)
FC 1201-1005-2 FC 1201-1010-2 FC 1201-2005-2 FC 1201-2010-2 FC 1201-12010-2	Granulocyte Mosaic 2 EUROPattern cANCA, pANCA, GS-ANA, EUROPattern cANCA, pANCA, EUROPattern	IgG EB	2 BIOCHIPS per field: granulocytes (EOH) granulocytes (HCHO)	human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system)





Diagnostics for Indirect Immunofluorescence: EUROPattern, Autoantibodies					
Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FC 1201-1005-13 FC 1201-1010-13 FC 1201-2005-13 FC 1201-2010-13 FC 1201-12010-13 FC 1201-2450-13 FW1201-1005-13 FW1201-2010-13	<b>Granulocyte Mosaic 13 EUROPattern</b> cANCA, pANCA, GS-ANA, EUROPattern cell nuclei (ANA), cANCA, pANCA cANCA, pANCA, EUROPattern	IgG EB	3 BIOCHIPS per field: granulocytes (EOH) HEp-2+granulocytes (EOH) granulocytes (HCHO)	human human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system) 24 x 50 (test system) 10 x 05 (single slides) 20 x 10 (single slides)
FC 1201-1005-15 FC 1201-1010-15 FC 1201-2010-15 FC 1201-1050-15 FW1201-1005-15	<b>Granulocyte Mosaic 15 EUROPattern</b> cANCA, pANCA, GS-ANA, EUROPattern cell nuclei (ANA), cANCA, pANCA	IgG EB	2 BIOCHIPS per field: granulocytes (EOH) HEp-2+granulocytes (EOH)	human human	10 x 05 (test system) 10 x 10 (test system) 20 x 10 (test system) 10 x 50 (test system) 10 x 05 (single slides)
FC 1201-1005-22 FC 1201-1010-22 FC 1201-2005-22 FC 1201-2010-22	<b>EUROPLUS Granulocyte Mosaic 22</b> EUROPattern cANCA, pANCA, GS-ANA, EUROPattern cANCA, pANCA, EUROPattern pANCA: myeloperoxidase (MPO), EUROPattern cANCA: proteinase 3 (PR3), EUROPattern	IgG EB	4 BIOCHIPS per field: granulocytes (EOH) granulocytes (HCHO) MPO BIOCHIPS PR3 BIOCHIPS	human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FC 1201-1005-25 FC 1201-1010-25 FC 1201-2005-25 FC 1201-2010-25 FW1201-1005-25 FW1201-2010-25	<b>EUROPLUS Granulocyte Mosaic 25</b> EUROPattern cANCA, pANCA, GS-ANA, EUROPattern cell nuclei (ANA), cANCA, pANCA cANCA, pANCA, EUROPattern glom. basement membrane (GBM), EUROPattern pANCA: myeloperoxidase (MPO), EUROPattern cANCA: proteinase 3 (PR3), EUROPattern	IgG EB	6 BIOCHIPS per field: granulocytes (EOH) HEp-2+granulocytes (EOH) granulocytes (HCHO) GBM BIOCHIPS MPO BIOCHIPS PR3 BIOCHIPS	human human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (single slides) 20 x 10 (single slides)
FC 1201-1005-32 FC 1201-1010-32 FC 1201-2005-32 FC 1201-2010-32 FC 1201-12010-32 FW1201-1005-32 FW1201-1010-32	<b>EUROPLUS Granulocyte Mosaic 32</b> EUROPattern cANCA, pANCA, GS-ANA, EUROPattern cANCA, pANCA, EUROPattern cell nuclei (ANA), cANCA, pANCA pANCA: myeloperoxidase (MPO), EUROPattern cANCA: proteinase 3 (PR3), EUROPattern	IgG EB	5 BIOCHIPS per field: granulocytes (EOH) granulocytes (HCHO) HEp-2+granulocytes (EOH) MPO BIOCHIPS PR3 BIOCHIPS	human human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides)
FC 1250-2005	<b>Nephrology Screen (KM) EUROPattern</b> renal glomeruli (GBM)	IgG	kidney	monkey	20 x 05 (test system)
FC 1250-2005-1	<b>EUROPLUS Nephrology Screen 1 EUROPattern</b> Renal glomeruli (GBM) glomerular basement membrane (GBM)	IgG	2 BIOCHIPS per field kidney GBM-EUROPLUS	monkey	20 x 05 (test system)
FC 1254-1005-50 FC 1254-1010-50 FC 1254-2005-50 FC 1254-2010-50	<b>phospholipase A2 receptor (PLA2R)</b> EUROPattern	IgG PI	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FC 1300-1005-9 FC 1300-1010-9 FC 1300-2005-9 FC 1300-2010-9	<b>Autoimmune liver diseases Screen 9</b> EUROPattern mitochondria (AMA), LKM LKM, ANA smooth muscles (ASMA) F-actin	IgG PI	4 BIOCHIPS per field: kidney liver stomach VSM47	rat rat rat rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FC 1360-2005 FC 1360-2010	<b>Anti-Parietal cells (SM) IIFT EUROPattern</b>	IgG	stomach	monkey	20 x 05 test system 20 x 10 test system
FC 1430-2005	<b>Myasthenia gravis Screen (SMM) EUROPattern</b> skeletal muscle	IgG	1 BIOCHIP per field: musculus iliopsoas	monkey	20 x 05 (test system)
FC 1439-1005-1 FC 1439-12010-1	<b>Anti-VGKC-Ass. Proteins Mosaic 1 EUROPattern</b> leucine-rich glioma-inact. prot. 1 (LG1) contactin-associated protein 2 (CASPR2)	IgG PI	3 BIOCHIPS per field: transfected cells transfected cells control transfection	EU 90 EU 90 EU 90	10 x 05 (test system) 120 x 10 (test system)



## Diagnostics for Indirect Immunofluorescence: EUROPattern, Autoantibodies

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FC 1501-1005 FC 1501-1010 FC 1501-2005	<b>Dermatology Screen (EM) EUROPattern</b> epidermis: prickle cell desmosomes epidermal basement membrane	IgG+IgG4	oesophagus	monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system)
FC 1501-1005-7 FC 1501-1010-7 FC 1501-2005-7 FC 1501-2010-7	<b>EUROPLUS Dermatology Mosaic 7 EUROPattern</b> epidermis pemphigoid antigens BP230gC desmoglein 1 desmoglein 3 BP180-NC16A-4X	IgG+IgG4	6 BIOCHIPS per field: oesophagus salt-split skin transfected cells transfected cells transfected cells BP180-NC16A-4X EUROPLUS	monkey monkey EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FC 1501-1010-20 FC 1501-2005-20 FC 1501-2010-20	<b>Dermatology Mosaic 20 EUROPattern</b> epidermis pemphigoid antigens	IgG+IgG4	2 BIOCHIPS per field: oesophagus salt-split skin	monkey monkey	10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FC 1510-1005-1 FC 1510-1010-1 FC 1510-2005-1 FC 1510-2010-1 FC 1510-12010-1 FC 1510-2450-1 FW1510-2010-1 FW1510-1050-1	<b>cell nuclei (ANA) EUROPattern</b> cell nuclei (ANA)	IgG PI	HEp-2 cells liver (2 BIOCHIPS per field)	human monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system) 24 x 50 (test system) 20 x 10 (single slides) 10 x 50 (single slides)
FC 1512-1005-1 FC 1512-1010-1 FC 1512-2005-1 FC 1512-2010-1 FC 1512-1050-1 FC 1512-12010-1 FC 1512-2450-1 FW1512-1005-1 FW1512-1010-1 FW1512-2010-1 FW1512-1050-1	<b>cell nuclei (ANA) EUROPattern</b> cell nuclei (ANA)	IgG PI	HEp-20-10 cells liver (2 BIOCHIPS per field)	human monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 50 (test system) 120 x 10 (test system) 24 x 50 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 10 (single slides) 10 x 50 (single slides)
FC 1512-1005-2 FC 1512-12010-2 FC 1512-2450-2	<b>cell nuclei (ANA) EUROPattern</b> mitochondria (AMA)	IgG PI	HEp-20-10 cells kidney (2 BIOCHIPS per field)	human rat	10 x 05 (test system) 120 x 10 (test system) 24 x 50
FC 1520-1005 FC 1520-1010 FC 1520-2005 FC 1520-2010 FC 1520-1050 FC 1520-12010 FC 1520-2450 FW1520-1005 FW1520-1010 FW1520-2005 FW1520-2010 FW1520-1050	<b>cell nuclei (ANA) EUROPattern</b>	IgG PI	HEp-2 cells	human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 50 (test system) 120 x 10 (test system) 24 x 50 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides) 10 x 50 (single slides)
FC 1522-1005 FC 1522-1010 FC 1522-2005 FC 1522-2010 FC 1522-1050 FC 1522-12010 FW1522-1005 FW1522-2005 FW1522-2010	<b>cell nuclei (ANA) EUROPattern</b>	IgG PI	HEp-20-10 cells	human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 50 (test system) 120 x 10 (test system) 10 x 05 (single slides) 20 x 05 (single slides) 20 x 10 (single slides)



Diagnostics for Indirect Immunofluorescence: EUROPattern, Autoantibodies					
Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FC 1572-1005 FC 1572-1010 FC 1572-2005 FC 1572-2010	<b>dsDNA EUROPattern</b>	IgG EB	flagellates	Crithidia luciliae	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FC 1572-1005-1 FC 1572-1010-1 FC 1572-2005-1 FC 1572-2010-1 FC 1572-12010-1	<b>dsDNA (sensitive) EUROPattern</b>	IgG EB	flagellates	Crithidia luciliae	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system)
FC 1620-1005-1 FC 1620-1010-1 FC 1620-2005-1 FC 1620-2010-1	<b>AMA/ASMA IIFT (KR/SR) EUROPattern mitochondria (AMA) smooth muscles (ASMA)</b>	IgG	2 BIOCHIPs per field: kidney stomach	rat rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FC 1651-1005 FC 1651-1010	<b>F-actin EUROPattern</b>	IgG PI	VSM47	rat	10 x 05 (test system) 10 x 10 (test system)
FC 1800-1010-2 FC 1800-2005-2 FC 1800-2010-2 FC 1800-12010-2	<b>Mosaic Basic Profile 2 EUROPattern cell nuclei (ANA), LKM mitochondria (AMA), LKM smooth muscles (ASMA)</b>	IgG	3 BIOCHIPs per field: liver kidney stomach	rat rat rat	10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system)
FC 1802-1005-3 FC 1802-1010-3 FC 1802-2005-3 FC 1802-2010-3	<b>Mosaic Basic Profile 3A EUROPattern cell nuclei (ANA) EUROPattern cell nuclei (ANA) mitochondria (AMA) smooth muscles (ASMA)</b>	IgG PI	4 BIOCHIPs per field: HEp-20-10 cells liver kidney stomach	human monkey rat rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FC 1805-1010-13 FC 1805-2005-13 FC 1805-2010-13	<b>Mosaic Basic Profile 13B EUROPattern cell nuclei (ANA), EUROPattern cell nuclei (ANA), LKM mitochondria (AMA), LKM smooth muscles (ASMA)</b>	IgG PI	4 BIOCHIPs per field: HEP-2 cells liver kidney stomach	human rat rat rat	10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FC 1812-1005-3 FC 1812-1010-3 FC 1812-2005-3 FC 1812-0010-3	<b>Mosaic Basic Profile 3C EUROPattern cell nuclei (ANA), EUROPattern cell nuclei (ANA), LKM mitochondria (AMA), LKM smooth muscles (ASMA)</b>	IgG PI	4 BIOCHIPs per field: HEP-20-10 cells liver kidney stomach	human rat rat rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 100 x 10 (test system)
FC 1914-1005 A FC 1914-1010 A FC 1914-2005 A FC 1914-2010 A FC 1914-1005 G FC 1914-1010 G FC 1914-2005 G FC 1914-2010 G	<b>Coeliac Disease Screen (LM) EUROPattern endomysium</b>	IgA  IgGpa	liver	monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)



## Diagnostics for Indirect Immunofluorescence: EUROPattern, Infectious Serology

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FR 2191-1005-3 A FR 2191-1010-3 A FR 2191-1005-3 G FR 2191-1010-3 G FR 2191-1005-3 M FR 2191-1010-3 M	<b>Anti-Chlamydia MIF EUROPattern</b> Chlamydia trachomatis Chlamydia pneumoniae Chlamydia psittaci	IgA EB IgG EB IgM EB	4 BIOCHIPS per field: elementary bodies and non-infected cells	EU 40 EU 40 EU 40	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FR 2192-1005-80 A FR 2192-1005-80 G FR 2192-1005-80 M	<b>Chlamydia pneumoniae EUROPattern</b>	IgA EB IgG EB IgM EB	elementary bodies (MIF) non-infected cells (2 BIOCHIPS per field)	EU 40 EU 40	10 x 05 (test system) 10 x 05 (test system) 10 x 05 (test system)
FR 219b-1005-1 G FR 219b-1010-1 G  FR 219b-2010-1 M	<b>Bartonella henselae EUROPattern</b> <b>Bartonella quintana EUROPattern</b>	IgG PI  IgM EB	infected cells infected cells (2 BIOCHIPS per field) infected and non- infected cells (4 BIOCHIPS per field)	EU 70 EU 70 EU 70 EU 38	10 x 05 (test system) 10 x 10 (test system)  20 x 10 (test system)
FR 2201-1005-1 G FR 2201-1010-1 G	<b>Mycoplasma hominis EUROPattern</b> <b>Ureaplasma urealyticum EUROPattern</b>	IgG EB	infected cells infected cells non-infected cells (3 BIOCHIPS per field)	EU 38 EU 38 EU 38	10 x 05 (test system) 10 x 10 (test system)
FR 2536-1005 G FR 2536-1010 G FR 2536-2005 G FR 2536-2010 G FR 2536-1005 M FR 2536-1010 M FR 2536-2005 M FR 2536-2010 M	<b>HHV-6 EUROPattern</b>	IgG EB  IgM EB	infected cells	EU 30	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FR 2665-1005 G FR 2665-1005 M	<b>Yellow fever virus (YFV) EUROPattern</b>	IgG PI IgM PI	infected and non- infected cells (2 BIOCHIPS per field)	EU 14	10 x 05 (test system) 10 x 05 (test system)
FR 2668-1005 G FR 2668-1010 G FR 2668-1005 M FR 2668-1010 M	<b>Zika virus (ZIKV) EUROPattern</b>	IgG PI IgM PI	infected and non- infected cells (2 BIOCHIPS per field)	EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FR 2668-1005-1 G FR 2668-1010-1 G FR 2668-1005-1 M FR 2668-1010-1 M	<b>Arbovirus Fever Mosaic 2 EUROPattern</b> Zika virus (ZIKV) Chikungunya virus (CHIKV) Dengue virus types 1 - 4 (DENV)	IgG PI IgM PI	6 BIOCHIPS per field: infected cells infected cells infected cells	EU 14 EU 14 EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FR 266a-1005-1 G FR 266a-1010-1 G FR 266a-1005-1 M FR 266a-1010-1 M	<b>Mosaic Dengue virus types 1 - 4 (DENV) EUROPattern</b>	IgG PI IgM PI	4 BIOCHIPS per field: infected cells	EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FR 2730-2010-2 G FR 2730-2010-2 M	<b>Coxsackie virus screen (types A) EUROPattern</b> types A7, A9, A16, A24	IgG PI IgM PI	4 BIOCHIPS per field: infected cells	EU 38	20 x 10 (test system) 20 x 10 (test system)
FR 2730-2010-3 G FR 2730-2010-3 M	<b>Coxsackie virus screen (types B) EUROPattern</b> types B1, B2, B3, B4, B5, B6	IgG PI IgM PI	6 BIOCHIPS per field: infected cells	EU 38	20 x 10 (test system) 20 x 10 (test system)
FR 277a-1005-1 G FR 277a-1005-1 M	<b>Sandfly fever virus Mosaic 1 EUROPattern</b> types Sicilian, Naples, Toscana, Cyprus	IgG PI IgM PI	4 BIOCHIPS per field: infected cells	EU 14	10 x 05 (test system) 10 x 05 (test system)
FR 278h-1005-1 G FR 278h-1005-1 M	<b>Hantavirus Mosaic 1 EUROPattern</b> types Hantaan (HTNV), Sin Nombre (SNV), Puumala (PUUV), Dobrava (DOBV), Seoul (SEOV), Saaremaa (SAAV)	IgG PI IgM PI	6 BIOCHIPS per field: infected cells	EU 14	10 x 05 (test system) 10 x 05 (test system)



## Diagnostics for Indirect Immunofluorescence: EUOPattern, Infectious Serology

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FR 278m-1005-3 G FR 278m-1005-3 M	Hantavirus Mosaic 3: America types Sin Nombre (SNV), Andes (ANDV) EUOPattern	IgG PI IgM PI	2 BIOCHIPS per field: infected cells	EU 14	10 x 05 (test system) 10 x 05 (test system)
FR 2791-1005 G FR 2791-1010 G FR 2791-2010 G FR 2791-1010 M	Epstein-Barr virus capsid antigen (EBV-CA) EUOPattern Anti-EBV-CA IIFT EUOPattern (IgM)	IgG PI IgM PI	expressing cells	P3HR1	10 x 05 (test system) 10 x 10 (test system) 20 x 10 (test system) 10 x 10 (test system)
FR 2793-1010 C	Epstein-Barr virus nuclear antigen (EBNA) EUOPattern	C3c PI	expressing cells	Raji	10 x 10 (test system)
FR 2795-1005 G FR 2795-1010 G	Epstein-Barr virus early antigen (EBV-EA) EUOPattern	IgG PI	expressing cells	EU 33	10 x 05 (test system) 10 x 10 (test system)
FR 293a-1005 G FR 293a-1010 G FR 293a-1005 M FR 293a-1010 M	Chikungunya virus (CHIKV) EUOPattern	IgG PI IgM PI	infected and non- infected cells (2 BIOCHIPS per field)	EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)



## Diagnostics for Indirect Immunofluorescence: EUROLabWorkstation IFA

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FA 1111-12010-8	<b>Neurology Mosaic 8</b> Yo, Hu, Ri, CV2, Ma, amphiphysin medullated nerves non-medullated nerves pancreas islets	IgAGM	4 BIOCHIPS per field cerebellum nerves intestinal tissue pancreas	monkey monkey monkey monkey	120 x 10 (test system)
FC 1111-12010-14	<b>Neurology Mosaic 14 EUROPattern</b> cerebellum antigens medullated nerves	IgG	2 BIOCHIPS per field cerebellum intestinal tissue	monkey monkey	120 x 10 (test system)
FC 112d-12010-51	<b>glutamate receptor (type NMDA) EUROPattern</b>	IgG PI	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	120 x 10 (test system)
FC 1200-12010	<b>cytoplasm of granulocytes (cANCA, pANCA), nuclei of granulocytes (GS-ANA) EUROPattern</b>	IgG EB	granulocytes, ethanol-fixed	human	120 x 10 (test system)
FC 1201-12010-2	<b>Granulocyte Mosaic 2 EUROPattern</b> cANCA, pANCA, GS-ANA, EUROPattern cANCA, pANCA, EUROPattern	IgG EB	2 BIOCHIPS per field: granulocytes (EOH) granulocytes (HCHO)	human human	120 x 10 (test system)
FA 1201-12010-13 FA 1201-2450-13	<b>Granulocyte Mosaic 13</b> cANCA, pANCA, GS-ANA cell nuclei (ANA), cANCA, pANCA cANCA, pANCA	IgG	3 BIOCHIPS per field: granulocytes (EOH) HEp-2+granulocytes (EOH) granulocytes (HCHO)	human human human	120 x 10 (test system) 24 x 50 (test system)
FC 1201-12010-13 FC 1201-2450-13	<b>Granulocyte Mosaic 13 EUROPattern</b> cANCA, pANCA, GS-ANA, EUROPattern cell nuclei (ANA), cANCA, pANCA cANCA, pANCA, EUROPattern	IgG EB	3 BIOCHIPS per field: granulocytes (EOH) HEp-2+granulocytes (EOH) granulocytes (HCHO)	human human human	120 x 10 (test system) 24 x 50 (test system)
FC 1201-12010-32	<b>EUROPLUS Granulocyte Mosaic 32</b> EUROPattern cANCA, pANCA, GS-ANA, EUROPattern cANCA, pANCA, EUROPattern cell nuclei (ANA), cANCA, pANCA pANCA: myeloperoxidase (MPO), EUROPattern cANCA: proteinase 3 (PR3), EUROPattern	IgG EB	5 BIOCHIPS per field:  granulocytes (EOH) granulocytes (HCHO) HEp-2+granulocytes (EOH) MPO BIOCHIPS PR3 BIOCHIPS	human human human	120 x 10 (test system)
FC 1439-12010-1	<b>Anti-VGKC-Ass. Proteins Mosaic 1 EUROPattern</b> leucine-rich glioma-inact. prot. 1 (LGI1) contactin-associated protein 2 (CASPR2)	IgG PI	3 BIOCHIPS per field: transfected cells transfected cells control transfection	EU 90 EU 90 EU 90	120 x 10 (test system)
FA 1510-12010-1 FA 1510-2450-1	<b>cell nuclei</b> (ANA global test)	IgG	HEp-2 cells liver (2 BIOCHIPS per field)	human monkey	120 x 10 (test system) 24 x 50 (test system)
FC 1510-12010-1 FC 1510-2450-1	<b>cell nuclei (ANA) EUROPattern</b> cell nuclei (ANA)	IgG PI	HEp-2 cells liver (2 BIOCHIPS per field)	human monkey	120 x 10 (test system) 24 x 50 (test system)
FA 1512-12010-1 FA 1512-2450-1	<b>cell nuclei</b> (ANA global test)	IgG	HEp-20-10 cells liver (2 BIOCHIPS per field)	human monkey	120 x 10 (test system) 24 x 50 (test system)
FC 1512-12010-1 FC 1512-2450-1	<b>cell nuclei (ANA) EUROPattern</b> cell nuclei (ANA)	IgG PI	HEp-20-10 cells liver (2 BIOCHIPS per field)	human monkey	120 x 10 (test system) 24 x 50 (test system)
FC 1512-12010-2 FC 1512-2450-2	<b>cell nuclei (ANA) EUROPattern</b> mitochondria (AMA)	IgG PI	HEp-20-10 cells kidney (2 BIOCHIPS per field)	human rat	120 x 10 (test system) 24 x 50
FA 1520-12010	<b>cell nuclei (ANA)</b>	IgG	HEp-2 cells	human	120 x 10 (test system)





## Diagnostics for Indirect Immunofluorescence: EUROLabWorkstation IFA

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FC 1520-12010 FC 1520-2450	cell nuclei (ANA) EUROPattern	IgG PI	HEp-2 cells	human	120 x 10 (test system) 24 x 50 (test system)
FC 1522-12010	cell nuclei (ANA) EUROPattern	IgG PI	HEp-20-10 cells	human	120 x 10 (test system)
FC 1572-12010-1	dsDNA (sensitive) EUROPattern	IgG EB	flagellates	Crithidia luciliae	120 x 10 (test system)
FA 1800-12010-2	Mosaic Basic Profile 2 cell nuclei (ANA), LKM mitochondria (AMA), LKM smooth muscles (ASMA)	IgG	3 BIOCHIPS per field: liver kidney stomach	rat rat rat	120 x 10 (test system)
FC 1800-12010-2	Mosaic Basic Profile 2 EUROPattern cell nuclei (ANA), LKM mitochondria (AMA), LKM smooth muscles (ASMA)	IgG	3 BIOCHIPS per field: liver kidney stomach	rat rat rat	120 x 10 (test system)
FA 1914-12010 A FA 1914-12010 G	endomysium	IgA IgGpa	liver	monkey	120 x 10 (test system) 120 x 10 (test system)



# Autoimmune diagnostics





# Rheumatology

CTD · SLE · Vasculitis · RA · APS



For more information on this subject scan the QR code or enter the Quick Link code **q030** at [www.euroimmun.com](http://www.euroimmun.com)

## Connective tissue diseases

■ **Clinical information:** Connective tissue diseases (CTD) are rheumatic diseases. They include, for example, systemic *lupus erythematosus* (see chapter SLE), progressive systemic sclerosis, Sjögren's syndrome, myositis or Sharp syndrome.


Autoantibodies whose target antigens are located in the nucleus (so-called anti-nuclear antibodies, ANA) are important serological markers for CTD. Target antigens include, for example, nucleic acids, cell nuclear proteins and ribonuclear proteins.

The frequency (prevalence) of anti-nuclear antibodies in inflammatory rheumatic diseases lies between 20 and 100%. Therefore, differential ANA diagnostics is indispensable for the diagnosis of individual rheumatic diseases and their differentiation from other autoimmune diseases.

■ **Diagnostics:** The gold standard for the determination of ANA is the indirect immunofluorescence test (IIFT) with human epithelial cells (HEp-2), which is known for its high sensitivity and specificity. Positive and negative samples produce a large signal difference. In the microscopic evaluation it is possible to establish precisely how an indicator dye (generally fluorescein) is distributed in the tissue or the cells. A typical fluorescence pattern is produced for every bound autoantibody, depending on the location of the individual autoantigens.

The first International Consensus Statement on standardised nomenclature of HEp-2 cell patterns in indirect immunofluorescence (ICAP, [www.anapatterns.org](http://www.anapatterns.org)) defined fifteen nuclear, five mitotic and nine cytoplasmic patterns which are relevant for the diagnosis of various autoimmune diseases.

Furthermore, the consensus recommends that autoantibodies detected in indirect immunofluorescence be confirmed by additional specific tests (e.g. ELISA, line blot). The exclusive use of these monospecific test methods is inadequate for the determination of autoantibodies against cell nuclei, as not all relevant antigens are available in a purified form as yet. Thus, the corresponding ANA can only be detected by IIFT.




HEp-2 cells: ANA, granular pattern



## Product overview

Method	Substrate	Application	Order number	Page
IIFT	HEp-2 cells	Gold standard ANA screen	FA 1520-####	161
	HEp-20-10 cells	Easier evaluation due to increased number of mitotic phases	FA 1522-####	161
	HEp-2 cells/ liver	Additional differentiation of patterns using liver tissue	FA 1510-####-1	160
	HEp-20-10 cells/ liver/nRNP/Sm + Sm + SS-A SS-B + Scl-70 + Jo-1	Screening and confirmation on monospecific EUROPLUS antigen dots in one test system	FA 1512-####-22	161
ELISA	dsDNA, histones, ribosomal P-proteins, nRNP/Sm, Sm, SS-A, SS-B, Scl-70, Jo-1, centromeres	ANA screen ELISA using an antigen mixture that is specific for rheumatic diseases	EA 1590-9601-8 G	144
	Ribosomal P-proteins, nRNP/Sm, Sm, SS-A, SS-B, Scl-70, Jo-1, centromeres	ENA profile ELISA as confirmatory test based on individual monospecific antigens	EA 1590-9601-2 G	144
	cN-1A	First serological marker for inclusion body myositis	EA 1675-4801 G	145
Blot	dsDNA, nucleosomes, histones, SS-A, Ro-52, SS-B, nRNP/Sm, Sm, Mi-2 $\alpha$ , Mi-2 $\beta$ , Ku, CENP A, CENP B, Sp100, PML, Scl-70, PM-Scl100, PM-Scl75, RP11, RP155, gp210, PCNA, DFS70	Multiplex approach for confirmation and differentiation of all ANA patterns in agreement with the international consensus, ICAP ( <a href="http://www.anapatterns.org">www.anapatterns.org</a> )	DL 1590-1601-23 G	141
	AMA-M2, M2-3E, ribosomal P-proteins, Jo-1, SRP, PL-7, PL-12, EJ, OJ, Ro-52	Profile for confirmation and differentiation of all cytoplasmic patterns (ICAP)	DL 1590-1601-35	142
	Mi-2 $\alpha$ , Mi-2 $\beta$ , TIF1 $\gamma$ , MDA5, NXP2, SAE1, Ku, PM-Scl100, PM-Scl75, Jo-1, SRP, PL-7, PL-12, EJ, OJ, Ro-52, cN-1A	Comprehensive profile of myositis-specific antigens	DL 1530-1601-7 G	141
	Scl-70, CENP A, CENP B, RP11, RP155, fibrillarin, NOR90, Th/To, PM-Scl100, PM-Scl75, Ku, PDGFR, Ro-52	Comprehensive profile of systemic sclerosis-specific antigens	DL 1532-1601 G	141

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 148).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g077** at [www.euroimmun.com](http://www.euroimmun.com)



# Rheumatology

CTD · SLE · Vasculitis · RA · APS



For more information on this subject scan the QR code or enter the Quick Link code **q042** at [www.euroimmun.com](http://www.euroimmun.com)


## Systemic lupus erythematosus

■ **Clinical information:** Systemic *lupus erythematosus* (SLE) is a systemic autoimmune disease belonging to the collagenosis group. Diagnosis is based on 11 criteria defined by the American College of Rheumatology (ACR) and modified in 1997. If 4 of 11 criteria are present, the probability of SLE is between 80 and 90%.

Antibodies against dsDNA are the main focus in the serological diagnosis of SLE. These antibodies can be found in 60 to 90% of patients, depending on the activity of the disease. Anti-dsDNA antibodies are in rare cases also found in patients with other autoimmune diseases (e.g. autoimmune hepatitis) or infections as well as in clinically healthy persons. 85% of people in the latter group develop SLE within 5 years of initial detection of anti-dsDNA. However, SLE cannot be excluded if anti-dsDNA antibodies are not detected.

Antibodies against nucleosomes are also an exclusive marker of SLE, provided that they are determined using an advanced test system with a target antigen that is free of histone H1, Scl-70 and other non-histone proteins.

■ **Diagnostics:** Various test methods are available for the routine detection of autoantibodies against dsDNA: enzyme immunotests (ELISA, EURO-LINE), Farr RIA and the Crithidia luciliae immunofluorescence test (CLIFT). The various test systems differ, sometimes greatly, in sensitivity and specificity. Conventional CLIFT shows a particularly high disease specificity, while the IIFT Crithidia luciliae sensitive is a very sensitive test.



Crithidia luciliae: Aab against dsDNA

Using an innovative biological preparation, scientists at EUROIMMUN have developed a new test system: the Anti-dsDNA-NcX ELISA, which surpasses by far the diagnostic quality characteristics of all conventional anti-dsDNA ELISA. The secret of the innovation lies in the use of highly purified nucleosomes as the new linking substance. Since nucleosomes have a strong adhesive ability, even the smallest concentration of these is highly suited to coupling isolated dsDNA to the surface of a microplate well. Poly-L-lysine and protamine sulphate are now obsolete, and many false positive reactions can be avoided. In a clinical comparative study of 378 patients with rheumatic diseases (of these 209 with SLE), the Anti-dsDNA-NcX ELISA yielded an 8% higher sensitivity than the anti-dsDNA RIA (Farr assay), demonstrating its superior capabilities.


Nevertheless, different test methods identify different SLE subgroups. To increase the serological detection rate different test systems should be combined.





## Product overview

Method	Substrate	Application	Order number	Page
IIFT	Crithidia luciliae	Conventional IIFT with high specificity	FA 1572-####	162
	Crithidia luciliae sensitive	Screening IIFT with high sensitivity	FA 1572-####-1	162
	HEp-2 cells	Detection of the SLE-specific pattern homogeneous ANA on HEp-2 cells	FA 1520-####	161
ELISA	Highly purified genomic double-stranded DNA complexed with nucleosomes	Optimal first-line test, increased sensitivity and specificity through use of nucleosome linker	EA 1572-9601 G	144
	Nucleosomes	Highly specific detection of anti-nucleosome antibodies through use of highly purified mononucleosomes, which are free of contaminating proteins	EA 1574-9601 G	144
	dsDNA, histones, nucleosomes, nRNP/Sm, Sm, SS-A, SS-B, Scl-70	Profile ELISA with SLE-relevant antigens	EA 1590-9601-12 G	144
RIA	Plasmid DNA	Gold standard Farr assay for detection of anti-dsDNA antibodies	RA 1571-10001	150

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 148).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **Q096** at [www.euroimmun.com](http://www.euroimmun.com)



# Rheumatology

CTD · SLE · Vasculitis · RA · APS




For more information on this subject scan the QR code or enter the Quick Link code **q046** at [www.euroimmun.com](http://www.euroimmun.com)

## Vasculitis

■ **Clinical information:** According to the consensus introduced at the Chapel-Hill-Consensus conference and the generally renowned classification system, granulomatosis with polyangiitis (GPA, formerly: Wegener's granulomatosis, WG), microscopic polyangiitis (MPA), eosinophilic granulomatosis with polyangiitis (EGPA, formerly: Churg-Strauss syndrome (CSS)) are classed as the group of ANCA-associated vasculitides (AAV). ANCA (anti-neutrophil cytoplasm antibodies) are autoantibodies directed against antigens found in cytoplasmic granules of neutrophils and monocytes. They are important serological markers for the diagnosis of AAV.

Moreover, an association with ANCA has been described for some of the immune complex vasculitides. Patients with anti-GBM glomerulonephritides (serological marker: antibodies against the glomerular basement membrane; anti-GBM) are often ANCA positive (>35%). A positive result can indicate rapid-progressive glomerulonephritis or GPA. In patients with AAV with renal involvement, the parallel analysis of ANCA and anti-GBM antibodies is thus recommended.



Ethanol-fixed granulocytes: cANCA

■ **Diagnostics:** AAV diagnostics are primarily based on IIFT. Standard for IIFT is a BIOCHIP mosaic of ethanol (EOH)- and formaldehyde (HCHO)-fixed human granulocytes. Further EUROIMMUN-exclusive BIOCHIPS, e.g. HEp-2 cells with sedimented granulocytes, further increase the diagnostic certainty. The EUROPLUS technique allows the combination of conventional cell culture substrates with defined single antigens (PR3, MPO, GBM) on one test field. This considerably simplifies the interpretation of the immunofluorescence patterns.

IIFT allows the differentiation of two ANCA types: the cytoplasmic type (cANCA), which is associated with GPA and is almost always directed against proteinase 3 (PR3), and the perinuclear type (pANCA), which indicates a spectrum of various diseases. The main target antigen of pANCA in MPA and EGPA is myeloperoxidase (MPO), but antibodies against granulocyte elastase, lactoferrin, lysozyme, cathepsin G, beta-glucuronidase, azurocidin, h-lamp-2 and alpha-enolase are also found in connection with pANCA.

Positive IIFT results should always be confirmed with a monospecific anti-PR3 and anti-MPO test (e.g. ChLIA or ELISA (International Consensus Statement, Savige et al., Am J Clin Pathol, 1999 & 2003)). Since not all cANCA and pANCA are positive in a monospecific test, the highest sensitivity and specificity for ANCA detection can only be achieved with parallel performance of IIFT and ChLIA/ELISA.

pANCA are also of great relevance in the differentiation of chronic inflammatory bowel diseases (67% ulcerative colitis, 7% Crohn's disease). DNA-bound lactoferrin has been identified as the main target antigen (Teegen et al., Ann N Y Acad Sci, 2009).



**Innovative Anti-PR3-hn-hr ELISA with designer antigen:** The reagent wells of the Anti-PR3-hn-hr ELISA are coated with a mixture of human native (hn) and human recombinant (hr) PR3. Owing to this, the test has a significantly higher sensitivity (94%) at a very good specificity (99%) compared to other ELISAs using only a native antigen (88% and 78%, respectively). The significantly higher sensitivity of the PR3-hn-hr ELISA and its suitability for identifying relapses in patients under treatment has been described in an independent publication (Damoiseau et al., Ann Rheum Dis, 2009).

## Product overview

Method	Substrate	Application	Order number	Page
IIFT	Granulocytes (EOH)/ HEp-2 + granulocytes (EOH)/ granulocytes (HCHO)	Gold standard IIF screening test for ANCA	FA 1201-####-13	155
	Granulocytes (EOH)/ HEp-2 + granulocytes (EOH)/ granulocytes (HCHO)/ PR3/MPO/GBM/ BIOCHIPS	ANCA screening and con- firmation on monospecific EUROPLUS antigen dots (incl. GBM) in one test sys- tem	FA 1###-####-25	155
ELISA	Human proteinase 3 native and recombinant (human cDNA expressed in a human cell line, PR3-hn-hr)	Monospecific confirmatory test for anti-PR3 antibodies: increased sensitivity with highest specificity	EA 1201-9601-2 G	143
	Human MPO native	Monospecific confirmatory test for anti-MPO	EA 1211-9601 G	143
	PR3, MPO, elastase, cathepsin G, BPI, lactoferrin	Profile ELISA with ANCA- associated antigens	EA 1200-1208-1 G	143
Blot	PR3, MPO, GBM	Monospecific multiplex test for ANCA	DL 1200-1601-3 G	140
ChLIA	Human recombinant proteinase 3	Monospecific confirmatory test for anti-PR3 antibodies	LA 1201-10010 G	147
	Human MPO, native	Monospecific confirmatory test for anti-MPO antibodies	LA 1211-10010 G	147
	GBM (purified alpha-3 chain of type IV collagen)	Qualitative and quantitative test for anti-GBM antibodies	LA 1251-10010 G	147

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems **ids** for this indication in the following product lists (page 148).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q103** at [www.euroimmun.com](http://www.euroimmun.com)



# Rheumatology

CTD · SLE · Vasculitis · RA · APS



For more information on this subject scan the QR code or enter the Quick Link code **q037** at [www.euroimmun.com](http://www.euroimmun.com)

## Rheumatoid arthritis

■ **Clinical information:** Rheumatoid arthritis (RA) is characterised by painful, swollen joints, movement restriction and progressing joint destruction. 0.5 to 1% of the worldwide population is affected, women approximately twice as often as men. Most new cases are diagnosed in women between 55 and 64 years and in men between 65 and 75 years. A large share of RA patients (approx. 70%) produce autoantibodies against citrullinated peptides (ACPA). Consequently, immune complexes are formed and the inflammation of the joints proceeds.

Autoantibodies in RA appear on average 3 to 5 years, sometimes even 15 years before the first joint complaints. The most important autoantibodies in preclinical RA are rheumatoid factors (RF) and ACPA and those directed against Sa (citrullinated vimentin) and citrullinated enolase peptide 1 (CEP-1). For the detection of ACPA, mainly cyclic citrullinated peptides (CCP) are used as target antigens. ACPA are specific for RA and indicators of a severe, erosive destructive course. During the shift from the undifferentiated arthritis phase towards RA, ACPA levels increase and remain high. ACPA have a high predictive value for the development of RA. Their detection supports the early recognition of the disease.

■ **Diagnostics:** Since 2010, ACPA determination has been a component of the RA classification criteria of the American College of Rheumatology (ACR) and the European League Against Rheumatism (EULAR). ACPA are determined in parallel to rheumatoid factors. According to the scoring system of the ACR/EULAR classification, a high ACPA or RF titer is more relevant for the diagnosis of RA than a lower titer. Laboratory findings such as increased erythrocyte sedimentation rate, increased C-reactive protein and the detection of RF and/or ACPA are indicative of RA.


With ELISA and ChLIA, two different test systems are available for the determination of autoantibodies against CCP. For the detection of ACPA, the CCP antigen of the 2<sup>nd</sup> generation (CCP 2) is considered the gold standard. Test systems based on this antigen provide the highest sensitivity (80%, with a specificity of 98%). Antibodies against CCP are mainly IgG class antibodies and are more specific than RF, with a similar sensitivity. Anti-CCP antibodies are found in up to 60% of RF-negative patients.

CEP-1 is a further relevant autoantigen which is present in approx. 60% of the anti-CCP positive RA patients. The detection of antibodies against CEP-1 is highly specific for RA (specificity: 97.6%) and therefore suited as a supplementary test for confirmation of serological findings. Moreover, the detection of anti-CEP-1 supports the risk stratification: Anti-CEP-1 antibodies are associated with an erosive disease course and with interstitial lung diseases (Alunno et al. 2018). Furthermore, anti-CEP-1 antibodies occur with a subtype of RA in which smoking and the HLA-DRB1 "shared epitope" alleles represent the main risk factors (Mahdi et al. 2009). Since anti-CEP-1 antibodies are directed against a target antigen which actually occurs in RA, their detection can provide insight into the cause and the pathogenesis of the disease.



## Product overview

Method	Substrate	Application	Order number	Page
IIFT	HEp-2 cells	Gold standard ANA screen	FA 1520-####	161
ELISA	Cyclic citrullinated peptide (CCP)	Highly specific and prognostic test for the detection of RA-specific anti-CCP antibodies	EA 1505-9601 G	144
	Citrullinated alpha-enolase peptide 1 (CEP-1)	Highly specific autoantigen associated with particular subtypes of RA	EA 151b-9601 G	144
	Human IgG	Conventional rheumatoid factor IgM detection (also available for detection of rheumatoid factor IgA/IgG)	EA 1814-9601 M	145
ChLIA	Cyclic citrullinated peptides (CCP)	Highly automated random access test for detection of RA-specific anti-CCP antibodies	LA 1505-10010 G	147

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 148).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q093** at [www.euroimmun.com](http://www.euroimmun.com)



# Rheumatology

CTD · SLE · Vasculitis · RA · APS



For more information on this subject scan the QR code or enter the Quick Link code **q004** at [www.euroimmun.com](http://www.euroimmun.com)

## Anti-phospholipid syndrome

■ **Clinical information:** The first official classification criteria for anti-phospholipid syndrome (APS) were drafted in 1998 at a workshop at the 8<sup>th</sup> International Symposium on Anti-phospholipid Antibodies in Sapporo, Japan (Sapporo criteria; Wilson et al., *Arthritis & Rheumatism* 1999). According to these criteria, APS can be considered proven if at least one clinical and one serological criterion are met. Clinical criteria include vascular thrombosis, which must be established according to the stipulated criteria, and pregnancy complications such as premature births, spontaneous abortions and eclampsia. When the criteria were updated in 2004 (Miyakis criteria; Miyakis et al., *Journal of Thrombosis and Haemostasis* 2005) antibodies against  $\beta 2$  glycoprotein 1 were added. Fulfilment of the criteria now encompasses at least one of the following three parameters: antibodies against cardiolipin (ACA; IgG or IgM) or  $\beta 2$  glycoprotein 1 (anti- $\beta 2$ GP1; IgG or IgM) or a positive lupus anticoagulant (LA) test. The latter is a coagulation test. According to official recommendations the serological criteria for APS diagnosis are only fulfilled when the result is confirmed 12 weeks later in a further test. A further update of the classification criteria in 2012 (Lakos et al., *Arthritis & Rheumatism* 2012) included the additional recommendation that when IgG and IgM tests for ACA or anti- $\beta 2$ GP1 IgG are negative, IgA should be tested as well.

In serological APS diagnostics autoantibodies of several immunoglobulin classes (IgAGM) can occur simultaneously, although often only one Ig class is detected. The association of particular immunoglobulin classes (IgAGM) with particular clinical parameters is controversially discussed.

Since around 10% of the healthy normal population exhibit anti-phospholipid antibodies (APLA) in the form of ACA or LA and these antibodies can also be induced by infections or specific medications (e.g. procainamide and hydralazine), both a positive serological result and a clinical criterion must be present in order to establish the diagnosis APS.

■ **Diagnostics:** ELISA is the method of choice for detection of APLA, since it is highly sensitive, simple to perform and does not require fresh plasma. EUROIMMUN offers microtiter ELISAs for quantitative determination of autoantibodies against cardiolipin,  $\beta 2$ GP1 and phosphatidylserine. The immunoglobulin classes IgA, IgG and IgM can be investigated separately or together (IgAGM). Alternatively, lupus anticoagulant can be determined using a multi-stage procedure according to the guidelines of the International Society on Thrombosis and Haemostasis. The phospholipid-dependent coagulation tests used for this purpose have a high specificity for APS, but a low sensitivity. Moreover, since there is no gold standard, results vary depending on the test method used, making it difficult to obtain reliable serological results.

EUROIMMUN ELISAs for the detection of antibodies against cardiolipin and  $\beta 2$ GP1 show a very high specificity in clinical studies. Sera from patients with viral hepatitis or parvovirus B19 infections and sera from healthy blood donors demonstrated only 0 to 2% positive results, while in studies using tests from other manufacturers values of between 12 and 50% were obtained. APLA can occur in cases of syphilis, which explains the somewhat high occurrence (11 to 13%) of ACA and anti- $\beta 2$ GP1 antibodies in these patients. The prevalence of both autoanti-






bodies in APS (86%) and SLE (24 to 25%) corresponds to data in current literature. For ACA in particular a very high agreement with an international meta-study was found (cohort of 1000 patients, 88% of APS patients were ACA positive; Cervera R. et al., Arthritis & Rheumatism 2002).

## Product overview

Method	Substrate	Application	Order number	Page
ELISA	Cardiolipin (AMA-M1)	Highly specific ELISA for the detection of anti-cardiolipin antibodies of classes IgG and IgM as recommended by the consensus statement (also available for detection of IgA and IgAGM)	EA 1621-9601 G/M	145
	$\beta$ 2-glycoprotein 1	ELISA for the detection of antibodies against $\beta$ 2-glycoprotein 1 of classes IgG and IgM as recommended by the consensus statement (also available for detection of IgA and IgAGM)	EA 1632-9601 G/M	145
	Phosphatidylserine	ELISA for the detection of antibodies against phosphatidylserine (also available for detection of IgA and IgAGM)	EA 162a-9601 G/M	145

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 148).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q052** at [www.euroimmun.com](http://www.euroimmun.com)



# Hepatology

Autoimmune hepatitis · Primary biliary cholangitis




For more information on this subject scan the QR code or enter the Quick Link code **q007** at [www.euroimmun.com](http://www.euroimmun.com)

## Autoimmune hepatitis

■ **Clinical information:** Autoimmune hepatitis (AIH; previously called lupoid hepatitis, chronic active hepatitis) predominantly affects women (75% of cases). The disease manifests by an increase in bilirubin, liver enzymes and immunoglobulins, by characteristic histological changes (liver biopsy shows necrosis of the parenchyma cells with lymphocyte and plasma cell infiltration) and the presence of various autoantibodies. The disease can occur from early childhood up to old age, but is most frequent in young to middle adulthood. In Western Europe the incidence of AIH is 1.9 cases per 100,000 inhabitants per year. Untreated, AIH soon develops into liver cirrhosis. However, with low-dose immunosuppressive therapy administered in good time and consistently right up until death, patients have a normal life expectancy. In the differential diagnosis, an infection with hepatitis viruses must be ruled out through the investigation of the appropriate serological parameters.

■ **Diagnostics:** Circulating autoantibodies have come to play a significant role in the diagnosis of AIH. They occur in the majority of patients, although their role in pathogenesis is debatable. There is no clear correlation between the disease activity or prognosis and the antibody titer.

The following autoantibodies are associated with AIH: antibodies against cell nuclei (ANA), native DNA, smooth muscle (ASMA, most important target antigen: F-actin), soluble liver antigen/liver-pancreas antigen (SLA/LP), liver-kidney microsomes (LKM-1, target antigen: cytochrome P450 IID6) and liver cytosolic antigen type 1 (LC-1, target antigen: formiminotransferase cyclodeaminase). The autoantibodies against SLA/LP that can today be detected by various EUROIMMUN enzyme immunoassays have the highest diagnostic accuracy of all antibodies involved in AIH. Anti-SLA/LP antibodies occur in AIH either alone or together with other autoantibodies. Their prevalence is only between 10 and 30%, but the predictive value is almost 100%. Essentially, every positive finding is evidence of autoimmune hepatitis (as long as the corresponding clinical symptoms are present).




VSM47 cells: Aab against F-actin

Furthermore, high concentrations of autoantibodies against smooth muscles (ASMA) indicate AIH. One part of the antibodies is directed against conformational epitopes of F-actin, which are only present in frozen tissue sections or tissue cells and cannot therefore be detected by ELISA or Westernblot. In contrast to other ASMA, antibodies against F-actin are a very specific marker for type 1 AIH. With the cell line VSM47 (vascular smooth muscle) the microfilamentous (MF) fluorescence pattern can be easily and clearly differentiated from non-MF patterns, thus facilitating the diagnosis of type 1 AIH.



## Product overview

Method	Substrate	Application	Order number	Page
IIFT	VSM47	Specific cell line for the detection of antibodies against F-actin by IIFT	FA 1651-####	162
	HEp-2 cells, liver, kidney, stomach	Basic profile for the detection of ANA, AMA, ASMA, LKM	FA 1800-####-3	163
	Liver, VSM47, HEp-2 cells, liver, kidney, stomach	Comprehensive detection of AIH-specific antibodies with a BIOCHIP Mosaic of 6 substrates	FA 1300-####-8	156
ELISA	Soluble liver antigen/ liver-pancreas antigen (SLA/LP)	Specific antibodies for precise discrimination from other hepatitides	EA 1302-9601 G	143
	Liver-kidney microsomes (LKM-1)	Serological marker for type 1 AIH	EA 1321-9601 G	143
	Cytosolic liver antigen type 1 (LC-1)	Supplementary diagnostic parameter for AIH	EA 1307-9601 G	143
Blot	AMA-M2, M2-3E, Sp100, PML, gp210, LKM-1, LC-1, SLA/LP, Ro-52	EUROLINE Profile Autoimmune Liver Diseases enables analysis of nine different AIH- and PBC-relevant autoantibodies on one test strip	DL 1300-1601-4 G	140
	AMA-M2, M2-3E, Sp100, PML, gp210, LKM-1, LC-1, SLA/LP, SS-A, Ro-52, Scl-70, CENP A, CENP B and PGDH	The EUROLINE enables analysis of fourteen different autoantibodies for the diagnosis of PBC, in suspected cases of AIH and overlap syndromes	DL 1300-1601-5 G	140

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 148).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g057** at [www.euroimmun.com](http://www.euroimmun.com)



# Hepatology

Autoimmune hepatitis · Primary biliary cholangitis




For more information on this subject scan the QR code or enter the Quick Link code **q035** at [www.euroimmun.com](http://www.euroimmun.com)

## Primary biliary cholangitis

■ **Clinical information:** Primary biliary cholangitis (PBC) is an immune-mediated chronic inflammatory cholestatic liver disease of unknown aetiology. The disease is characterised by female predominance (>90%) with most cases observed between the ages of 40 and 60. PBC incidence in different parts of the world is estimated to be 4 to 31 cases/million persons per year. PBC is marked by lymphocellular infiltration around the small intra-hepatic biliary ducts (bile canaliculi) and the build-up of bile (cholestasis). The disease often begins with unspecific, very varying general symptoms, such as itching (pruritus), fatigue and pain in the upper right region of the abdomen. An obstructive jaundice develops after a varying period of time. The increase in serum lipids is an important indicator for PBC. Histologically, changes occur in the liver corresponding to a chronic, non-suppurative destructive cholangitis: granulating pericholangitis, i.e. slowly progressing destruction of the small and medium-sized biliary ducts with subsequent fibrosis, the final stage of which is complete cirrhosis. In addition to the liver, often other organs with exocrine functions are also affected, above all the lachrymal and salivary glands and the pancreas.

■ **Diagnostics:** The diagnosis of PBC includes liver function tests (determination of alkaline phosphatase, aspartate transaminase and alanine transaminase), the determination of serum lipids, screening for anti-mitochondrial antibodies (AMA) and anti-nuclear antibodies (ANA) and the differentiation from other chronic inflammatory diseases of the liver, such as chronic viral hepatitis, autoimmune hepatitis or primary sclerosing cholangitis.

The detection of AMA is of great importance in the diagnosis of PBC. Antibodies against the M2 antigen are the most sensitive and specific diagnostic marker. These antibodies can be found in 94% of PBC patients. High-titer anti-M2 antibody seropositivity is an important tool in the diagnosis of PBC and a very powerful predictor of future development of PBC in patients without significant liver function disorders or symptoms suggestive of cholestatic diseases. Besides AMA, ANA may also be found in about one third of patients with PBC by indirect immunofluorescence. Promyelocytic leukaemia (PML) proteins and Sp100, which generate a nuclear dot pattern in IIFT, and two components of the nuclear pore complex (gp210 and p62) that have been specifically associated with a perinuclear pattern have been identified as specific ANA target antigens in PBC.




Rat kidney: AMA



## Product overview

Method	Substrate	Application	Order number	Page
IIFT	Kidney	Gold standard for the detection of AMA	FA 1620-####	162
	HEp-2 cells, liver, kidney, stomach	Basic profile for the detection of ANA, AMA, ASMA	FA 1800-####-3	163
	HEp-2 cells	Detection of further antibodies besides AMA: nuclear dots (Sp100, PML) and nuclear membrane (gp210 and p62)	FA 1520-####	161
	Kidney, stomach, HEp-2 cells, M2 BIOCHIPs	Mosaic of tissue substrates and HEp-2 cells supplemented by a EUROPLUS BIOCHIP with purified M2 antigen	FA 1620-####-5	162
ELISA	AMA M2-3E	ELISA with highest sensitivity through a combination of all three multi-enzyme complexes of the M2 antigen	EA 1622-9601 G	145
Blot	AMA-M2, M2-3E, Sp100, PML, gp210, LKM-1, LC-1, SLA/LP, Ro-52	EUROLINE Profile Autoimmune Liver Diseases enables analysis of nine different AIH- and PBC-relevant autoantibodies on one test strip	DL 1300-1601-4 G	140
	AMA-M2, M2-3E, Sp100, PML, gp210, LKM-1, LC-1, SLA/LP, SS-A, Ro-52, Scl-70, CENP A, CENP B and PGDH	The EUROLINE enables analysis of fourteen different autoantibodies for the diagnosis of PBC, in suspected cases of AIH and overlap syndromes	DL 1300-1601-5 G	140

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 148).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q091** at [www.euroimmun.com](http://www.euroimmun.com)



# Gastroenterology

Coeliac disease · CIBD · Autoimmune gastritis / Pernicious anaemia




For more information on this subject scan the QR code or enter the Quick Link code **q048** at [www.euroimmun.com](http://www.euroimmun.com)

## Coeliac disease

■ **Clinical information:** Coeliac disease (also gluten-sensitive enteropathy, GSE) is a systemic autoimmune disease in which genetic predisposition play a pronounced role. Coeliac disease may affect different organ systems. Its prevalence is estimated to be around 1%, with experts assuming a large number of undiagnosed cases due to atypical or mild symptoms. Coeliac disease mostly manifests as a severe inflammation and damage of the mucosa of the small intestine (enteropathy). In conjunction with the resulting disruption of the nutrient absorption, a wide range of clinical gastrointestinal and non-gastrointestinal symptoms (among others chronic diarrhoea, abdominal pain, weight loss), can be observed. In addition, the clinical manifestation of coeliac disease may include a chronic rash in the form of Duhring's dermatitis.

Coeliac disease is caused by an overreaction of the immune system following ingestion of gluten, especially of the so-called gliadin, which accounts for around 90% of the protein content of many grains. Gliadin can be only partially digested in the small intestine. If the intestinal epithelium presents gaps, as typically occurs in patients with coeliac disease, gliadin fragments may pass the intestinal barrier and reach the underlying connective tissue. There, the enzyme tissue transglutaminase (tTG) deamidates the amino acid glutamine into glutamic acid at specific loci of the gliadin peptides. Given a genetic predisposition, this modification causes the peptides to have an immunological effect. Activation of the B cells leads to the formation of antibodies against the deamidated gliadin peptides (DGP) and the body-own tTG. Furthermore, T-cells secrete proinflammatory cytokines, which cause inflammatory reactions in the tissue.

■ **Diagnostics:** According to the guidelines of the European Society of Pediatric Gastroenterology, Hepatology and Nutrition (ESPGHAN) (Husby et al., 2020), patients with corresponding symptoms should be first investigated for anti-tTG antibodies (IgA) and total IgA antibodies. In the case of a positive test result, this should be confirmed by determination of EmA (IgA). Moreover, the guidelines point out the additional use of coeliac-specific IgG-based tests, e.g. tests for detection of antibodies against DGP. If there is a general IgA deficiency – a state often observed in coeliac disease patients – anti-DGP antibodies (IgG) are considered an important indicator of coeliac disease. EmA can be detected by IIFT on tissue sections of primate liver, primate oesophagus or primate intestine. The target antigen of EmA is tTG. Anti-tTG antibodies can be detected by ChLIA, ELISA or EUROLINE tests. In addition, anti-DGP antibodies can be detected using ChLIA, ELISA, EUROLINE and the monospecific EUROPLUS substrate.




Monkey liver: Aab against endomysium





## Product overview

Method	Substrate	Application	Order number	Page
IIFT	Liver	Characteristic fluorescence enables easy EmA identification	FA 1914 A or G	164
	Oesophagus	Classic substrate for detection of EmA	FA 1911 A or G	165
	Liver, gliadin (GAF-3X) BIOCHIPS	Mosaic of tissue substrate supplemented by EUROPLUS BIOCHIP with GAF-3X antigen	FA 1914-1 A or G	164
ELISA	Tissue transglutaminase (endomysium; class IgA)	Established anti-tTG ELISA to support the diagnosis and monitor therapy	EA 1910-9601 A	145
	Tissue transglutaminase (endomysium; class IgG)	ELISA to support the diagnosis (esp. in IgA deficiency)	EA 1910-9601 G	145
	Gliadin (GAF-3X; class IgG)	Detection of Aab against DGP (esp. in IgA deficiency)	EV 3011-9601 G	146
	Gliadin (GAF-3X; class IgA)	Supplementary serological test	EV 3011-9601 A	146
ChLIA	Tissue transglutaminase (endomysium; class IgA)	ChLIA for determination of anti-tTG antibodies (IgA)	LA 1910-10010 A	147
	Tissue transglutaminase (endomysium; class IgG)	ChLIA to support the diagnosis (esp. in IgA deficiency)	LA 1910-10010 G	147
	Gliadin (GAF-3X; class IgG)	ChLIA for detection of Aab (esp. in IgA deficiency)	LV 3011-10010 G	147
	Gliadin (GAF-3X; class IgA)	Supplementary serol. test	LV 3011-10010 A	147
Blot	Tissue transglutaminase, gliadin (GAF-3X)	Detection of selective IgA deficiency and ">10xULN"	DL 1910-#### G DL 1910-#### A	142
	Saccharomyces cerevisiae, intrinsic factor, parietal cells (PCA), gliadin (GAF-3X), tissue transglutaminase (tTG)	EUROLINE for differential diagnostics of coeliac disease, autoimmune gastritis/pern. anaemia & Crohn's disease	DL 1360-#### G DL 1360-#### A	140

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 148).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g107** at [www.euroimmun.com](http://www.euroimmun.com)



# Gastroenterology

Coeliac disease · CIBD · Autoimmune gastritis / Pernicious anaemia



For more information on this subject scan the QR code or enter the Quick Link code **q011** at [www.euroimmun.com](http://www.euroimmun.com)

## Chronic inflammatory bowel diseases


■ **Clinical information:** The most important chronic inflammatory bowel diseases (CIBD) include ulcerative colitis (UC) and Crohn's disease (CD).

UC belongs to the CIBD with autoimmune reactions against the mucosa and submucosa of the colon or rectum and increased immune reactions against the intestinal flora. A genetic susceptibility for UC is assumed and the disease is supposed to be triggered by certain environmental factors. The inflammation spreads continuously from the rectum, that is from the anal region upwards.

CD is classified as an autoimmune disease of the intestinal mucosa and is characterised by a high recurrence rate. The chronic granulomatous inflammation, which can affect the whole digestive tract from the oral cavity to the anus, is found in most cases only in the lower small intestine (terminal ileum) and the large intestine (colon), very rarely in the oesophagus and mouth. CD is characterised by discontinuous, segmental attack on the intestinal mucosa. Resulting thereof, several sections of the intestine may be affected simultaneously, being interrupted by healthy sections.

■ **Diagnostics:** Initial differentiation between irritable bowel syndrome and CIBD can be achieved by non-invasive antigen detection of calprotectin in stool and thus provide a decisive precharacterisation of bowel-associated inflammation (see chapter Calprotectin). Alongside the single IIF tests, the high diagnostic demands on differentiated CIBD diagnostics are also met by various highly specific mosaics (CIBD profiles) specifically developed for serological diagnostics of the autoimmune intestinal diseases CD and UC.

Autoantibodies against the exocrine pancreas are a characteristic feature of CD. They have a high disease-specific significance due to their organ specificity, disease association and frequently high serum concentration. Due to the fact that the inflammation of the intestinal wall in CD is caused by the autoantigens contained in the pancreas secretion, particularly the proteoglycans CUZD1 and GP2, the determination of autoantibodies against the pancreas antigens rPAg1 (CUZD1) and PAg2 (GP2) using IIFT represents a new dimension in serological CD diagnostics. Antibodies against *Saccharomyces cerevisiae* (ASCA) enrich the serodiagnostics for CD by a further specific parameter.




rPAg1/2 transfected EU90 cells

Autoantibodies against intestinal goblet cells, which occur exclusively in UC, are pathognomonic markers for this autoimmune disease. The target antigen responsible for UC has not yet been exactly identified.



## Product overview

Method	Substrate/Analyte	Application	Order number	Page
IIFT	Pancreas antigens rPAg1(CUZD1) / rPAg2(GP2), intestinal goblet cells	Efficient screening and differentiation test for detection of antibodies in CIBD; differentiation between UC and CD	FA 1391-####-3	165
	Pancreas antigens rPAg1(CUZD1) / rPAg2(GP2), intestinal goblet cells, granulocytes, <i>Saccharomyces cerevisiae</i>	Efficient screening and differentiation test for detection of antibodies in CIBD; differentiation between UC and CD	FA 1391-####-7	156
ELISA	<i>Saccharomyces cerevisiae</i>	Monospecific detection of antibodies against <i>S. cerevisiae</i> in CD (also available for IgG detection)	EV 2841-9601 A	146
Antigen ELISA	Faecal calprotectin	Ideally suited for discrimination of inflammatory bowel disease from irritable bowel syndrome and for monitoring of the disease course	EQ 6831 W	261
Blot	<i>Saccharomyces cerevisiae</i> , intrinsic factor, parietal cells (PCA), gliadin (GAF-3X), tissue transglutaminase (tTG)	EUROLINE profile for differential diagnostics of coeliac disease, autoimmune gastritis/pernicious anaemia and CD	DL 1360-#### G DL 1360-#### A	140

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 148).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q062** at [www.euroimmun.com](http://www.euroimmun.com)



# Gastroenterology

Coeliac disease · CIBD · Autoimmune gastritis / Pernicious anaemia




For more information on this subject scan the QR code or enter the Quick Link code **q034** at [www.euroimmun.com](http://www.euroimmun.com)

## Autoimmune gastritis / Pernicious anaemia

■ **Clinical information:** Autoimmune gastritis (AIG) is a chronic inflammation of the stomach mucosa which hinders iron and vitamin B12 uptake and may lead to atrophic gastritis with malabsorption. The stomach mucosa is infiltrated by lymphocytes, plasma cells and granulocytes. Epithelial cells become necrotic, and main and parietal cells are replaced by mucoid cells. As a final stage, atrophy develops over many years. AIG causes a limited production of pepsin, hydrochloric acid and intrinsic factor (IF). Over the course of year, the vitamin B12 deficiency leads to pernicious anaemia (PA). In most patients, AIG remains asymptomatic over many years until reaching advanced stages of atrophy. Symptoms of PA are anaemia, fatigue, light-headedness and tachycardia. Moreover, the vitamin B12 deficiency hinders DNA synthesis, which causes megaloblasts to be formed in the bone marrow and the gastrointestinal epithelium. This results in malabsorption and diarrhoea with weight loss, anorexia, glossitis, icterus and neurological complaints.

■ **Diagnostics:** AIG is characterised by the presence of autoantibodies against parietal cells (PCA) and IF.

Antibodies against PCA occur in patients with AIG as well as PA. They mainly belong to the classes IgG and IgA. The prevalence of antibodies against PCA is very high in almost all patients with chronic-atrophic gastritis, amounting to nearly 100%. Antibodies against PCA also have a very high sensitivity for PA, amounting to 80% to 90% at the time of diagnosis. To increase the specificity, EUROIMMUN developed the Anti-ATP4B ELISA, which specifically detects the  $\beta$ -subunit of H<sup>+</sup>/K<sup>+</sup>-ATPase, the main antigen of anti-parietal cell antigens. Over the course of disease, their prevalence decreases due to the progressing destruction of the parietal cells. With respect to the specificity of the anti-PCA antibodies, it must be taken into account that they can also be detected in patients with endocrinopathies and in healthy blood donors.



Monkey stomach: Aab against parietal cells

IF is a glycoprotein secreted by the parietal cells. It forms complexes with vitamin B12, the absorption of which in the ileum is impaired by anti-intrinsic factor antibodies (IFA). Sera from AIG or PA patients contain two types of IFA (both IgG). IFA of type 1 react with the vitamin B12 binding site of the IF, IFA of type 2 hinder the binding of the IF to the receptors in the ileum. IFA have a very high specificity for AIG. With PA, IFA occur in 40% to 80% of patients depending on the disease stage.



## Product overview

Method	Substrate	Application	Order number	Page
IIFT	Stomach	Standard method for the detection of antibodies against parietal cells	FA 1360-####	157
	Stomach, intrinsic factor BIOCHIPs	The substrate combination of primate stomach and intrinsic factor BIOCHIPs in IIFT facilitates diagnosis of pernicious anaemia	FA 1362-####-1	157
	ATP4B	Semiquantitative or quantitative determination of antibodies against the recombinant beta-subunit of H <sup>+</sup> /K <sup>+</sup> -ATPase of the parietal cells	EA 1361-9601-1 G	143
ELISA	Parietal cells (PCA)	Semiquantitative or quantitative determination of antibodies against the native target antigen H <sup>+</sup> /K <sup>+</sup> -ATPase	EA 1361-9601 G	143
	Intrinsic factor	Specific detection of antibodies against intrinsic factor	EA 1362-9601 G	143
Blot	Saccharomyces cerevisiae, intrinsic factor, parietal cells (PCA), gliadin (GAF-3X), tissue transglutaminase (tTG)	EUROLINE profile for differential diagnostics of coeliac disease, autoimmune gastritis/pernicious anaemia and Crohn's disease	DL 1360-#### G DL 1360-#### A	140



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q086** at [www.euroimmun.com](http://www.euroimmun.com)



# Endocrinology

Diabetes · Thyroid diseases



For more information on this subject scan the QR code or enter the Quick Link code **q012** at [www.euroimmun.com](http://www.euroimmun.com)

## Diabetes


■ **Clinical information:** Type I diabetes mellitus (T1DM) is an autoimmune disease which is characterised by the destruction of the insulin-producing beta cells of the pancreatic islets of Langerhans. Genetic predisposition, as well as exogenous factors, e.g. viral infections, diet or obesity are considered to be the causative factors of the disease. Autoantibodies occurring with T1DM are called islet cell antibodies (ICA) and are directed against several antigens of the pancreatic islet cells. The most relevant antibodies are the 65-kDa isoform of the enzyme glutamic acid decarboxylase (GAD65), insulinoma-associated antigen 2 (IA2), zinc transporter 8 (ZnT8) and insulin.

The autoimmune reaction usually sets in years before the hyperglycaemic symptoms of T1DM. The destructive process, i.e. insulinitis, is characterised by immune cell infiltration in the pancreatic islets. T1DM becomes manifest when the major part of beta cells has been destroyed and the blood sugar level is no longer regulated. This development mostly takes place during childhood or adolescence. T1DM is the most severe form of diabetes and leads to lifelong dependence on insulin injections. 5 to 10% of all diabetes cases are of type I. The worldwide incidence of T1DM increases by 3 to 5% each year.

■ **Diagnostics:** ICA are detected in 70 to 80% of newly diagnosed T1DM cases. The different antibodies of this group usually develop subsequently, not simultaneously. The development of ICA precedes manifest T1DM by months or even years. In 90% of patients, one or more ICA can be detected even before the onset of clinical symptoms. The higher the number of different ICA in one person, the higher is their risk of developing T1DM.

Autoantibodies against insulin (IAA) are often the first autoantibodies to occur in T1DM. They can be found in almost all prediabetic persons; their prevalence decreases with increasing age of the patients. IAA can be detected in 80% of patients under ten years and around 60% of patients between 10 and 20 years of age. Children under 5 years present the highest IAA titers.

Autoantibodies against GAD65 (GADA) can be found in around 70% of patients before onset of T1DM and in 70 to 90% of T1DM patients at the beginning of the disease. GADA are the most sensitive markers for T1DM occurring in the adult age, as well as for LADA (latent autoimmune diabetes in adulthood). LADA is present in 3 to 12% of patients with phenotypical type II diabetes mellitus, which is characterised by insulin resistance and disturbed insulin secretion from the beta cells. 90% of LADA patients present GADA and most of them are positive for GADA already several years before the diagnosis.



Monkey pancreas: Aab against islet cells





Autoantibodies against IA2 can be found in 50 to 70% of children and adolescents and in 30 to 50% of adults with newly diagnosed T1DM. In around half of the patients, IA2A are detected even prior to the disease manifestation. IA2A are highly specific for T1DM.

Anti-ZnT8 antibodies are detectable in the sera of many children with prediabetes. They persist until manifestation of T1DM. The anti-ZnT8 level drops rapidly over the first years following disease onset. Anti-ZnT8 antibodies are also detected in nearly 25% of LADA patients. As with other autoantibodies, their presence can predict the transition to the insulin-dependent stage in LADA patients. Combined determination of antibodies against GAD65, IA2, ZnT8 and insulin enables the identification of T1DM already at disease onset in 98% of cases.

## Product overview

Method	Substrate	Application	Order number	Page
IIFT	Pancreas	Detection of autoantibodies against islet cells (ICA)	FA 1020-#### FC 1020-####	151
ELISA	Glutamic acid decarboxylase (GAD)	Solid-phase test systems for non-radioactive, monospecific detection of autoantibodies against the biochemically characterised antigens GAD, IA2 and ZnT8	EA 1022-9601 G	143
	Tyrosine phosphatase (IA2)		EA 1023-9601 G	143
	Zinc transporter 8 (ZnT8)		EA 1027-9601	143
	GAD/IA2 pool		EA 1022-9601-1 G	143
RIA	Insulin	Liquid-phase test systems for radioactive, monospecific detection of autoantibodies against the biochemically characterised insulin antigen	RA 1024-####	150



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g064** at [www.euroimmun.com](http://www.euroimmun.com)



# Endocrinology

Diabetes · Thyroid diseases



For more information on this subject scan the QR code or enter the Quick Link code **q038** at [www.euroimmun.com](http://www.euroimmun.com)

## Thyroid diseases

■ **Clinical information:** The sensitive equilibrium of the thyroid hormone loop can be disturbed due to the presence of different autoantibodies. Autoimmune thyroid diseases are characterised by antibodies against thyroid microsomes, whose main target antigen is thyroperoxidase (TPO), and antibodies against thyroglobulin (TG) or the receptor of thyrotropin (also known as thyroid stimulating hormone (TSH)). The most frequent autoimmune thyroid diseases are Hashimoto's autoimmune thyroiditis (AIT) and immunohyperthyroidism, also known as Graves' disease. While AIT can manifest as a thyroid overfunction (hyperthyroidism) or underfunction (hypothyroidism), Graves' disease is always associated with hyperthyroidism.

Hashimoto's thyroiditis leads to autoimmune-mediated lymphocytic infiltration and consequently to the destruction of the thyroid tissue, in the long term often resulting in reduced thyroid hormone production.

A special form of autoimmune thyroiditis is post-partum thyroiditis, a temporary hypothyroid functional disorder of the thyroid accompanied by high titers of anti-TPO antibodies. The disease affects around 5 to 9% of women after giving birth, and the risk is especially high in diabetes mellitus patients.

The permanent stimulation of TSH receptors by binding of autoantibodies is one of the most relevant factors for the pathogenesis of Graves' disease. The permanent binding activates signal cascades leading to an increased uptake of iodine by the thyroid. As a consequence, the thyroid hormones triiodothyronine (T3) and thyroxine (T4) are produced and secreted in larger quantities.

■ **Diagnostics:** In suspected cases of thyroid disease, the TSH concentration in serum should be determined. An increased TSH level indicates hypothyroidism, low values indicate hyperthyroidism. Additionally, the values of the free thyroid hormones FT3 or FT4 in serum should be determined. The detection of antibodies against thyroid antigens enables differentiation of autoimmune thyroid diseases from acute (bacterial) or subacute (non-infectious) thyroiditis or non-autoimmune disturbed thyroid hormone regulation.



Monkey thyroid: Aab against TPO + TG

With Hashimoto's thyroiditis, anti-TPO antibodies are detected in 90% of patients; autoantibodies against TSH receptor (TRAb) are found in 6 to 60%, and anti-TG antibodies occur in 45 to 60% of cases.


TRAb are the most important serological marker in Graves' disease. They are detectable in over 90% of patients. Higher antibody titers are associated with severe disease courses. Moreover, anti-TPO and anti-TG antibodies occur with a prevalence of approx. 80% and 30%, respectively.



For sufficient differential diagnostics, the overall picture obtained from the investigation of different parameters must be evaluated. Besides serological analyses, clinical examinations (e.g. ultrasound, scintigraphy) and symptoms must be taken into account.

## Product overview

Method	Substrate	Application	Order number	Page
IIFT	Thyroid gland, TG BIOCHIP	Detection of antibodies against TPO and TG	FA 1010-####-3	151
ELISA	TSH receptor	Non-radioactive test systems of 2 <sup>nd</sup> and 3 <sup>rd</sup> generation for the specific detection of TRAb in Graves' disease	EA 1015-9601 G	143
			EA 1015-9601-1 G	143
	Thyroglobulin (TG)	Non-radioactive test systems for diagnosis of Graves' disease and Hashimoto's thyroiditis	EA 1013-9601 G	143
Thyroid peroxidase (TPO)	EA 1012-9601 G		143	
RIA	TSH receptor	Radioactive test systems of the 2 <sup>nd</sup> generation for the specific detection of TRAb in Graves' disease	RA 1015-10001-1	150
	Thyroglobulin (TG)	Radioactive test systems for diagnosis of Graves' disease and Hashimoto's thyroiditis	RA 1013-10001-#	150
	Thyroid peroxidase (TPO)		RA 1012-#####-#	150
	Thyrotropin (TSH)	Test systems for basic evaluation of thyroid gland function	RD 1018-10001	150
	Free triiodothyronine (FT3)		RD 1016-10001	150
	Free thyroxine (FT4)		RD 1017-10001	150

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 148).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g095** at [www.euroimmun.com](http://www.euroimmun.com)



# Neurology

PNS · Autoimmune encephalitis · Other



For more information on this subject scan the QR code or enter the Quick Link code **q033** at [www.euroimmun.com](http://www.euroimmun.com)


## Paraneoplastic neurological syndromes

■ **Clinical information:** Paraneoplastic neurological syndromes (PNS) are diseases of the central and peripheral nervous system that occur in direct relation to tumour development. However, these are not caused directly by the tumour, by its metastases or by any side-effects from therapy using cytostatic drugs or radiation treatment. PNS occur in approximately 15% of malignant diseases, particularly in lung tumours.

Depending on the type of tumour, tumour cells express antigens, e.g. amphiphysin, CV2/CRMP5, PNMA2 (Ma2/Ta), Ri, Yo, Hu, ZIC4 or Tr (DNER) which can induce the formation of specific autoantibodies. These autoantibodies bind to the respective antigens localised in the nervous tissue and can thus cause neurological disorders.

In the literature two types of nomenclature are used for PNS-specific autoantibodies. One is based on the first two letters of the index patient's name (e.g. Hu for Hull, Yo for Young, Ma for Margret), the other on the initial letters of the immunohistochemical staining (ANNA = anti-nuclear neuronal antibodies). We use the nomenclature of Posner (anti-Hu, -Yo, -Ma etc.), since this is antigen-based and independent of the test procedure.

■ **Diagnostics:** In serological diagnostics, autoantibodies in PNS should always be determined using two unrelated methods. Various line blots (EUROLINE) are available in addition to indirect immunofluorescence tests with special BIOCHIP Mosaics for neurology. Thus, test results can be compared and, if necessary, confirmed. Results should only be used for diagnosis when both test results are congruent in qualitative determination and are in line with the clinical symptoms.



Primate cerebellum: Aab against Yo



## Product overview

Method	Substrate	Application	Order number	Page
IIFT	Cerebellum	Basic substrate for autoantibody detection in PNS	FA 1111-####	151
	Cerebellum, nerve, intestinal tissue	Combination of tissue substrates for further diagnostics and antibody differentiation in neurological diseases	FA 1111-####-1	151
	Cerebellum, nerve, intestinal tissue, pancreas	Neurology Mosaic with pancreas tissue for supplementary detection of antibodies against GAD	FA 1111-####-8	152
Blot	Amphiphysin, CV2, PNMA2 (Ma-2/Ta), Ri, Yo, Hu	Secondary test for the detection of the six classic paraneoplastic antibodies	DL 1111-1601-2 G	140
	Amphiphysin, CV2, PNMA2 (Ma-2/Ta), Ri, Yo, Hu, recoverin, SOX1, titin, GAD65, Zic4, Tr (DNER)	Test system for classic paraneoplastic antibodies supplemented with the antigens recoverin, SOX-1, titin, GAD65, Zic4 and Tr (DNER)	DL 1111-1601-7 G	140



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g089** at [www.euroimmun.com](http://www.euroimmun.com)



# Neurology

PNS · Autoimmune encephalitis · Other




For more information on this subject scan the QR code or enter the Quick Link code **q006** at [www.euroimmun.com](http://www.euroimmun.com)

## Autoimmune encephalitis

■ **Clinical information:** Patients with autoimmune encephalopathies exhibit autoantibodies against neuronal cell surface antigens. The antibodies are directed against glutamate receptors (type NMDA or type AMPA), GABAB receptors, DPPX, voltage-gated potassium channels (VGKC) or VGKC-associated proteins (LG11, CASPR2, TAG-1/contactin-2). Since these antigens play a direct or indirect role in synaptic signal transduction, the associated autoimmunities manifest with seizures and neuropsychiatric symptoms. The resulting conditions include special forms of autoimmune limbic encephalitis, neuromyotonia or Morvan's syndrome. These severe, potentially lethal syndromes can have a non-paraneoplastic or paraneoplastic aetiology. The frequency of underlying tumours ranges from 10 to 70%, depending on the type of antibody. The antibodies most likely play a causal role in the pathogenesis. Since appropriate therapy (immunomodulatory intervention, tumour resection) results in considerable regression of symptoms in most patients, early diagnosis is important for a favourable prognosis.

■ **Diagnostics:** The diagnosis of autoimmune encephalitis is generally based on a combination of the characteristic clinical picture, supporting findings from brain MRT, EEG and CSF analysis if necessary, and antibody determination in serum/CSF. Monospecific recombinant assays are the method of choice for serological diagnostics and can be combined with conventional immunohistochemical detection procedures. The following conditions must be excluded by differential diagnostics: infectious encephalitis (especially HSV), other autoimmune aetiologies (e.g. limbic encephalitis with autoantibodies against Hu, Ma2, CV2, amphiphysin) and clinically similar diseases of the central and/or peripheral nervous system.

A diagnostic discrimination from atypical encephalitis should also be taken into consideration. It should be taken into account that overlap syndromes and combinations of different syndromes can also occur. When a positive serological result is obtained, a comprehensive tumour investigation should be undertaken.



Transfected cells: Aab against NMDA





## Product overview

Method	Substrate	Application	Order number	Page
IIFT	Glutamate receptors (type NMDA) expressed in a human cell line	Highly sensitive mono-specific detection of NMDAR antibodies using a recombinant cell line	FA 112d-####-51	153
	GABAB receptors expressed in a human cell line	Detection of antibodies against GABAB receptors in patients with autoimmune encephalopathies	FA 112l-####-50	152
	Hippocampus, cerebellum, glutamate receptors (type NMDA) expressed in a human cell line, control-transfected cells	Combination of tissue sections for screening of antibodies against cell-surface antigens and NMDAR-transfected cells for monospecific detection of reactivity against NMDAR	FA 111m-####-3	152
	Glutamate receptors (type NMDA), glutamate receptors (type AMPA), CASPR2, LGI1, GABAB receptors, DPPX, expressed in a human cell line	BIOCHIP Mosaic for detection of differentially diagnostically relevant antibodies in autoimmune encephalopathies	FA 112d-####-6	153
	IgLON5 expressed in a human cell line	Detection of antibodies against IgLON5 in patients with atypical encephalitis and accompanying dementia	FA 1151-####-50	154
	LGI1, CASPR2 expressed in a human cell line	Detection of antibodies against LGI1 and CASPR2, the main target antigens in patients with VGKC-antibody-associated syndromes	FA 1439-####-1	151



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q056** at [www.euroimmun.com](http://www.euroimmun.com)



# Neurology

PNS · Autoimmune encephalitis · Other




For more information on this subject scan the QR code or enter the Quick Link code **q047** at [www.euroimmun.com](http://www.euroimmun.com)

## Other diseases of the central and peripheral nervous system

■ **Stiff-person syndrome:** Stiff-person syndrome (SPS) is a disease of the CNS, which manifests with progressive muscle stiffness, typically in the trunk and extremities, as well as spontaneous or triggered spasms. Up to 80% of patients show a high serum titer and intrathecal synthesis of anti-glutamic acid decarboxylase (GAD) antibodies. Around 5% of all SPS cases are paraneoplastic and usually associated with antibodies against amphiphysin.

■ **Diseases with demyelination:** These diseases are characterised by progressive destruction of the myelin sheath. The demyelinating foci are predominantly in the brain and spinal cord. The loss of myelin impairs neuronal signal transduction, leading to motor, visual and sensory disorders. These encompass neuromyelitis optica spectrum disorders (NMOSD), which affect in particular the optical nerve and the spinal cord. NMOSD is associated with pathogenic antibodies against the CNS water-channel protein aquaporin-4 (AQP-4). Antibodies against myelin oligodendrocyte glycoprotein (MOG) occur in around 20% of AQP-4-negative NMOSD patients. Antibodies against MOG also occur in other demyelinating diseases of the CNS, e.g. acute demyelinating encephalomyelitis (ADEM). The determination of anti-AQP-4 and anti-MOG antibodies enables early delimitation from multiple sclerosis, the most important differential diagnosis.



Transfected cells: Aab against AQP4

■ **Autoimmune neuropathies:** The peripheral nervous system can also be the target of autoaggression, affecting nerves, ganglia or myelin sheaths. Manifestations encompass motor paralysis, sensitivity disorders or dysautonomy. Autoantibodies against cell-membrane glycolipids or glycoproteins of neurons or glial cells are diagnostically definitive for many forms of peripheral neuropathy. Antibodies against gangliosides are characteristic markers for Guillain-Barré syndrome and its variants, for example, acute motor axonal neuropathy (GM1/ GM1b/ GD1a/ GalNac-GD1a IgG), Miller-Fisher syndrome (GQ1b/GT1a IgG), and multifocal motor neuropathy (GM1/GD1b/ asialo-GM1 IgM). Further, IgM antibodies against myelin-associated glycoprotein (MAG) typically occur in demyelinating polyneuropathy with monoclonal IgM gammopathy.

■ **Myasthenia syndrome:** In myasthenia gravis (MG) and Lambert-Eaton myasthenic syndrome (LEMS) the dominant symptom is muscle weakness, which is mainly due to antibody-mediated transmission disorders of the neuromuscular synapses. Antibodies against nicotinic acetylcholine receptors (AChR) are detected in 85 to 90% of patients with generalised MG. Additional reactivities against antigens of the striated muscle (e.g. titin) often occur in connection with neoplasia (thymoma in 15% of all myasthenia cases) and a severe disease course.



## Product overview

Method	Substrate	Application	Order number	Page
IIFT	Aquaporin-4 (AQP-4) expressed in a human cell line	Substrate for the most sensitive detection of antibodies against AQP-4	FA 1128-####-50	152
	AQP-4, myelin-oligodendrocyte glycoprotein (MOG) expressed in a human cell line	Highly specific detection of antibodies against AQP-4 and MOG	FA 1128-1	154
	Glutamic acid decarboxylase (GAD) 65kDA expressed in a human cell line	Monospecific detection of antibodies against GAD for diagnosis of stiff-person syndrome	FA 1022-####-50	151
	Nerves	Substrate for the detection of antibodies against myelinated nerves (myelin, MAG)	FA 1120-####	152
Blot	GM1, GM2, GM3, GD1a, GD1b, GT1b, GQ1b	EUROLINE for the determination of antibodies against gangliosides for the diagnosis of peripheral neuropathies	DL 1130-1601-2 G/M	127
ELISA	Acetylcholine receptor (AChR)	Sensitive and specific test for the serological diagnosis of MG	EA 1435-9601 G	143
RIA	Acetylcholine receptor (AChR)	Standard method in routine analysis for the serological diagnosis of MG	RA 1435-####-1	150
IIFT	Acetylcholine receptor (AChR)/muscle-specific kinase (MuSK) expressed in human cell lines	Highly sensitive, monospecific detection of AChR and MuSK antibodies using recombinant cell lines	FA 1435-####-2	158



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q106** at [www.euroimmun.com](http://www.euroimmun.com)



# Nephrology

Primary MN · Goodpasture's syndrome




For more information on this subject scan the QR code or enter the Quick Link code **q036** at [www.euroimmun.com](http://www.euroimmun.com)

## Primary membranous nephropathy

■ **Clinical information:** Primary membranous nephropathy (pMN), also described as primary membranous glomerulonephritis, is a chronic inflammatory disease of the glomeruli which is accompanied by a progressive impairment of the kidney function. The underlying autoimmune mechanism is based on the reaction of autoantibodies directed against the glycoproteins phospholipase A2 receptor (PLA2R) and thrombospondin type-1 domain-containing protein 7A (THSD7A). These transmembrane proteins are expressed on the surface of podocytes in human glomeruli. As a result of the binding of antibodies, the podocytes are damaged and protein enters the primary urine (proteinuria). pMN is the most frequent kidney disorder with nephrotic syndrome in adults. The disease is prevalent in all ethnic groups and genders, with men over 40 years old with white skin colour being more frequently affected. In young women with suspected pMN, lupus nephritis should be considered. Primary MN occurs very rarely in children. The primary form of MN should be discriminated from the secondary form, which can occur in infections, in drug therapy or abuse or intake of toxins, in collagenoses and other autoimmune diseases and in tumours, and which improves with treatment of the underlying disease. The treatment of pMN improves prognosis, particularly with respect to nephrotic syndrome and hypertonicity.

■ **Diagnostics:** Diagnosis of pMN is made by kidney puncture, histological examination and electron microscopy of the kidney tissue. Characteristic here is the deposition of immunocomplexes on the outside of the glomerular basement membrane. Serological diagnosis of pMN, however, is less time-consuming and less stressful for the patient. The identification and characterisation of PLA2R and THSD7A as target antigens of circulating antibodies in pMN has proven to be of major importance for non-invasive diagnostics. Autoantibodies of class IgG against PLA2R are highly specific and can be found in the serum of up to 80% of patients with pMN. In contrast, they are not exhibited by healthy blood donors or patients with secondary MN. In healthy persons and patients with secondary MN, these autoantibodies are not present. Reported prevalences for autoantibodies against THSD7A range up to 10%. Even though both antibodies can occur in parallel, anti-THSD7A antibodies are mainly found in anti-PLA2R-seronegative pMN patients. As a supplement to anti-PLA2R antibodies, anti-THSD7A antibodies are therefore another marker in the serological diagnosis of pMN. Due to their high specificity, they are equally suited for differentiation from secondary MN as anti-PLA2R antibodies.



The three methods IIFT, ELISA and ChLIA are available for the determination of autoantibodies against PLA2R. The IIFT allows qualitative to semiquantitative determination of human IgG autoantibodies against PLA2R, whilst the ELISA and ChLIA allow reliable quantification. The anti-PLA2R titer helps to assess the success of therapeutic measures. The serological finding with increase, decrease or disappearance of the antibody titer precedes the clinical image. Thus, the determination of the autoantibody titer has a high predictive value with respect to clinical remission or relapse and estimation of the risk of pMN recurrence after kidney transplantation.



The Anti-THSD7A IIFT is an ideal supplementary test to the anti-PLA2R test systems. The serological detection rate is increased with parallel determination or a two-step screening strategy in which patients with a seronegative anti-PLA2R result are additionally investigated for anti-THSD7A antibodies.

## Product overview

Method	Substrate	Application	Order number	Page
IIFT	Phospholipase A2 receptors (PLA2R) expressed in a human cell line	Transfected cells for qualitative and semiquantitative detection of anti-PLA2R and anti-THSD7A antibodies	FA 1254-####-50	156
	Thrombospondin type-1 domain-containing protein 7A (THSD7A) expressed in a human cell line		FA 1254-####-51	156
	Membranous Nephropathy Mosaic 1 (PLA2R and THSD7A)		FA 1254-####-1	156
ELISA	Phospholipase A2 receptors (PLA2R)	ELISA with purified human recombinant receptor for qualitative and quantitative detection of anti-PLA2R antibodies	EA 1254-9601 G	143
ChLIA	Phospholipase A2 receptors (PLA2R)	ChLIA with purified human recombinant receptor for qualitative and quantitative detection of anti-PLA2R antibodies	LA 1254-10010 G	147



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g088** at [www.euroimmun.com](http://www.euroimmun.com)



# Nephrology

Primary MN · Goodpasture's syndrome




For more information on this subject scan the QR code or enter the Quick Link code **q129** at [www.euroimmun.com](http://www.euroimmun.com)

## Goodpasture's syndrome

■ **Clinical information:** Glomerulonephritis (actually glomerulitis) is an inflammation of the glomeruli (kidney filters, part of the 1.2 million nephrons of each kidney). Chronic glomerulonephritis, which eventually leads to glomerulosclerosis, represents the main cause of dialysis-dependent kidney failure. In autoimmune glomerulonephritis autoantibodies are directed against the basement membrane of the kidney glomeruli (GBM antigens). Anti-GBM glomerulonephritis accounts for 0.5 to 2% of all glomerulonephritides.

Goodpasture's syndrome (pulmonary-renal syndrome) is a special form of autoimmune glomerulonephritis named after the US American pathologist Ernest William Goodpasture (1886-1960), who described the combination of glomerulonephritis with pulmonary haemorrhage in 1919. This rare syndrome affects men six times more often than women, and predominantly those in young adulthood. It is clinically characterised by the combination of rapid progressive anti-basement membrane glomerulonephritis and pulmonary haemosiderosis, whereby pulmonary haemorrhage often occurs as the first sign.

■ **Diagnostics:** The primary target antigen of all anti-GBM glomerulonephritides, including classic Goodpasture's syndrome, is the NC1 region of the alpha-3 chain of the network-structured type IV collagen of the basement membrane lamina densa. These autoantibodies, which can be detected qualitatively or quantitatively in IIFT and quantitatively in the Anti-GBM ELISA or ChLIA, can be directed against the alveolar basement membrane or against the glomerular basement membrane. In cases without lung involvement GBM antibodies are detected in the serum or plasma of over 60% of patients, in cases with lung involvement in over 90%. They are predominantly of class IgG, more rarely of class IgA and IgM. Clinical progression of the disease correlates with antibody concentration. High-titer circulating GBM antibodies indicate an unfavourable progression. With a negative serum result and continuing suspicion of anti-GBM glomerulonephritis, a kidney biopsy should be performed.



Monkey kidney: Aab against GBM


Patients with anti-GBM glomerulonephritides are often also ANCA positive (>35%). Positive results can indicate rapid-progressive glomerulonephritis or GPA. Therefore, parallel analysis of ANCA and anti-GBM antibodies is recommended in patients with ANCA-associated vasculitis (AAV) with renal involvement.





## Product overview

Method	Substrate	Application	Order number	Page
IIFT	Kidney	Standard substrate for the detection of anti-GBM autoantibodies	FA 1250-####	156
	Kidney, GBM BIOCHIPS	Anti-GBM standard substrate supplemented by a EURO-PLUS BIOCHIP with purified GBM antigen	FA 1250-####-1	156
	Granulocytes (EOH)/ HEp-2 + granulocytes (EOH)/ granulocytes (HCHO)/ PR3/MPO/GBM/ BIOCHIPS	ANCA screening and confirmation on monospecific EUROPLUS antigen dots (incl. GBM) in one test system	FA 1201-####-25	155
ELISA	Glomerular basement membrane (GBM)	ELISA with purified alpha-3 chain of type IV collagen for qualitative and quantitative detection of anti-GBM antibodies	EA 1251-9601 G	143
Blot	MPO, PR3, GBM	Immunoblot for multiplex detection of ANCA and anti-GBM antibodies	DL 1200-####-3 G	140
ChLIA	GBM (purified alpha-3 chain of type IV collagen)	Qualitative and quantitative detection of anti-GBM antibodies	LA 1251-10010 G	147

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 148).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q068** at [www.euroimmun.com](http://www.euroimmun.com)



# Dermatology

## Autoimmune dermatoses




For more information on this subject scan the QR code or enter the Quick Link code **q005** at [www.euroimmun.com](http://www.euroimmun.com)

## Autoimmune dermatoses

■ **Clinical information:** Bullous autoimmune dermatoses are rare, blister-forming diseases of the outer skin and the adjacent mucous membranes. They are characterised by the formation of autoantibodies against structural proteins of the skin. These structural proteins establish the cell-to-cell contact in keratinocytes within the epidermis and the adhesion of the epidermis to the dermis. Bullous autoimmune dermatoses are divided into four main groups based on their target antigens and the localisation of the blisters:

- Pemphigus diseases: desmoglein 1 (Dsg1), desmoglein 3 (Dsg3), different plakins (mostly envoplakin)
- Pemphigoid diseases: BP180, BP230, laminin 332
- Epidermolysis bullosa acquisita: collagen type VII
- Dermatitis herpetiformis: endomysium (tissue/epidermal transglutaminase), deamidated gliadin peptides (GAF-3X)

■ **Diagnostics:** A conclusive diagnosis of bullous autoimmune dermatoses requires the detection of both tissue-bound autoantibodies by direct immunofluorescence and circulating autoantibodies. The circulating specific autoantibodies against epidermal antigens (prickle cell desmosomes and epidermal basement membrane) in patient serum are detected using the indirect immunofluorescence test (IIFT) with tissue sections of primary oesophagus. For further differentiation of autoantibodies against basement membrane structures, tissue sections of primate salt-split skin are used. Final diagnosis is based on a combination of the clinical picture with the detection of autoantibodies against the individual target antigens using IIFT and monospecific ELISAs.



Monkey oesophagus: Aab against epid. BM

Patients who suffer from bullous pemphigoid (BP) exhibit autoantibodies against BP180 and frequently also against BP230. The serum level of autoantibodies against BP180 correlates with the disease activity of BP, the serum level of autoantibodies against BP230 with the duration of the disease. Autoantibodies against desmoglein 1 and 3 are markers for pemphigus diseases. IIFT has proven valuable for detecting circulating autoantibodies in pemphigus. ELISA using recombinant desmoglein 1 and 3 offer the same sensitivity and specificity as IIFT. The anti-Dsg1 and -Dsg3 antibody levels measured correlate to a large extent with the severity and activity of the disease and the therapy success. The determination of autoantibodies against envoplakin contributes to diagnosis of PNP as well as differential diagnostic clarification. The determination of autoantibodies against collagen type VII confirms the diagnosis of EBA and enables the delimitation from other bullous autoimmune dermatoses.



## Product overview

Method	Substrate	Application	Order number	Page
IIFT	Oesophagus	Substrate for detection of circulating Ab in bullous autoimmune dermatoses	FA 1501-####	158
	Oesophagus, salt-split skin	Salt-split skin enables autoantibody specification in pemphigoid diseases	FA 1501-####-20	159
	Oesophagus, salt-split skin, BP230gC-transfected cells, desmoglein-1-transfected cells, desmoglein-3-transfected cells, BP180-NC16A-4X BIOCHIP	The combination of all substrates enables fast and comprehensive investigation in one step	FA 1501-####-7	153
	Laminin-332-transfected cells	Determination of Ab against laminin-332 for diagnosis of mucous pemphigoid	FA 150b-1005-50	159
ELISA	Desmoglein 1	Detection of Ab against Dsg1	EA 1495-4801 G	143
	Desmoglein 3	Detection of Ab against Dsg3	EA 1496-4801 G	143
	BP180-NC16A-4X	ELISA for the most important antibody parameter in BP	EA 1502-4801-2 G	144
	BP230-CF	Supplementary serological parameter for diagnosis of BP	EA 1502-4801-1 G	144
	Envoplakin	Monospecific detection of Ab against envoplakin	EA 1491-4801 G	143
	Collagen type VII	Monospecific detection of Ab against collagen type VII	EA 1947-4801 G	145
	Dermatology Profile (separate: BP180-NC16A-4X, BP230-CF, desmoglein 1, desmoglein 3, envoplakin, collagen type VII)	Simultaneous detection of the six most important Ab in one test	EA 1490-1208-1 G	143



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g054** at [www.euroimmun.com](http://www.euroimmun.com)



# Products for autoimmune diagnostics





### Format

- 1601: 16 single test strips
- 1208: 12 microplate strips with 8 wells each
- 9601: 96 individual break-apart wells (12 microplate strips, 8 wells each)
- 5001: 50 individual tubes
- 10001: 100 individual tubes
- 1003: 10 slides with 3 fields each
- 1005: 10 slides with 5 fields each
- 2005: 20 slides with 5 fields each
- 1010: 10 slides with 10 fields each
- 1050: 10 slides with 50 fields each
- 1001: 10 slides to be incubated with 1 patient serum each
- 1002: 10 slides to be incubated with 2 patient sera each

**FA** **1914** - **1005** **-1** **A**

### Product code

### Immunoglobulin class

- A: IgA
- G: IgG
- M: IgM
- O: IgGM
- P: Polyvalent (IgAGM)

### Product classification

- CL: Control for EUROLINE (autoimmune diagnostics) ..... page 138
- DA: Test system EUROASSAY (autoimmune diagnostics) ..... page 139
- DL: Test system EUROLINE (autoimmune diagnostics) ..... page 140
- EA: Test system microplate ELISA (autoimmune diagnostics) ..... page 143
- EV: Test system microplate ELISA (determination of further antibodies) ..... page 146
- ED: Test system microplate ELISA therapeutic drug monitoring) ..... page 146
- LA: Test system chemiluminescence test (autoimmune diagnostics) ..... page 147
- LR: Control set chemiluminescence test ..... page 147
- Test system **ids** chemiluminescence test (autoimmune diagnostics) ..... page 148
- Control set **ids** chemiluminescence test (autoimmune diagnostics) ..... page 149
- RA: Radioimmunoassay (autoimmune diagnostics) ..... page 150
- RD: Radioimmunoassay (direct detection of autoantigens, hormone determination) ..... page 150
- FA: Test system indirect immunofluorescence (autoimmune diagnostics) ..... page 151
- FB: Single slides indirect immunofluorescence (autoimmune diagnostics) ..... page 151
- FC: Test system indirect immunofluorescence (EUROPattern) ..... page 151
- FW: Single slides indirect immunofluorescence (EUROPattern) ..... page 151
- FV: Test system indirect immunofluorescence (determination of further antibodies) ..... page 165
- FX: Single slides indirect immunofluorescence (determination of further antibodies) ..... page 165

For product orders the amount, product code and test name are required. **Test kits** comprise all reagents needed to perform the serological investigation. For diagnostics in indirect immunofluorescence, for example, these include slides, FITC-labelled antibodies against human immunoglobulin, positive and negative control sera (not available for some products) as well as embedding medium, cover glasses, sachets of PBS and Tween 20.

Substrates consisting of cell cultures and tissues which do not appear in this catalogue can be made to specification. In addition, BIOCHIP mosaics can be produced according to individual requirements. Apart from the customary package sizes and slide formats, special sizes are available as well. Quotations can be provided upon request.



## Controls for EUROLINE: Autoantibodies

Order No.	Control (Ready for Use)	Ig Class	Format
CL 1000-0101 Z	autoantibody-free control (aab negative)	IgA, IgG, IgM	0.1 ml
CL 1111-0107 G	positive control serum: IgG, human, 100x concentrated for DL 1111-1 G, DL 1111-2 G, DL 1111-4 G and DL 1111-7 G	IgG	0.1 ml for EUROBlotOne
CL 1111-0107-6 G	positive control serum: IgG, human, 100x concentrated for DL 1111-6 G	IgG	0.1 ml for EUROBlotOne
CL 1200-0107-2 G	positive control serum: IgG, human, 100x concentrated for DL 1200-X G	IgG	0.1 ml for EUROBlotOne
CL 1300-0107 G	positive control serum: IgG, human, 100x concentrated for DL 1300-X G	IgG	0.1 ml for EUROBlotOne
CL 1530-0107 G	positive control serum: IgG, human, 100x concentrated for DL 1530-X G	IgG	0.1 ml for EUROBlotOne
CL 1532-0107 G	positive control serum: IgG, human, 100x concentrated for DL 1532 G	IgG	0.1 ml for EUROBlotOne
CL 1590-0107 G	positive control serum: IgG, human, 100x concentrated for DL 1590-X G	IgG	0.1 ml for EUROBlotOne
CL 1590-0107-35 G	positive control serum: IgG, human, 100x concentrated for DL 1590-35 G	IgG	0.1 ml for EUROBlotOne
CL 159z-0107 G	positive control serum: IgG, human, 100x concentrated for DL 159z-X G	IgG	0.1 ml for EUROBlotOne
CL 1910-0107 A	positive control serum: IgA, human, 100x concentrated for DL 1910 A	IgA	0.1 ml for EUROBlotOne
CL 1910-0107 G	positive control serum: IgG, human, 100x concentrated for DL 1910 G	IgG	0.1 ml for EUROBlotOne





<b>EUROASSAY for the Determination of Autoantibodies (Test Systems)</b>				
Order No.	Antibodies against	Ig Class	Substrate	Format Slides x Fields
DA 1300-1003 G	AMA M2, LKM-1, SLA/LP	IgG	EUROASSAY strip with antigens	10 x 03
DA 1300-1003-2 G	LKM-1, LC-1, SLA/LP	IgG	EUROASSAY strip with antigens	10 x 03
DA 1300-1003-3 G	Liver Profile AMA M2, LKM-1, LC-1, SLA/LP	IgG	EUROASSAY strip with antigens	10 x 03
DA 1302-1003 G	SLA/LP	IgG	EUROASSAY strip with antigens	10 x 03
DA 1590-1003-1 G DA 1590-1005-1 G	Anti-ENA ProfilePlus (nRNP/Sm, Sm, SS-A, SS-B, Scl-70, Jo-1 separately)	IgG	EUROASSAY strip with antigens	10 x 03 10 x 05
DA 1590-1003-2 G	Anti-ENA ProfilePlus with AMA M2 (nRNP/Sm, Sm, SS-A, SS-B, Scl-70, Jo-1, AMA M2 separately)	IgG	EUROASSAY strip with antigens	10 x 03
DA 1590-1005-20 G	Anti-ENA ProfilePlus with histones (nRNP/Sm, Sm, SS-A, SS-B, Scl-70, Jo-1, histones separately)	IgG	EUROASSAY strip with antigens	10 x 05
DA 1590-1003-29 G DA 1590-1005-29 G	Anti-ENA ProfilePlus with Ro-52 (nRNP/Sm, Sm, SS-A, SS-B, Scl-70, Jo-1, Ro-52 separately)	IgG	EUROASSAY strip with antigens	10 x 03 10 x 05
DA 1590-1005-32 G	Anti-ENA ProfilePlus with ribosomal P-proteins (nRNP/Sm, Sm, SS-A, SS-B, Scl-70, Jo-1, ribosomal P-proteins separately)	IgG	EUROASSAY strip with antigens	10 x 05
DA 1620-1003-1 O	AMA Profile (AMA M2, M4, M9 separately)	IgGM	EUROASSAY strip with antigens	10 x 03



## EUROLINE for the Determination of Autoantibodies (Test Systems)

Order No.	Antibodies against	Ig Class	Substrate	Format
DL 0160-1601 G DL 0160-5001 G	EUROLINE validation	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ
DL 1111-1601-2 G	Neuronal Antigens Profile 2 (amphiphysin, CV2, PNMA2 (Ma-2/Ta), Ri, Yo, Hu separately)	IgG	EUROLINE	16 strips
DL 1111-1601-4 G	Neuronal Antigens Profile PLUS RST (amphiphysin, CV2, PNMA2 (Ma-2/Ta), Ri, Yo, Hu, recoverin, SOX1, titin separately)	IgG	EUROLINE	16 strips
DL 1111-1601-6 G	Neuronal Antigens Profile SOX1, titin	IgG	EUROLINE	16 strips
DL 1111-1601-7 G DL 1111-5001-7 G DL 1111-6401-7 G	Paraneoplastic Neurologic Syndromes - 12 Ag (amphiphysin, CV2, PNMA2 (Ma-2/Ta), Ri, Yo, Hu, recoverin, SOX1, titin, Zic4, GAD65, Tr (DNER) separately)	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips
DL 1130-1601-1 G	Gangliosides Profile 1 (GM1, GD1b, GQ1b separately)	IgG	EUROLINE	16 strips
DL 1130-1601-1 M	Gangliosides Profile 1 (GM1, GD1b, GQ1b separately)	IgM	EUROLINE	16 strips
DL 1130-1601-2 G	Gangliosides Profile 2 (GM1, GM2, GM3, GD1a, GD1b, GT1b, GQ1b separately)	IgG	EUROLINE	16 strips
DL 1130-1601-2 M	Gangliosides Profile 2 (GM1, GM2, GM3, GD1a, GD1b, GT1b, GQ1b separately)	IgM	EUROLINE	16 strips
DL 1200-1601-2 G DL 1200-6401-2 G	myeloperoxidase (MPO) proteinase 3 (PR3)	IgG	EUROLINE	16 strips 64 strips
DL 1200-1601-3 G DL 1200-6401-3 G	myeloperoxidase (MPO) proteinase 3 (PR3) glomerular basement membrane (GBM)	IgG	EUROLINE	16 strips 64 strips
DL 1300-1601-2 G DL 1300-6401-2 G	Liver Profile 2 (AMA M2, M2-3E, LKM-1, LC-1, SLA/LP separately)	IgG	EUROLINE	16 strips 64 strips
DL 1300-1601-3 G DL 1300-6401-3 G	Liver Profile (AMA M2, LKM-1, LC-1, SLA/LP separately)	IgG	EUROLINE	16 strips 64 strips
DL 1300-1601-4 G DL 1300-5001-4 G DL 1300-6401-4 G	Autoimmune Liver Diseases (AMA M2, M2-3E, Sp100, PML, gp210, LKM-1, LC-1, SLA/LP, Ro-52 separately)	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips
DL 1300-1601-5 G	Autoimmune Liver Diseases 14 Ag (AMA-M2, M2-3E, Sp100, PML, gp210, LKM-1, LC-1, SLA/LP, SS-A, Ro-52, Scl-70, CENP A, CENP B, PGDH separately)	IgG	EUROLINE	16 strips
DL 1360-1601 A DL 1360-0510 A DL 1360-6401 A	Autoimmune Gastrointestinal Diseases IgA (tissue transglutaminase (endomysium), gliadin-analogue fusion peptide (GAF-3X), mannan (ASCA))	IgA	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips
DL 1360-1601 G DL 1360-5001 G DL 1360-6401 G	Autoimmune Gastrointestinal Diseases IgG (tissue transglutaminase (endomysium), gliadin-analogue fusion peptide (GAF-3X), parietal cell antigen (PCA) separately Intrinsic factor, mannan (ASCA))	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips



EUROLINE for the Determination of Autoantibodies (Test Systems)				
Order No.	Antibodies against	Ig Class	Substrate	Format
DL 1530-1601 G	<b>Myositis Profile</b> (Mi-2, Ku, PM-Scl, Jo-1, PL-7, PL-12, Ro-52 separately)	IgG	EUROLINE	16 strips
DL 1530-1601-3 G DL 1530-6401-3 G	<b>Myositis Profile 3</b> (Mi-2, Ku, PM-Scl100, PM-Scl75, Jo-1, SRP, PL-7, PL-12, EJ, OJ, Ro-52 separately)	IgG	EUROLINE	16 strips 64 strips
DL 1530-1601-4 G DL 1530-5001-4 G DL 1530-6401-4 G	<b>Autoimmune Inflammatory Myopathies 16 Ag</b> (Mi-2 alpha, Mi-2 beta, TIF1g, MDA5, NXP2, SAE1, Ku, PM-Scl100, PM-Scl75, Jo-1, SRP, PL-7, PL-12, EJ, OJ, Ro-52 separately)	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips
DL 1530-1601-7 G DL 1530-5001-7 G DL 1530-6401-7 G	<b>Autoimmune Inflammatory Myopathies 16 Ag et cN-1A</b> (Mi-2 alpha, Mi-2 beta, TIF1g, MDA5, NXP2, SAE1, Ku, PM-Scl100, PM-Scl75, Jo-1, SRP, PL-7, PL-12, EJ, OJ, Ro-52, cN-1A separately)	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips
DL 1532-1601 G DL 1532-5001 G DL 1532-6401 G	<b>Systemic Sclerosis Profile (Nucleoli)</b> (Scl-70, CENP A, CENP B, RP11, RP155, fibrillar, NOR90, Th/To, PM-Scl100, PM-Scl75, Ku, PDGFR, Ro-52 separately)	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips
DL 1590-1601-1 G DL 1590-6401-1 G	<b>Anti-ENA ProfilePlus 1</b> (nRNP/Sm, Sm, SS-A, Ro-52, SS-B, Scl-70, Jo-1 separately)	IgG	EUROLINE	16 strips 64 strips
DL 1590-1601-3 G DL 1590-5001-3 G DL 1590-6401-3 G	<b>ANA Profile 3</b> (nRNP/Sm, Sm, SS-A, Ro-52, SS-B, Scl-70, PM-Scl, Jo-1, CENP B, PCNA, dsDNA, nucleosomes, histones, ribosomal P-proteins, AMA M2 separately)	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips
DL 1590-1601-5 G DL 1590-6401-5 G	<b>ANA Profile 5</b> (nRNP/Sm, Sm, RNP70, RNPA, RNPC, SS-A, Ro-52, SS-B, Scl-70, PM-Scl, Jo-1, CENP B, PCNA, dsDNA, nucleosomes, histones, ribosomal P-proteins, AMA M2 separately)	IgG	EUROLINE	16 strips 64 strips
DL 1590-1601-8 G DL 1590-5001-8 G DL 1590-6401-8 G	<b>ANA Profile 1</b> (nRNP/Sm, Sm, SS-A, Ro-52, SS-B, Scl-70, Jo-1, CENP B, dsDNA, nucleosomes, histones, ribosomal P-proteins separately)	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips
DL 1590-1601-23 G DL 1590-5001-23 G DL 1590-6401-23 G	<b>ANA Profile 23</b> (nucleosomes, dsDNA, histones, SS-A, Ro-52, SS-B, nRNP/Sm, Sm, Mi-2 alpha, Mi-2 beta, Ku, CENP A, CENP B, Sp100, PML, Scl-70, PM-Scl100, PM-Scl75, RP11, RP155, gp210, PCNA, DFS70 separately)	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips
DL 1590-1601-30 G DL 1590-5001-30 G DL 1590-6401-30 G	<b>ANA Profile 3 plus DFS70</b> (nRNP/Sm, Sm, SS-A, Ro-52, SS-B, Scl-70, PM-Scl, Jo-1, CENP B, PCNA, dsDNA, nucleosomes, histones, ribosomal P-proteins, AMA M2, DFS70 separately)	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips
DL 1590-1601-31 G DL 1590-6401-31 G	<b>ANA Profile et Mi-2 et Ku</b> (Mi-2, Ku, nRNP/Sm, Sm, SS-A, Ro-52, SS-B, Scl-70, PM-Scl, Jo-1, CENP B, PCNA, dsDNA, nucleosomes, histones, ribosomal P-proteins, AMA M2 separately)	IgG	EUROLINE	16 strips 64 strips
DL 1590-1601-32 G DL 1590-5001-32 G	<b>dsDNA, nucleosomes, histones, DFS70</b>	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ
DL 1590-1601-33 G DL 1590-5001-33 G DL 1590-6401-33 G	<b>ANA Profile et Mi-2, Ku, DFS70</b> (Mi-2, Ku, nRNP/Sm, Sm, SS-A, Ro-52, SS-B, Scl-70, PM-Scl100, Jo-1, CENP B, PCNA, dsDNA, nucleosomes, histones, ribosomal P-proteins, AMA M2, DFS70 separately)	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips



## EUROLINE for the Determination of Autoantibodies (Test Systems)

Order No.	Antibodies against	Ig Class	Substrate	Format
DL 1590-1601-34 G DL 1590-6401-34 G	Mi2 alpha, Mi2 beta, Ku, DFS70	IgG	EUROLINE	16 strips 64 strips
DL 1590-1601-35 G DL 1590-5001-35 G DL 1590-6401-35 G	Cytoplasm profile (AMA M2, M2-3E, ribosomal P-proteins, Jo-1 SRP, PL-7, PL-12, EJ, OJ, Ro-52 separately)	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips
DL 159z-1601 G DL 159z-5001 G	EUROLINE Anti-DFS70	IgG	EUROLINE	16 strips 50 strips for Immunoblot PreQ
DL 1620-1601-1 O DL 1620-6401-1 O	AMA-Profile EUROLINE (separate: AMA-M2, M2-3E, M4, M9)	IgGM	EUROLINE	16 strips 64 strips
DL 1910-1601 A	Coeliac Disease Profile (tissue transglutaminase (endomysium), gliadin-analogue fusion peptide (GAF-3X) separately)	IgA	EUROLINE	16 strips
DL 1910-1601 G	Coeliac Disease Profile (tissue transglutaminase (endomysium), gliadin-analogue fusion peptide (GAF-3X) separately)	IgG	EUROLINE	16 strips



Microplate ELISA for the Determination of Autoantibodies (Test Systems)				
Order No.	Antibodies against	Ig Class	Calibration	Format
EA 1012-9601 G	thyroid peroxidase (TPO)	IgG	10/50/500 IU/ml	96 x 01
EA 1013-9601 G	thyroglobulin (TG)	IgG	20/100/1000 IU/ml	96 x 01
EA 1015-9601 G	TSH receptor (thyrotropin receptor)	IgG	0/1/2/8/40 IU/l	96 x 01
EA 1015-9601-1 G	TSH receptor (thyrotropin receptor) Fast ELISA	IgG	0.1/1/2/8/40 IU/l	96 x 01
EA 1022-9601 G	GAD	IgG	5/15/35/120/250/2000 IU/ml	96 x 01
EA 1022-9601-1 G	GAD/IA2 Pool	IgG	4/10/20/70/145/450 IU/ml	96 x 01
EA 1023-9601 G	IA2	IgG	10/20/75/250/400/4000 IU/ml	96 x 01
EA 1027-9601	zinc transporter 8		10/20/75/500/2000 RU/ml	96 x 01
EA 1200-1208-1 G	ANCA Profile (proteinase 3, MPO, elastase, cathepsin G, BPI, lactoferrin separately)	IgG	semi-quantitative	12 x 08
EA 1201-9601-2 G	cANCA: proteinase 3 (PR3-hn-hr)	IgG	2/20/200 RU/ml	96 x 01
EA 1211-9601 G	pANCA: myeloperoxidase (MPO)	IgG	2/20/200 RU/ml	96 x 01
EA 1251-9601 G	glomerular basement membrane (GBM)	IgG	2/20/200 RU/ml	96 x 01
EA 1254-9601 G	phospholipase A2 receptor (PLA2R)	IgG	2/20/100/500/1500 RU/ml	96 x 01
EA 1302-9601 G	soluble liver antigen/ liver-pancreas antigen (SLA/LP)	IgG	2/20/200 RU/ml	96 x 01
EA 1307-9601 G	cytosolic liver antigen type 1 (LC-1)	IgG	semi-quantitative	96 x 01
EA 1321-9601 G	liver-kidney microsomes (LKM-1)	IgG	2/20/200 RU/ml	96 x 01
EA 1361-9601 G	parietal cells (PCA)	IgG	2/20/200 RU/ml	96 x 01
EA 1361-9601-1 G	ATP4B	IgG	2/20/200 RU/ml	96 x 01
EA 1362-9601 G	intrinsic factor	IgG	2/20/200 RU/ml	96 x 01
EA 1435-9601 G	acetylcholine receptor	IgG	0/0.25/0.75/2.5/8 nmol/l	96 x 01
EA 1490-1208-1 G	Dermatology Profile (BP180-NC16A-4X, BP230-CF, desmoglein 1, desmoglein 3, envoplakin, collagen type VII separately)	IgG	semi-quantitative	12 x 08
EA 1491-4801 G	envoplakin	IgG	semi-quantitative	48 x 01
EA 1495-4801 G	desmoglein 1	IgG	2/20/200 RU/ml	48 x 01
EA 1496-4801 G	desmoglein 3	IgG	2/20/200 RU/ml	48 x 01


**Microplate ELISA for the Determination of Autoantibodies (Test Systems)**

Order No.	Antibodies against	Ig Class	Calibration	Format
EA 1502-4801-1 G	BP230-CF	IgG	2/20/200 RU/ml	48 x 01
EA 1502-4801-2 G	BP180-NC16A-4X	IgG	2/20/200 RU/ml	48 x 01
EA 1505-9601 G	cyclic citrullinated peptides (CCP)	IgG	1/5/20/100/200 RU/ml	96 x 01
EA 151a-4802 G	Sa	IgG	2/20/200 RU/ml	48 x 02
EA 151b-9601 G	CEP-1	IgG	2/20/200 RU/ml	96 x 01
EA 1560-9601 G	histones	IgG	2/20/200 RU/ml	96 x 01
EA 1571-9601 G	double-stranded DNA (dsDNA)	IgG	10/100/800 IU/ml	96 x 01
EA 1572-9601 G	dsDNA-NcX	IgG	10/100/800 IU/ml	96 x 01
EA 1574-9601 G	nucleosomes	IgG	2/20/200 RU/ml	96 x 01
EA 1576-9601 G	single-stranded DNA (ssDNA)	IgG	2/20/200 RU/ml	96 x 01
EA 1584-9601 G	PM-Scl	IgG	2/20/200 RU/ml	96 x 01
EA 1590-1208-1 G	Anti-ENA ProfilePlus 1 (nRNP/Sm, Sm, SS-A, SS-B, Scl-70, Jo-1 separately)	IgG	semi-quantitative	12 x 08
EA 1590-1208-2 G	Anti-ENA ProfilePlus 2 (ribosomal P-proteins, nRNP/Sm, Sm, SS-A, SS-B, Scl-70, Jo-1, centromeres, separately)	IgG	semi-quantitative	12 x 08
EA 1590-9601-7 G	Anti-ENA PoolPlus (antigen mixture: nRNP/Sm, Sm, SS-A, SS-B, Scl-70, Jo-1)	IgG	semi-quantitative	96 x 01
EA 1590-9601-8 G	ANA screen (antigen mixture: dsDNA, histones, ribosomal P-proteins, nRNP/Sm, Sm, SS-A, SS-B, Scl-70, Jo-1, centromeres)	IgG	semi-quantitative	96 x 01
EA 1590-9601-9 G	Anti-ENA Pool (antigen mixture: nRNP/Sm, Sm, SS-A, SS-B, Scl-70, ribosomal P-proteins, Ro-52)	IgG	semi-quantitative	96 x 01
EA 1590-9601-11 G	ANA screen 11 (antigen mixture: PCNA, PM-Scl, ribosomal P-proteins, nRNP/Sm, Sm, SS-A, Ro-52, SS-B, Scl-70, Jo-1, centromeres)	IgG	semi-quantitative	96 x 01
EA 1590-1208-12 G	Anti-ENA SLE Profile 2 (dsDNA, histones, nucleosomes, nRNP/Sm, Sm, SS-A, SS-B, Scl-70 separately)	IgG	semi-quantitative	12 x 08
EA 1590-9601-14 G	ANA screen 9 (antigen mixture: PCNA, PM-Scl, ribosomal P-proteins, nRNP/Sm, Sm, SS-A, SS-B, Scl-70, Jo-1)	IgG	semi-quantitative	96 x 01
EA 1591-9601 G	nRNP/Sm	IgG	2/20/200 RU/ml	96 x 01
EA 1593-9601 G	Sm	IgG	2/20/200 RU/ml	96 x 01
EA 1595-9601 G	SS-A (Ro)	IgG	2/20/200 RU/ml	96 x 01
EA 1597-9601 G	SS-B (La)	IgG	2/20/200 RU/ml	96 x 01
EA 1599-9601 G	Scl-70	IgG	2/20/200 RU/ml	96 x 01
EA 159z-9601 G	DFS70	IgG	semi-quantitative	96 x 01
EA 1611-9601 G	centromeres	IgG	2/20/200 RU/ml	96 x 01





Microplate ELISA for the Determination of Autoantibodies (Test Systems)				
Order No.	Antibodies against	Ig Class	Calibration	Format
EA 1621-9601 A	cardiolipin (AMA M1)	IgA	2/12/120 PL IgA U/ml	96 x 01
EA 1621-9601 G	cardiolipin (AMA M1)	IgG	2/12/120 PL IgG U/ml	96 x 01
EA 1621-9601 M	cardiolipin (AMA M1)	IgM	2/12/120 PL IgM U/ml	96 x 01
EA 1621-9601 P	cardiolipin (AMA M1)	IgAGM	2/12/120 RU/ml	96 x 01
EA 1622-9601 G	AMA M2-3E	IgG	2/20/200 RU/ml	96 x 01
EA 162a-9601 A	phosphatidylserine	IgA	2/12/120 RU/ml	96 x 01
EA 162a-9601 G	phosphatidylserine	IgG	2/12/120 RU/ml	96 x 01
EA 162a-9601 M	phosphatidylserine	IgM	2/12/120 RU/ml	96 x 01
EA 162a-9601 P	phosphatidylserine	IgAGM	2/12/120 RU/ml	96 x 01
EA 1632-9601 A	$\beta$ 2-glycoprotein 1	IgA	2/20/200 RU/ml	96 x 01
EA 1632-9601 G	$\beta$ 2-glycoprotein 1	IgG	2/20/200 RU/ml	96 x 01
EA 1632-9601 M	$\beta$ 2-glycoprotein 1	IgM	2/20/200 RU/ml	96 x 01
EA 1632-9601 P	$\beta$ 2-glycoprotein 1	IgAGM	2/20/200 RU/ml	96 x 01
EA 1641-9601 G	ribosomal P-proteins	IgG	2/20/200 RU/ml	96 x 01
EA 1661-9601 G	Jo-1	IgG	2/20/200 RU/ml	96 x 01
EA 1675-4801 G	cN-1A (Mup44, NT5C1A)	IgG	semi-quantitative	48 x 01
EA 1814-9601 A	IgA rheumatoid factor (ab of class IgA against IgG)	IgA	2/20/200 RU/ml	96 x 01
EA 1814-9601 G	IgG rheumatoid factor (ab of class IgG against IgG)	IgG	2/20/200 RU/ml	96 x 01
EA 1814-9601 M	IgM rheumatoid factor (ab of class IgM against IgG)	IgM	2/20/200 RU/ml	96 x 01
EA 1818-9601 G	circulating immune complexes (CIC)	IgG	2/20/200 RU/ml	96 x 01
EA 1910-9601 A	tissue transglutaminase (endomysium)	IgA	2/20/200 RU/ml	96 x 01
EA 1910-9601 G	tissue transglutaminase (endomysium)	IgG	semi-quantitative	96 x 01
EA 1947-4801 G	collagen type VII	IgG	2/20/200 RU/ml	48 x 01



### Microplate ELISA for the Determination of Antibodies against Other Antigens (Test Systems)

Order No.	Antibodies against	Ig Class	Calibration	Format
EV 2841-9601 A	<b>Saccharomyces cerevisiae</b>	IgA	2/20/200 RU/ml	96 x 01
EV 2841-9601 G	<b>Saccharomyces cerevisiae</b>	IgG	2/20/200 RU/ml	96 x 01
EV 3011-9601 A	<b>gliadin (GAF-3X)</b>	IgA	2/25/200 RU/ml	96 x 01
EV 3011-9601 G	<b>gliadin (GAF-3X)</b>	IgG	2/25/200 RU/ml	96 x 01
EV 3840-9601 E	<b>total IgE</b>	IgE	0/10/100/500 IU/ml	96 x 01

### Microplate ELISA for Therapeutic Drug Monitoring (Test Systems)

Order No.	Antibodies against	Ig Class	Format
ED 4110-9601	<b>MabTrack level adalimumab</b>		96 x 01
ED 4111-4801 G	<b>MabTrack anti-drug antibody adalimumab</b>	IgG	48 x 01
ED 4120-9601	<b>MabTrack level infliximab</b>		96 x 01
ED 4121-4801 G	<b>MabTrack anti-drug antibody infliximab</b>	IgG	48 x 01



### Chemiluminescence Tests for the Determination of Autoantibodies (Test Systems)

Order No.	Antibodies against	Ig Class	Calibration	Format
LA 1201-10010 G	proteinase 3 (PR3)	IgG	quantitative	100 determinations for RA Analyzer 10
LA 1211-10010 G	MPO	IgG	quantitative	100 determinations for RA Analyzer 10
LA 1251-10010 G	GBM	IgG	quantitative	100 determinations for RA Analyzer 10
LA 1254-10010 G	phospholipase A2 receptor (PLA2R)	IgG	quantitative	100 determinations for RA Analyzer 10
LA 1505-10010 G	CCP	IgG	quantitative	100 determinations for RA Analyzer 10
LA 1910-10010 A	tissue transglutaminase (endomysium)	IgA	quantitative	100 determinations for RA Analyzer 10
LA 1910-10010 G	tissue transglutaminase (endomysium)	IgG	quantitative	100 determinations for RA Analyzer 10
LV 3011-10010 A	Gliadin (GAF-3X)	IgA	quantitative	100 determinations for RA Analyzer 10
LV 3011-10010 G	Gliadin (GAF-3X)	IgG	quantitative	100 determinations for RA Analyzer 10

### Control Sets for Chemiluminescence Tests

Order No.	Control Set (Ready for use)	Ig Class	Format
LR 1201-20210 G	Control set Proteinase 3 (PR3)	IgG	2 x 0.4 ml control QC1/2
LR 1211-20210 G	Control set MPO	IgG	2 x 0.4 ml control QC1/2
LR 1251-20210 G	Control set GBM	IgG	2 x 0.4 ml control QC1/2
LR 1254-20210 G	Control set phospholipase A2 receptor (PLA2R)	IgG	2 x 0.4 ml control QC1/2
LR 1505-20210 G	Control set CCP	IgG	2 x 0.4 ml control QC1/2
LR 1910-20210 A	Control set Human Tissue Transglutaminase (tTG)	IgA	2 x 0.4 ml control QC1/2
LR 1910-20210 G	Control set Human Tissue Transglutaminase (tTG)	IgG	2 x 0.4 ml control QC1/2
LR 3011-20210 A	Control set Gliadin (GAF-3X)	IgA	2 x 0,4 ml control QC1/2
LR 3011-20210 G	Control set Gliadin (GAF-3X)	IgG	twice each 0,4 ml control QC1/2


**IDS Chemiluminescence Tests for the Determination of Autoantibodies (Test Systems)**

IDS Order No.	Description	Format
IS-AI1902	IDS Anti-TPO	100 determinations, calibrators incl.
IS-AI1901	IDS Anti-TG	100 determinations, calibrators incl.
IS-AI1702II	IDS PR3-II	50 determinations, calibrators incl.
IS-AI1701	IDS MPO	50 determinations, calibrators incl.
IS-AI1703	IDS GBM	50 determinations, calibrators incl.
IS-AI1802	IDS LKM-1	50 determinations, calibrators incl.
IS-AI1201	IDS CCP	100 determinations, calibrators incl.
IS-AI1101	IDS dsDNA IgG	100 determinations, calibrators incl.
IS-AI1002	IDS ENA Screen	100 determinations, calibrators incl.
IS-AI1001	IDS ANA Screen	100 determinations, calibrators incl.
IS-AI1107	IDS U1-snRNP	50 determinations, calibrators incl.
IS-AI1106	IDS Sm	50 determinations, calibrators incl.
IS-AI1102	IDS SS-A/Ro	50 determinations, calibrators incl.
IS-AI1103	IDS SS-A/Ro 52 kDa	50 determinations, calibrators incl.
IS-AI1104	IDS SS-A/Ro 60 kDa	50 determinations, calibrators incl.
IS-AI1105	IDS SS-B/La	50 determinations, calibrators incl.
IS-AI1108	IDS Scl-70	50 determinations, calibrators incl.
IS-AI1110	IDS Centromere B	50 determinations, calibrators incl.
IS-AI1801	IDS AMA (M2)	50 determinations, calibrators incl.
IS-AI1501	IDS Cardiolipin IgG	100 determinations, calibrators incl.
IS-AI1601	IDS Cardiolipin IgM	100 determinations, calibrators incl.
IS-AI1502	IDS B2-Glycoprotein I IgG	100 determinations, calibrators incl.
IS-AI1602	IDS B2-Glycoprotein I IgM	100 determinations, calibrators incl.
IS-AI1109	IDS Jo-1	50 determinations, calibrators incl.
RFCOL-B00/IDS	Rheumatoid Factor	100 determinations
IS-AI1303	IDS t-TG IgA	100 determinations, calibrators incl.
IS-AI1401	IDS t-TG IgG	50 determinations, calibrators incl.
IS-AI1301	IDS Deamidated Gliadin IgA	100 determinations, calibrators incl.
IS-AI1302	IDS Deamidated Gliadin IgG	100 determinations, calibrators incl.





## IDS Control Sets for Chemiluminescence Tests

IDS Order No.	Description	Format	
IS-AI1930	IDS Thyroid Control Set	2 concentrations	
IS-AI1730	IDS ANCA/GBM Control Set	2 concentrations	
IS-AI1830	IDS Liver Control Set	2 concentrations	
IS-AI1230	IDS CCP Control Set	2 concentrations	
IS-AI1130	IDS ANA Control Set	2 concentrations	
IS-AI1030	IDS ANA Screen Control Set	2 concentrations	
IS-AI1530	IDS APS IgG Control Set	2 concentrations	
IS-AI1630	IDS APS IgM Control Set	2 concentrations	
RFREK-000/IDS	Rheumatoid Factor Calibration Set	5 concentrations	
RFCOK-000/IDS	Rheumatoid Factor Control Set	2 concentrations	
RFCON-002/IDS	Rheumatoid Factor Control	1 concentration	
IS-AI1330	IDS CELIAC Control Set	2 concentrations	
IS-AI1430	IDS t-TG IgG Control Set	2 concentrations	



## Radioimmunoassays (RIA) for the Determination of Autoantibodies (Test Systems)

Order No.	Antibodies against	Antigen and Antigen Source	Calibration	Format
RA 1012-10001-1	thyroid peroxidase (TPO) coated tubes (CT)	native thyroid peroxidase, human	0/8/40/200/1000/ 7500 U/ml	100 x 01
RA 1012-10001-3 RA 1012-20001-3	thyroid peroxidase (TPO) magnetic separation	native thyroid peroxidase, human	20/80/400/2000/ 8000 U/ml	100 x 01 200 x 01
RA 1013-10001-1	thyroglobulin (TG) coated tubes (CT)	native thyroglobulin, human	0/20/50/200/1000/ 4000 U/ml	100 x 01
RA 1013-10001-3	thyroglobulin (TG) magnetic separation	native thyroglobulin, human	20/80/250/1000/ 4000 U/ml	100 x 01
RA 1015-10001-1	TSH receptor coated tubes (CT)	native TSH receptor, porcine	0/1/2/8/40 IU/l	100 x 01
RA 1024-5001 RA 1024-10001	insulin precipitation	synthetic product, human	0/0.4/1/10/50 U/ml	50 x 01 100 x 01
RA 1435-3001-1 RA 1435-10001-1	acetylcholine receptor (ACHR) precipitation	extract, human	0/0.25/0.75/ 2.5/8 nmol/l	30 x 01 100 x 01
RA 1571-10001	double-stranded DNA (dsDNA) precipitation	plasmid DNA	6 standards, variable 0-100 IU/ml	100 x 01

## RIA for Direct Detection of Autoantigens, Hormone Determination (Test Systems)

Order No.	Antigen	Analyte	Calibration	Format
RD 1013-10001	thyroglobulin (TG) coated tubes (CT); IRMA	native thyroglobulin	0.3/1/4/20/100/ 250 ng/ml	100 x 01
RD 1016-10001-1	free triiodothyronine (FT3) coated tubes (CT)	triiodothyronine, human	0/2/5/10/20/ 40 pmol/l	100 x 01
RD 1017-10001-1	free thyroxine (FT4) coated tubes (CT)	thyroxine, human	0/6/12/25/50/ 100 pmol/l	100 x 01
RD 1018-10001-1	Turbo thyrotropin (TSH) coated tubes (CT); IRMA	thyrotropin, human	0/0.06/0.15/0.6/2.5/ 15/50/100 µIU/ml	100 x 01
RD 1019-10001-1	calcitonin coated tubes (CT); IRMA	calcitonin, human	6 standards, variable 0-2000 pg/ml	100 x 01





Diagnostics for Indirect Immunofluorescence: Organ-Specific Autoantibodies					
Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FA 1010-1005	thyroid gland (MAb + TAb)	IgG	thyroid gland	monkey	10 x 05 (test system)
FA 1010-1005-2	Polyendocrinopathy Mosaic thyroid gland (MAb + TAb) pancreas islets adrenal cortex ovarian antigens Leydig cells parietal cells (PCA)	IgAGM	6 BIOCHIPS per field: thyroid gland pancreas adrenal gland ovary testis stomach	monkey monkey monkey monkey monkey monkey	10 x 05 (test system)
FA 1010-1005-3 FA 1010-1010-3	EUROPLUS thyroid gland (MAb + TAb) thyroglobulin (TG)	IgG	2 BIOCHIPS per field: thyroid gland TG BIOCHIPS	monkey human	10 x 05 (test system) 10 x 10 (test system)
FA 1020-1005 FA 1020-1010 FA 1020-2005 FA 1020-2010 FB 1020-1005 FB 1020-1010 FB 1020-2005 FB 1020-2010	pancreas islets	IgG	pancreas	monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides)
FC 1020-2005 FC 1020-2010	islet cells antibodies (PM) EUROPattern pancreas islets	IgG	1 BIOCHIP per field: pancreas	monkey	20 x 05 (test system) 20 x 10 (test system)
FA 1020-1005-3 FA 1020-1010-3 FA 1020-2005-3 FA 1020-2010-3	pancreas islets, GAD brain: grey and white matter, Purkinje cell cytoplasm (Yo), Hu and Ri antigen	IgG	pancreas cerebellum (2 BIOCHIPS per field)	monkey monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FA 1022-1005-50	glutamic acid decarboxylase (GAD) 65 kDa (stiff-person syndrome)	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system)
FA 1050-1005 FB 1050-1005	adrenal cortex	IgG	adrenal gland	monkey	10 x 05 (test system) 10 x 05 (single slides)
FC 1050-1005 FC 1050-1010 FC 1050-2005 FC 1050-2010	Endocrinology Screen (AM) EUROPattern adrenal cortex	IgG	1 BIOCHIP per field: adrenal gland	monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FA 1060-1005 FB 1060-1005	ovarian antigens	IgAGM	ovary	monkey	10 x 05 (test system) 10 x 05 (single slides)
FA 1086-1005 FA 1086-1010	spermatozoa	IgAGM	smear	human	10 x 05 (test system) 10 x 10 (test system)
FA 1111-1005 FA 1111-1010 FB 1111-1005 FB 1111-1010	brain: grey and white matter, Purkinje cell cytoplasm (Yo), Hu and Ri antigen CV2, Ma, amphiphysin	IgAGM	cerebellum	monkey	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides)
FA 1111-1005-1 FA 1111-1010-1 FB 1111-1005-1 FB 1111-1010-1	Neurology Mosaic 1 Yo, Hu, Ri, CV2, Ma, amphiphysin medullated nerves non-medullated nerves	IgAGM	3 BIOCHIPS per field: cerebellum nerves intestinal tissue	monkey monkey monkey	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides)
FC 1111-1005-1 FC 1111-1010-1	Neurology Mosaic 1 EUROPattern Yo, Hu, Ri, CV2, Ma, amphiphysin medullated nerves non-medullated nerves	IgG	3 BIOCHIPS per field: cerebellum nerves intestinal tissue	monkey monkey monkey	10 x 05 (test system) 10 x 10 (test system)
FA 1111-1005-2 FA 1111-1010-2	Neurology Mosaic 2 Yo, Hu, Ri, CV2, Ma, amphiphysin medullated nerves	IgAGM	2 BIOCHIPS per field: cerebellum nerves	monkey monkey	10 x 05 (test system) 10 x 10 (test system)



## Diagnostics for Indirect Immunofluorescence: Organ-Specific Autoantibodies

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FA 1111-1005-8 FA 1111-1010-8 FA 1111-12010-8 FB 1111-1005-8 FB 1111-1010-8	<b>Neurology Mosaic 8</b> Yo, Hu, Ri, CV2, Ma, amphiphysin medullated nerves non-medullated nerves pancreas islets	IgAGM	4 BIOCHIPS per field cerebellum nerves intestinal tissue pancreas	monkey monkey monkey monkey	10 x 05 (test system) 10 x 10 (test system) 120 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides)
FC 1111-1005-8 FC 1111-1010-8	<b>Neurology Mosaic 8 EUROPattern</b> Yo, Hu, Ri, CV2, Ma, amphiphysin medullated nerves non-medullated nerves pancreas islets	IgG	4 BIOCHIPS per field: cerebellum nerves intestinal tissue pancreas	monkey monkey monkey monkey	10 x 05 (test system) 10 x 10 (test system)
FA 1111-1005-14 FA 1111-1010-14 FB 1111-1005-14 FB 1111-1010-14	<b>Neurology Mosaic14</b> cerebellum antigens non-medullated nerves	IgAGM	2 BIOCHIPS per field: cerebellum non-medullated nerves	monkey monkey	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides)
FC 1111-12010-14	<b>Neurology Mosaic 14 EUROPattern</b> cerebellum antigens medullated nerves	IgG	2 BIOCHIPS per field cerebellum intestinal tissue	monkey monkey	120 x 10 (test system)
FA 1111-1005-16 FA 1111-1010-16 FB 1111-1005-16 FB 1111-1010-16	<b>Yo, Hu, Ri, CV2, Ma, amphiphysin</b> medullated nerves non-medullated nerves cell nuclei (ANA)	IgAGM	cerebellum nerves intestinal tissue HEp-2 cells (4 BIOCHIPS per field)	monkey monkey monkey human	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides)
FA 1113-1005-1	<b>Purkinje Cell Mosaic 1</b> Yo/CDR2 DNER ITPR1 CARP	IgG	4 BIOCHIPS per field: transfected cells transfected cells transfected cells transfected cells	EU 90 EU 90 EU 90 EU 90	10 x 05 (test system)
FA 111m-1005-3 FA 111m-1010-3 FB 111m-1005-3 FB 111m-1010-3	<b>hippocampus antigens</b> cerebellum antigens glutamate receptor (type NMDA)	IgG	hippocampus cerebellum transfected cells control transfection (4 BIOCHIPS per field)	rat rat EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides)
FA 1120-1005 FB 1120-1005	<b>medullated nerves</b>	IgAGM	nerves	monkey	10 x 05 (test system) 10 x 05 (single slides)
FA 1124-1005-50 *	<b>Flotillin (FLOT1/2)</b>	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system)
FA 1128-1005-1 FA 1128-1010-1	<b>NMOSD Screen 1</b> aquaporin-4 (AQP-4) Myelin-oligodendrocyte glycoprotein (MOG)	IgG	3 BIOCHIPS per field: transfected cells transfected cells control transfection	EU 90 EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system)
FC 1128-2005-1	<b>NMOSD Screen 1 EUROPattern</b> aquaporin-4 (AQP-4) Myelin-oligodendrocyte glycoprotein (MOG)	IgG PI	3 BIOCHIPS per field: transfected cells transfected cells control transfection	EU 90 EU 90 EU 90	20 x 05 (test system)
FA 1128-1005-50 FA 1128-1010-50 FB 1128-1005-50 FB 1128-1010-50	<b>aquaporin-4</b>	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides)
FC 1128-1005-50 FC 1128-1010-50 FC 1128-2005-50 FC 1128-2010-50	<b>aquaporin-4 EUROPattern</b>	IgG PI	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)

\* For research use only, not for in vitro diagnostic use in the sense of EU directive 98/79/EC.



Diagnostics for Indirect Immunofluorescence: Organ-Specific Autoantibodies					
Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FA 112d-1005-1 FB 112d-1005-1	<b>Autoimmune Encephalitis Mosaic 1</b> glutamate receptor (type NMDA) glutamate receptor (type AMPA1) glutamate receptor (type AMPA2) contactin-associated protein 2 (CASPR2) leucine-rich glioma-inactivated protein 1 (LGI1) GABA B receptor	IgG	6 BIOCHIPS per field: transfected cells transfected cells transfected cells transfected cells transfected cells transfected cells	EU 90 EU 90 EU 90 EU 90 EU 90 EU 90	10 x 05 (test system) 10 x 05 (single slides)
FA 112d-1005-6 FA 112d-1010-6 FB 112d-1005-6	<b>Autoimmune Encephalitis Mosaic 6</b> glutamate receptor (type NMDA) contactin-associated protein 2 (CASPR2) glutamate receptors (type AMPA1/2) leucine-rich glioma-inactivated protein 1 (LGI1) dipeptidyl aminopeptidase-like protein 6 (DPPX) GABA B receptor	IgG	6 BIOCHIPS per field: transfected cells transfected cells transfected cells transfected cells transfected cells transfected cells	EU 90 EU 90 EU 90 EU 90 EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (single slides)
FC 112d-1005-6 FC 112d-1010-6 FC 112d-2005-6 FC 112d-2010-6	<b>Autoimmune Encephalitis Mosaic 6 EUROPattern</b> glutamate receptor (type NMDA) contactin-associated protein 2 (CASPR2) glutamate receptors (type AMPA1/2) leucine-rich glioma-inactivated protein 1 (LGI1) dipeptidyl aminopeptidase-like protein 6 (DPPX) GABA B receptor	IgG PI	6 BIOCHIPS per field: transfected cells transfected cells transfected cells transfected cells transfected cells transfected cells	EU 90 EU 90 EU 90 EU 90 EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FA 112d-1005-14	<b>RC-IIFT Neurology Mosaic 14A</b> glutamate receptor (type NMDA) contactin-associated protein 2 (CASPR2) IgLON family member 5 (IgLON5) dipeptidyl aminopeptidase-like protein 6 (DPPX) leucine-rich glioma-inactivated protein 1 (LGI1) GABA B receptor	IgG	6 BIOCHIPS per field: transfected cells transfected cells transfected cells transfected cells transfected cells transfected cells	EU 90 EU 90 EU 90 EU 90 EU 90 EU 90	10 x 05 (test system)
FA 112d-1005-51 FA 112d-1010-51 FB 112d-1005-51 FB 112d-1010-51	<b>glutamate receptor (type NMDA)</b>	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides)
FC 112d-1005-51 FC 112d-1010-51 FC 112d-2005-51 FC 112d-2010-51 FC 112d-12010-51	<b>glutamate receptor (type NMDA) EUROPattern</b>	IgG PI	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system)
FA 112k-1003-1 FA 112k-1005-1 FB 112k-1005-1	<b>glutamate receptor (type AMPA1)</b> <b>glutamate receptor (type AMPA2)</b>	IgG	transfected cells transfected cells control transfection (3 BIOCHIPS per field)	EU 90 EU 90 EU 90	10 x 03 (test system) 10 x 05 (test system) 10 x 05 (single slides)
FA 112l-1005-50 FB 112l-1005-50	<b>GABA B receptor</b>	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system) 10 x 05 (single slides)
FA 112m-1005-50	<b>dipeptidyl aminopeptidase-like protein 6 (DPPX)</b>	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system)
FC 112m-2005-50	<b>dipeptidyl aminopeptidase-like protein 6 (DPPX) EUROPattern</b>	IgG PI	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	20 x 05 (test system)
FA 112n-1005-52 *	<b>metabotropic glutamate receptor 5 (mGluR5)</b>	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system)

\* For research use only, not for in vitro diagnostic use in the sense of EU directive 98/79/EC.



## Diagnostics for Indirect Immunofluorescence: Organ-Specific Autoantibodies

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FA 1151-1005-50	IgLON family member 5 (IgLON5)	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system)
FA 1156-1005-50 FA 1156-1010-50	Myelin-oligodendrocyte glycoprotein (MOG)	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system)
FC 1156-2005-50	Myelin-Oligodendrocyte-Glycoprotein (MOG) EUROPattern	IgG PI	transfected cells control transfection	EU 90 EU 90	20 x 05 (test system)
FA 1170-1005	eye antigens	IgAGM	eye	monkey	10 x 05 (test system)
FA 1172-1005	retina	IgAGM	eye	monkey	10 x 05 (test system)
FA 1200-1005 FA 1200-1010 FA 1200-2005 FA 1200-18010 FB 1200-1005 FB 1200-1010 FB 1200-2005 FB 1200-18010	cytoplasm of granulocytes (cANCA, pANCA), nuclei of granulocytes (GS-ANA)	IgG	granulocytes, ethanol-fixed	human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 180 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 180 x 10 (single slides)
FC 1200-1005 FC 1200-1010 FC 1200-2005 FC 1200-2010 FC 1200-12010	cytoplasm of granulocytes (cANCA, pANCA), nuclei of granulocytes (GS-ANA) EUROPattern	IgG EB	granulocytes, ethanol-fixed	human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system)
FA 1201-1005 FA 1201-1010 FB 1201-1005 FB 1201-1010	granulocytes (cANCA, pANCA)	IgG	granulocytes, formaldehyde-fixed	human	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides)
FC 1201-1005 FC 1201-1010 FC 1201-2005	granulocytes (cANCA, pANCA) EUROPattern	IgG EB	granulocytes, formaldehyde-fixed	human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system)
FA 1201-1005-2 FA 1201-1010-2 FA 1201-2005-2 FA 1201-2010-2 FB 1201-1005-2 FB 1201-1010-2 FB 1201-2005-2 FB 1201-2010-2	Granulocyte Mosaic 2 cANCA, pANCA, GS-ANA cANCA, pANCA	IgG	2 BIOCHIPS per field: granulocytes (EOH) granulocytes (HCHO)	human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides)
FC 1201-1005-2 FC 1201-1010-2 FC 1201-2005-2 FC 1201-2010-2 FC 1201-12010-2	Granulocyte Mosaic 2 EUROPattern cANCA, pANCA, GS-ANA, EUROPattern cANCA, pANCA, EUROPattern	IgG EB	2 BIOCHIPS per field: granulocytes (EOH) granulocytes (HCHO)	human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system)
FA 1201-1005-13 FA 1201-1010-13 FA 1201-2005-13 FA 1201-2010-13 FA 1201-1050-13 FA 1201-12010-13 FA 1201-2450-13 FB 1201-1005-13 FB 1201-1010-13 FB 1201-2005-13 FB 1201-2010-13 FB 1201-1050-13	Granulocyte Mosaic 13 cANCA, pANCA, GS-ANA cell nuclei (ANA), cANCA, pANCA cANCA, pANCA	IgG	3 BIOCHIPS per field: granulocytes (EOH) HEp-2+granulocytes (EOH) granulocytes (HCHO)	human human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 50 (test system) 120 x 10 (test system) 24 x 50 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides) 10 x 50 (single slides)



Diagnostics for Indirect Immunofluorescence: Organ-Specific Autoantibodies					
Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FC 1201-1005-13 FC 1201-1010-13 FC 1201-2005-13 FC 1201-2010-13 FC 1201-12010-13 FC 1201-2450-13 FW1201-1005-13 FW1201-2010-13	<b>Granulocyte Mosaic 13 EUROPattern</b> cANCA, pANCA, GS-ANA, EUROPattern cell nuclei (ANA), cANCA, pANCA cANCA, pANCA, EUROPattern	IgG EB	3 BIOCHIPS per field: granulocytes (EOH) HEp-2+granulocytes (EOH) granulocytes (HCHO)	human human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system) 24 x 50 (test system) 10 x 05 (single slides) 20 x 10 (single slides)
FA 1201-1005-15 FA 1201-1010-15 FA 1201-2005-15 FA 1201-2010-15 FB 1201-1005-15 FB 1201-1010-15 FB 1201-2005-15 FB 1201-2010-15	<b>Granulocyte Mosaic 15</b> cANCA, pANCA, GS-ANA cell nuclei (ANA), cANCA, pANCA	IgG	2 BIOCHIPS per field: granulocytes (EOH) HEp-2+granulocytes (EOH)	human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides)
FC 1201-1005-15 FC 1201-1010-15 FC 1201-2010-15 FC 1201-1050-15 FW1201-1005-15	<b>Granulocyte Mosaic 15 EUROPattern</b> cANCA, pANCA, GS-ANA, EUROPattern cell nuclei (ANA), cANCA, pANCA	IgG EB	2 BIOCHIPS per field: granulocytes (EOH) HEp-2+granulocytes (EOH)	human human	10 x 05 (test system) 10 x 10 (test system) 20 x 10 (test system) 10 x 50 (test system) 10 x 05 (single slides)
FA 1201-1005-22 FA 1201-1010-22 FA 1201-2005-22 FB 1201-1005-22 FB 1201-1010-22 FB 1201-2005-22	<b>EUROPLUS Granulocyte Mosaic 22</b> cANCA, pANCA, GS-ANA cANCA, pANCA pANCA: myeloperoxidase (MPO) cANCA: proteinase 3 (PR3)	IgG	4 BIOCHIPS per field: granulocytes (EOH) granulocytes (HCHO) MPO BIOCHIPS PR3 BIOCHIPS	human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides)
FC 1201-1005-22 FC 1201-1010-22 FC 1201-2005-22 FC 1201-2010-22	<b>EUROPLUS Granulocyte Mosaic 22 EUROPattern</b> cANCA, pANCA, GS-ANA, EUROPattern cANCA, pANCA, EUROPattern pANCA: myeloperoxidase (MPO), EUROPattern cANCA: proteinase 3 (PR3), EUROPattern	IgG EB	4 BIOCHIPS per field: granulocytes (EOH) granulocytes (HCHO) MPO BIOCHIPS PR3 BIOCHIPS	human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FA 1201-1005-25 FA 1201-1010-25 FA 1201-2005-25 FA 1201-2010-25 FB 1201-1005-25 FB 1201-1010-25 FB 1201-2005-25 FB 1201-2010-25	<b>EUROPLUS Granulocyte Mosaic 25</b> cANCA, pANCA, GS-ANA cell nuclei (ANA), cANCA, pANCA cANCA, pANCA glomerular basement membrane (GBM) pANCA: myeloperoxidase (MPO) cANCA: proteinase 3 (PR3)	IgG	6 BIOCHIPS per field: granulocytes (EOH) HEp-2+granulocytes (EOH) granulocytes (HCHO) GBM BIOCHIPS MPO BIOCHIPS PR3 BIOCHIPS	human human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides)
FC 1201-1005-25 FC 1201-1010-25 FC 1201-2005-25 FC 1201-2010-25 FW1201-1005-25 FW1201-2010-25	<b>EUROPLUS Granulocyte Mosaic 25 EUROPattern</b> cANCA, pANCA, GS-ANA, EUROPattern cell nuclei (ANA), cANCA, pANCA cANCA, pANCA, EUROPattern glom. basement membrane (GBM), EUROPattern pANCA: myeloperoxidase (MPO), EUROPattern cANCA: proteinase 3 (PR3), EUROPattern	IgG EB	6 BIOCHIPS per field: granulocytes (EOH) HEp-2+granulocytes (EOH) granulocytes (HCHO) GBM BIOCHIPS MPO BIOCHIPS PR3 BIOCHIPS	human human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (single slides) 20 x 10 (single slides)
FA 1201-1005-32 FA 1201-1010-32 FA 1201-2005-32 FA 1201-2010-32 FB 1201-1005-32 FB 1201-1010-32 FB 1201-2005-32 FB 1201-2010-32	<b>EUROPLUS Granulocyte Mosaic 32</b> cANCA, pANCA, GS-ANA cANCA, pANCA cell nuclei (ANA), cANCA, pANCA pANCA: myeloperoxidase (MPO) cANCA: proteinase 3 (PR3)	IgG	5 BIOCHIPS per field: granulocytes (EOH) granulocytes (HCHO) HEp-2+granulocytes (EOH) MPO BIOCHIPS PR3 BIOCHIPS	human human human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides)





## Diagnostics for Indirect Immunofluorescence: Organ-Specific Autoantibodies

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FC 1201-1005-32	<b>EUROPLUS Granulocyte Mosaic 32</b> <b>EUOPattern</b> <b>cANCA, pANCA, GS-ANA, EUOPattern</b> <b>cANCA, pANCA, EUOPattern</b> <b>cell nuclei (ANA), cANCA, pANCA</b> <b>pANCA: myeloperoxidase (MPO), EUOPattern</b> <b>cANCA: proteinase 3 (PR3), EUOPattern</b>	IgG EB	5 BIOCHIPS per field:  granulocytes (EOH) granulocytes (HCHO) HEp-2+granulocytes (EOH) MPO BIOCHIPS PR3 BIOCHIPS	human human human	10 x 05 (test system)
FC 1201-1010-32					10 x 10 (test system)
FC 1201-2005-32					20 x 05 (test system)
FC 1201-2010-32					20 x 10 (test system)
FC 1201-12010-32					120 x 10 (test system)
FW1201-1005-32					10 x 05 (single slides)
FW1201-1010-32					10 x 10 (single slides)
FA 1230-1005	<b>thrombocyte antigens</b>	IgG	thrombocytes	human	10 x 05 (test system)
FA 1230-1010					10 x 10 (test system)
FB 1230-1005					10 x 05 (single slides)
FB 1230-1010					10 x 10 (single slides)
FA 1250-1005	<b>renal glomeruli (GBM)</b> <b>and renal tubuli</b>	IgG	kidney	monkey	10 x 05 (test system)
FA 1250-1010					10 x 10 (test system)
FB 1250-1005					10 x 05 (single slides)
FB 1250-1010					10 x 10 (single slides)
FC 1250-2005	<b>Nephrology Screen (KM) EUOPattern</b> <b>renal glomeruli (GBM)</b>	IgG	kidney	monkey	20 x 05 (test system)
FA 1250-1005-1	<b>EUROPLUS</b> <b>kidney glomeruli and tubuli</b> <b>glomerular basement membrane (GBM)</b>	IgG	2 BIOCHIPS per field: kidney GBM BIOCHIPS	monkey	10 x 05 (test system)
FA 1250-1010-1					10 x 10 (test system)
FB 1250-1005-1					10 x 05 (single slides)
FB 1250-1010-1					10 x 10 (single slides)
FC 1250-2005-1	<b>EUROPLUS Nephrology Screen 1 EUOPattern</b> <b>Renal glomeruli (GBM)</b> <b>glomerular basement membrane (GBM)</b>	IgG	2 BIOCHIPS per field kidney GBM-EUROPLUS	monkey	20 x 05 (test system)
FA 1254-1005-1	<b>Membranous Nephropathy Mosaic 1</b> <b>phospholipase A2 receptor (PLA2R)</b> <b>Thrombospondin type-1 domain-containing</b> <b>protein 7A (THSD7A)</b>	IgG	3 BIOCHIPS per field: transfected cells transfected cells control transfection	EU 90	10 x 05 (test system)
FA 1254-1010-1				EU 90	10 x 10 (test system)
FB 1254-1005-1				EU 90	10 x 05 (single slides)
FB 1254-1010-1				EU 90	10 x 10 (single slides)
FA 1254-1005-50	<b>phospholipase A2 receptor (PLA2R)</b>	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90	10 x 05 (test system)
FA 1254-1010-50				EU 90	10 x 10 (test system)
FA 1254-2010-50					20 x 10 (test system)
FB 1254-1005-50					10 x 05 (single slides)
FB 1254-1010-50					10 x 10 (single slides)
FC 1254-1005-50				<b>phospholipase A2 receptor (PLA2R)</b> <b>EUOPattern</b>	IgG PI
FC 1254-1010-50	EU 90	10 x 10 (test system)			
FC 1254-2005-50		20 x 05 (test system)			
FC 1254-2010-50		20 x 10 (test system)			
FA 1254-1005-51	<b>Thrombospondin type-1 domain-</b> <b>containing protein 7A (THSD7A)</b>	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90	10 x 05 (test system)
FA 1254-2005-51				EU 90	20 x 05 (test system)
FA 1300-1005-1	<b>Liver Mosaic 1</b> <b>liver-kidney microsomes (LKM), ANA</b> <b>mitochondria (AMA), LKM</b>	IgG	2 BIOCHIPS per field: liver kidney	rat rat	10 x 05 (test system)
FA 1300-1010-1					10 x 10 (test system)
FA 1300-2005-1					20 x 05 (test system)
FB 1300-1005-1					10 x 05 (single slides)
FB 1300-1010-1					10 x 10 (single slides)
FB 1300-2005-1					20 x 05 (single slides)
FA 1300-1005-8	<b>Liver Mosaic 8</b> <b>liver antigens, cell nuclei (ANA)</b> <b>F-actin</b> <b>cell nuclei (ANA)</b> <b>LKM, ANA</b> <b>mitochondria (AMA), LKM</b> <b>smooth muscles (ASMA)</b>	IgG	6 BIOCHIPS per field: liver VSM47 HEp-2 cells liver kidney stomach	monkey rat human rat rat rat	10 x 05 (test system)
FA 1300-1010-8					10 x 10 (test system)
FA 1300-2005-8					20 x 05 (test system)
FB 1300-1005-8					10 x 05 (single slides)
FB 1300-1010-8					10 x 10 (single slides)
FB 1300-1010-8					10 x 10 (single slides)
FB 1300-2005-8					20 x 05 (single slides)
FB 1300-2005-8					20 x 05 (single slides)





Diagnostics for Indirect Immunofluorescence: Organ-Specific Autoantibodies					
Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FA 1300-1005-9	Liver Mosaic 9 mitochondria (AMA), LKM LKM, ANA smooth muscles (ASMA) F-actin	IgG	4 BIOCHIPS per field: kidney liver stomach VSM47	rat rat rat rat	10 x 05 (test system)
FA 1300-1010-9					10 x 10 (test system)
FB 1300-1005-9					10 x 05 (single slides)
FB 1300-1010-9					10 x 10 (single slides)
FC 1300-1005-9	Autoimmune liver diseases Screen 9 EUROPattern mitochondria (AMA), LKM LKM, ANA smooth muscles (ASMA) F-actin	IgG PI	4 BIOCHIPS per field: kidney liver stomach VSM47	rat rat rat rat	10 x 05 (test system)
FC 1300-1010-9					10 x 10 (test system)
FC 1300-2005-9					20 x 05 (test system)
FC 1300-2010-9					20 x 10 (test system)
FA 1302-1005-50	soluble liver antigen/ liver-pancreas antigen (SLA/LP)	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system)
FA 1302-1010-50					10 x 10 (test system)
FA 1360-1005	parietal cells (PCA)	IgG	stomach	monkey	10 x 05 (test system)
FA 1360-1010					10 x 10 (test system)
FA 1360-2005					20 x 05 (test system)
FA 1360-2010					20 x 10 (test system)
FB 1360-1005					10 x 05 (single slides)
FB 1360-1010					10 x 10 (single slides)
FB 1360-2005					20 x 05 (single slides)
FB 1360-2010					20 x 10 (single slides)
FC 1360-2005	Anti-Parietal cells (SM) IIFT EUROPattern	IgG	stomach	monkey	20 x 05 test system
FC 1360-2010					20 x 10 test system
FA 1362-1005	intrinsic factor	IgG	intrinsic factor BIOCHIPS		10 x 05 (test system)
FB 1362-1005					10 x 05 (single slides)
FA 1362-1005-1	EUROPLUS parietal cells (PCA) intrinsic factor	IgG	2 BIOCHIPS per field: stomach intrinsic factor BIOCHIPS	monkey	10 x 05 (test system)
FA 1362-1010-1					10 x 10 (test system)
FA 1362-2005-1					20 x 05 (test system)
FB 1362-1005-1					10 x 05 (single slides)
FB 1362-1010-1					10 x 10 (single slides)
FB 1362-2005-1					20 x 05 (single slides)
FA 1391-1005-3	CIBD Screen 3 pancreas ag rPAg1(CUZD1) / rPAg2(GP2) intestinal goblet cells	IgA/G	3 BIOCHIPS per field: transfected cells goblet cells control transfection	EU 90 EU 80 EU 90	10 x 05 (test system)
FB 1391-1005-3					10 x 05 (single slides)
FA 1391-1005-4	CIBD Profile 3 upper row: pancreas ag rPAg1(CUZD1) / rPAg2(GP2) intestinal goblet cells pANCA DNA-bound lactoferrin (pANCA) ANCA negative bottom row: Saccharomyces cerevisiae format 1003: slides with 3 patient profiles format 1005: slides with 5 patient profiles	IgA/G	transfected cells control transfection goblet cells granulocytes (EOH) LFS granulocytes HSS granulocytes fungal smear	EU 90 EU 90 EU 80 human human human S. cerevisiae	10 x 05 (test system)
FA 1391-1005-7	CIBD Profile 7 upper row: pancreas ag rPAg1(CUZD1) / rPAg2(GP2) intestinal goblet cells pANCA bottom row: Saccharomyces cerevisiae format 1003: slides with 3 patient profiles format 1005: slides with 5 patient profiles	IgA/G	transfected cells goblet cells granulocytes (EOH) control transfection fungal smear	EU 90 EU 80 human EU 90 S. cerevisiae	10 x 05 (test system)
FB 1391-1005-7					10 x 05 (single slides)



## Diagnostics for Indirect Immunofluorescence: Organ-Specific Autoantibodies

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FA 1420-1005 FB 1420-1005	parotid gland excretory ducts and acini	IgG	parotid gland	monkey	10 x 05 (test system) 10 x 05 (single slides)
FA 1430-1005 FB 1430-1005	skeletal muscle	IgG	musculus iliopsoas	monkey	10 x 05 (test system) 10 x 05 (single slides)
FC 1430-2005	Myasthenia gravis Screen (SMM) EUROPattern skeletal muscle	IgG	1 BIOCHIP per field: musculus iliopsoas	monkey	20 x 05 (test system)
FA 1430-1005-1 FB 1430-1005-1	Mosaic Heart Muscle/Skeletal Muscle heart muscle skeletal muscle	IgG	2 BIOCHIPS per field: heart musculus iliopsoas	monkey monkey	10 x 05 (test system) 10 x 05 (single slides)
FA 1434-1005-90 FA 1434-1010-90	Muscle-Specific Kinase (MuSK) ---	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system)
FA 1435-1005-2 FA 1435-1010-2	Myasthenia gravis Mosaic 2 adult acetylcholine receptor (AChR-E) fetal acetylcholine receptor (AChR-G) Muscle-specific Kinase (MuSK)	IgG	4 BIOCHIPS per field: transfected cells transfected cells transfected cells control transfection	EU 90 EU 90 EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system)
FA 1435-1005-90 FA 1435-1010-90	Anti-Acetylcholine Receptor (AChR) IIFT adulter Acetylcholinrezeptor (AChR-E) fetaler Acetylcholinrezeptor (AChR-G) ---	IgG	3 BIOCHIPS per field: transfected cells transfected cells control transfection	EU 90 EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system)
FA 1439-1005-1 FB 1439-1005-1	Anti-VGKC-Ass. Proteins Mosaic 1 leucine-rich glioma-inact. prot. 1 (LGI1) contactin-associated protein 2 (CASPR2)	IgG	3 BIOCHIPS per field: transfected cells transfected cells control transfection	EU 90 EU 90 EU 90	10 x 05 (test system) 10 x 05 (single slides)
FC 1439-1005-1 FC 1439-12010-1	Anti-VGKC-Ass. Proteins Mosaic 1 EUROPattern leucine-rich glioma-inact. prot. 1 (LGI1) contactin-associated protein 2 (CASPR2)	IgG PI	3 BIOCHIPS per field: transfected cells transfected cells control transfection	EU 90 EU 90 EU 90	10 x 05 (test system) 120 x 10 (test system)
FA 1439-1005-50	contactin-associated protein 2 (CASPR2)	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system)
FA 1439-1005-51	leucine-rich glioma-inactivated protein 1 (LGI1)	IgG	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system)
FA 1461-1005 FA 1461-2005 FB 1461-1005 FB 1461-2005	heart muscle	IgG	heart	monkey	10 x 05 (test system) 20 x 05 (test system) 10 x 05 (single slides) 20 x 05 (single slides)
FA 1501-1005 FA 1501-1010 FA 1501-2005 FB 1501-1005 FB 1501-1010 FB 1501-2005	epidermis: prickle cell desmosomes epidermal basement membrane	IgG	oesophagus	monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides)
FC 1501-1005 FC 1501-1010 FC 1501-2005	Dermatology Screen (EM) EUROPattern epidermis: prickle cell desmosomes epidermal basement membrane	IgG+IgG4	oesophagus	monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system)



## Diagnostics for Indirect Immunofluorescence: Organ-Specific Autoantibodies

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FA 1501-1005-7 FA 1501-1010-7 FB 1501-1005-7 FB 1501-1010-7	<b>Dermatology Mosaic 7</b> epidermis <b>pemphigoid antigens</b> BP230gC desmoglein 1 desmoglein 3 BP180-NC16A-4X	IgG	6 BIOCHIPS per field: oesophagus salt-split skin transfected cells transfected cells transfected cells BP180-NC16A-4X BIOCHIPS	monkey monkey EU 90 EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides)
FC 1501-1005-7 FC 1501-1010-7 FC 1501-2005-7 FC 1501-2010-7	<b>EUROPLUS Dermatology Mosaic 7</b> epidermis <b>pemphigoid antigens</b> BP230gC desmoglein 1 desmoglein 3 BP180-NC16A-4X	<b>EUROPattern</b> IgG+IgG4	6 BIOCHIPS per field: oesophagus salt-split skin transfected cells transfected cells transfected cells BP180-NC16A-4X EUROPLUS	monkey monkey EU 90 EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FA 1501-1005-20 FA 1501-1010-20 FA 1501-2005-20 FB 1501-1005-20 FB 1501-1010-20 FB 1501-2005-20	<b>Dermatology Mosaic 20</b> epidermis <b>pemphigoid antigens</b>	IgG	2 BIOCHIPS per field: oesophagus salt-split skin	monkey monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides)
FC 1501-1010-20 FC 1501-2005-20 FC 1501-2010-20	<b>Dermatology Mosaic 20</b> epidermis <b>pemphigoid antigens</b>	<b>EUROPattern</b> IgG+IgG4	2 BIOCHIPS per field: oesophagus salt-split skin	monkey monkey	10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FA 150b-1005-50	<b>laminin 332 (LAM332)</b>	IgG+IgG4	transfected cells control transfection (2 BIOCHIPS per field)	EU 90 EU 90	10 x 05 (test system)



## Diagnostics for Indirect Immunofluorescence: Systemic Autoantibodies

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FA 1510-1005-1 FA 1510-1010-1 FA 1510-2005-1 FA 1510-2010-1 FA 1510-1050-1 FA 1510-5010-1 FA 1510-0010-1 FA 1510-12010-1 FA 1510-2450-1 FB 1510-1005-1 FB 1510-1010-1 FB 1510-2005-1 FB 1510-2010-1 FB 1510-1050-1 FB 1510-5010-1 FB 1510-0010-1	cell nuclei (ANA global test)	IgG	HEp-2 cells liver (2 BIOCHIPs per field)	human monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 50 (test system) 50 x 10 (test system) 100 x 10 (test system) 120 x 10 (test system) 24 x 50 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides) 10 x 50 (single slides) 50 x 10 (single slides) 100 x 10 (single slides)
FC 1510-1005-1 FC 1510-1010-1 FC 1510-2005-1 FC 1510-2010-1 FC 1510-12010-1 FC 1510-2450-1 FW1510-2010-1 FW1510-1050-1	cell nuclei (ANA) EUROPattern cell nuclei (ANA)	IgG PI	HEp-2 cells liver (2 BIOCHIPs per field)	human monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system) 24 x 50 (test system) 20 x 10 (single slides) 10 x 50 (single slides)
FA 1510-1005-2 FA 1510-1010-2 FB 1510-1005-2 FB 1510-1010-2	cell nuclei (ANA) mitochondria (AMA)	IgG	HEp-2 cells kidney (2 BIOCHIPs per field)	human rat	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides)
FA 1512-1005-1 FA 1512-1010-1 FA 1512-2005-1 FA 1512-2010-1 FA 1512-1050-1 FA 1512-5010-1 FA 1512-0010-1 FA 1512-12010-1 FA 1512-2450-1 FB 1512-1005-1 FB 1512-1010-1 FB 1512-2005-1 FB 1512-2010-1 FB 1512-1050-1 FB 1512-5010-1 FB 1512-0010-1	cell nuclei (ANA global test)	IgG	HEp-20-10 cells liver (2 BIOCHIPs per field)	human monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 50 (test system) 50 x 10 (test system) 100 x 10 (test system) 120 x 10 (test system) 24 x 50 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides) 10 x 50 (single slides) 50 x 10 (single slides) 100 x 10 (single slides)
FC 1512-1005-1 FC 1512-1010-1 FC 1512-2005-1 FC 1512-2010-1 FC 1512-1050-1 FC 1512-12010-1 FC 1512-2450-1 FW1512-1005-1 FW1512-1010-1 FW1512-2010-1 FW1512-1050-1	cell nuclei (ANA) EUROPattern cell nuclei (ANA)	IgG PI	HEp-20-10 cells liver (2 BIOCHIPs per field)	human monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 50 (test system) 120 x 10 (test system) 24 x 50 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 10 (single slides) 20 x 10 (single slides) 10 x 50 (single slides) 20 x 10 (single slides) 10 x 50 (single slides)
FA 1512-1005-2 FA 1512-1010-2 FA 1512-1050-2 FB 1512-1005-2 FB 1512-1010-2 FB 1512-1050-2	cell nuclei (ANA) mitochondria (AMA)	IgG	HEp-20-10 cells kidney (2 BIOCHIPs per field)	human rat	10 x 05 (test system) 10 x 10 (test system) 10 x 50 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 10 x 50 (single slides)
FC 1512-1005-2 FC 1512-12010-2 FC 1512-2450-2	cell nuclei (ANA) EUROPattern mitochondria (AMA)	IgG PI	HEp-20-10 cells kidney (2 BIOCHIPs per field)	human rat	10 x 05 (test system) 120 x 10 (test system) 24 x 50



Diagnostics for Indirect Immunofluorescence: Systemic Autoantibodies					
Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FA 1512-1005-10 FA 1512-1010-10	<b>EUROPLUS ANA Mosaic 10A</b> cell nuclei (ANA) SS-A + SS-B	IgG	2 BIOCHIPS per field: HEp-20-10 cells SS-A+SS-B BIOCHIPS	human	10 x 05 (test system) 10 x 10 (test system)
FA 1512-1005-22 FA 1512-1010-22	<b>EUROPLUS ANA Mosaic 22A</b> cell nuclei (ANA) cell nuclei (ANA) nRNP/Sm + Sm + SS-A SS-B + Scl-70 + Jo-1	IgG	4 BIOCHIPS per field: HEp-20-10 cells liver nRNP/Sm+Sm+SS-A BIOCHIPS SS-B+Scl-70+Jo-1 BIOCHIPS	human monkey	10 x 05 (test system) 10 x 10 (test system)
FA 1520-1005 FA 1520-1010 FA 1520-2005 FA 1520-2010 FA 1520-1050 FA 1520-5010 FA 1520-0010 FA 1520-12010 FB 1520-1005 FB 1520-1010 FB 1520-2005 FB 1520-2010 FB 1520-1050 FB 1520-5010 FB 1520-0010	cell nuclei (ANA)	IgG	HEp-2 cells	human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 50 (test system) 50 x 10 (test system) 100 x 10 (test system) 120 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides) 10 x 50 (single slides) 50 x 10 (single slides) 100 x 10 (single slides)
FC 1520-1005 FC 1520-1010 FC 1520-2005 FC 1520-2010 FC 1520-1050 FC 1520-12010 FC 1520-2450 FW1520-1005 FW1520-1010 FW1520-2005 FW1520-2010 FW1520-1050	cell nuclei (ANA) EUROPattern	IgG PI	HEp-2 cells	human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 50 (test system) 120 x 10 (test system) 24 x 50 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides) 10 x 50 (single slides)
FA 1522-1005 FA 1522-1010 FA 1522-2005 FA 1522-2010 FA 1522-5010 FA 1522-0010 FB 1522-1005 FB 1522-1010 FB 1522-2005 FB 1522-2010 FB 1522-5010 FB 1522-0010	cell nuclei (ANA)	IgG	HEp-20-10 cells	human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 50 x 10 (test system) 100 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides) 50 x 10 (single slides) 100 x 10 (single slides)
FC 1522-1005 FC 1522-1010 FC 1522-2005 FC 1522-2010 FC 1522-1050 FC 1522-12010 FW1522-1005 FW1522-2005 FW1522-2010	cell nuclei (ANA) EUROPattern	IgG PI	HEp-20-10 cells	human	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 50 (test system) 120 x 10 (test system) 10 x 05 (single slides) 20 x 05 (single slides) 20 x 10 (single slides)
FA 1572-1005 FA 1572-1010 FA 1572-2005 FA 1572-2010 FB 1572-1005 FB 1572-1010 FB 1572-2005 FB 1572-2010	dsDNA	IgG	flagellates	Crithidia luciliae	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides)



## Diagnostics for Indirect Immunofluorescence: Systemic Autoantibodies

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FC 1572-1005 FC 1572-1010 FC 1572-2005 FC 1572-2010	<b>dsDNA EUROPattern</b>	IgG EB	flagellates	Crithidia luciliae	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FA 1572-1005-1 FA 1572-1010-1 FA 1572-2005-1 FA 1572-2010-1	<b>dsDNA (sensitive)</b>	IgG	flagellates	Crithidia luciliae	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FC 1572-1005-1 FC 1572-1010-1 FC 1572-2005-1 FC 1572-2010-1 FC 1572-12010-1	<b>dsDNA (sensitive) EUROPattern</b>	IgG EB	flagellates	Crithidia luciliae	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system)
FA 1620-1005 FA 1620-1010 FA 1620-2005 FA 1620-2010 FB 1620-1005 FB 1620-1010 FB 1620-2005 FB 1620-2010	<b>mitochondria (AMA)</b>	IgG	kidney	rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides)
FA 1620-1005-1 FA 1620-1010-1 FA 1620-2005-1 FA 1620-2010-1 FA 1620-1050-1 FB 1620-1005-1 FB 1620-1010-1 FB 1620-2005-1 FB 1620-2010-1 FB 1620-1050-1	<b>mitochondria (AMA) smooth muscles (ASMA)</b>	IgG	kidney stomach (2 BIOCHIPS per field)	rat rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 50 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides) 10 x 50 (single slides)
FC 1620-1005-1 FC 1620-1010-1 FC 1620-2005-1 FC 1620-2010-1	<b>AMA/ASMA IIFT (KR/SR) EUROPattern mitochondria (AMA) smooth muscles (ASMA)</b>	IgG	2 BIOCHIPS per field: kidney stomach	rat rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FA 1620-1005-5 FA 1620-1010-5 FB 1620-1005-5 FB 1620-1010-5	<b>EUROPLUS mitochondria (AMA) smooth muscles (ASMA) cell nuclei (ANA) M2 antigen</b>	IgG	4 BIOCHIPS per field: kidney stomach HEp-2 cells M2 BIOCHIPS	rat rat human	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides)
FA 1651-1005 FA 1651-1010	<b>F-actin</b>	IgG	VSM47	rat	10 x 05 (test system) 10 x 10 (test system)
FC 1651-1005 FC 1651-1010	<b>F-actin EUROPattern</b>	IgG PI	VSM47	rat	10 x 05 (test system) 10 x 10 (test system)
FA 1710-1005 FA 1710-1010 FA 1710-2005 FA 1710-2010 FB 1710-1005 FB 1710-1010 FB 1710-2005 FB 1710-2010	<b>smooth muscles (ASMA)</b>	IgG	stomach	rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides)
FA 1710-1005-1 FA 1710-2010-1 FB 1710-1005-1	<b>smooth muscles (ASMA) F-actin</b>	IgG	stomach VSM47 (2 BIOCHIPS per field)	rat rat	10 x 05 (test system) 20 x 10 (test system) 10 x 05 (single slides)





Diagnostics for Indirect Immunofluorescence: Systemic Autoantibodies					
Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FA 1800-1005-1 FA 1800-1010-1 FA 1800-2005-1 FB 1800-1005-1 FB 1800-1010-1 FB 1800-2005-1	<b>Mosaic Basic Profile 1</b> cell nuclei (ANA) mitochondria (AMA) smooth muscles (ASMA)	IgG	3 BIOCHIPS per field: HEp-2 cells kidney stomach	human rat rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides)
FA 1800-1005-2 FA 1800-1010-2 FA 1800-2005-2 FA 1800-2010-2 FA 1800-12010-2 FB 1800-1005-2 FB 1800-1010-2 FB 1800-2005-2 FB 1800-2010-2	<b>Mosaic Basic Profile 2</b> cell nuclei (ANA), LKM mitochondria (AMA), LKM smooth muscles (ASMA)	IgG	3 BIOCHIPS per field: liver kidney stomach	rat rat rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides)
FC 1800-1010-2 FC 1800-2005-2 FC 1800-2010-2 FC 1800-12010-2	<b>Mosaic Basic Profile 2 EUROPattern</b> cell nuclei (ANA), LKM mitochondria (AMA), LKM smooth muscles (ASMA)	IgG	3 BIOCHIPS per field: liver kidney stomach	rat rat rat	10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system)
FA 1800-1005-3 FA 1800-1010-3 FA 1800-2005-3 FB 1800-1005-3 FB 1800-1010-3 FB 1800-2005-3	<b>Mosaic Basic Profile 3</b> cell nuclei (ANA) cell nuclei (ANA) mitochondria (AMA) smooth muscles (ASMA)	IgG	4 BIOCHIPS per field: HEp-2 cells liver kidney stomach	human monkey rat rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides)
FA 1802-1005-3 FA 1802-1010-3 FA 1802-2005-3 FA 1802-2010-3 FB 1802-1005-3 FB 1802-1010-3 FB 1802-2005-3 FB 1802-2010-3	<b>Mosaic Basic Profile 3A</b> cell nuclei (ANA) cell nuclei (ANA) mitochondria (AMA) smooth muscles (ASMA)	IgG	4 BIOCHIPS per field: HEp-20-10 cells liver kidney stomach	human monkey rat rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides)
FC 1802-1005-3 FC 1802-1010-3 FC 1802-2005-3 FC 1802-2010-3	<b>Mosaic Basic Profile 3A EUROPattern</b> cell nuclei (ANA) EUROPattern cell nuclei (ANA) mitochondria (AMA) smooth muscles (ASMA)	IgG PI	4 BIOCHIPS per field: HEp-20-10 cells liver kidney stomach	human monkey rat rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FA 1805-1005-13 FA 1805-1010-13 FA 1805-2005-13 FB 1805-1005-13 FB 1805-1010-13 FB 1805-2005-13	<b>Mosaic Basic Profile 13B</b> cell nuclei (ANA) cell nuclei (ANA), LKM mitochondria (AMA), LKM smooth muscles (ASMA)	IgG	4 BIOCHIPS per field: HEp-2 cells kidney stomach	human rat rat rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides)
FC 1805-1010-13 FC 1805-2005-13 FC 1805-2010-13	<b>Mosaic Basic Profile 13B EUROPattern</b> cell nuclei (ANA), EUROPattern cell nuclei (ANA), LKM mitochondria (AMA), LKM smooth muscles (ASMA)	IgG PI	4 BIOCHIPS per field: HEp-2 cells liver kidney stomach	human rat rat rat	10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FA 1812-1005-3 FA 1812-1010-3 FA 1812-2005-3 FA 1812-0010-3 FB 1812-1005-3 FB 1812-1010-3 FB 1812-2005-3 FB 1812-0010-3	<b>Mosaic Basic Profile 3C</b> cell nuclei (ANA) cell nuclei (ANA), LKM mitochondria (AMA), LKM smooth muscles (ASMA)	IgG	4 BIOCHIPS per field: HEp-20-10 cells liver kidney stomach	human rat rat rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 100 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 100 x 10 (single slides)



## Diagnostics for Indirect Immunofluorescence: Systemic Autoantibodies

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FC 1812-1005-3 FC 1812-1010-3 FC 1812-2005-3 FC 1812-0010-3	<b>Mosaic Basic Profile 3C EUROPattern cell nuclei (ANA), EUROPattern cell nuclei (ANA), LKM mitochondria (AMA), LKM smooth muscles (ASMA)</b>	IgG PI	4 BIOCHIPS per field: HEp-20-10 cells liver kidney stomach	human rat rat rat	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 100 x 10 (test system)
FA 1913-1005 A FA 1913-1010 A FA 1913-2005 A FB 1913-1005 A FB 1913-1010 A FB 1913-2005 A	<b>endomysium</b>	IgA	small intestine	monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides)
FA 1913-1005-1 A FA 1913-1010-1 A FA 1913-2005-1 A FB 1913-1005-1 A FB 1913-1010-1 A FB 1913-2005-1 A	<b>EUROPLUS endomysium gliadin (GAF-3X)</b>	IgA	2 BIOCHIPS per field: small intestine gliadin (GAF-3X) BIOCHIPS	monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides)
FA 1914-1005 A FA 1914-1010 A FA 1914-2005 A FA 1914-2010 A FA 1914-12010 A FA 1914-1005 G FA 1914-1010 G FA 1914-2005 G FA 1914-12010 G FB 1914-1005 A FB 1914-1010 A FB 1914-2005 A FB 1914-2010 A FB 1914-1005 G FB 1914-1010 G FB 1914-2005 G	<b>endomysium</b>	IgA     IgGpa    IgA    IgGpa	liver	monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 120 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 120 x 10 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 20 x 10 (single slides) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides)
FC 1914-1005 A FC 1914-1010 A FC 1914-2005 A FC 1914-2010 A FC 1914-1005 G FC 1914-1010 G FC 1914-2005 G FC 1914-2010 G	<b>Coeliac Disease Screen (LM) EUROPattern endomysium</b>	IgA    IgGpa	liver	monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FA 1914-1005-1 A FA 1914-1010-1 A FA 1914-2005-1 A FA 1914-1005-1 G FA 1914-1010-1 G FA 1914-2005-1 G FB 1914-1005-1 A FB 1914-1010-1 A FB 1914-2005-1 A FB 1914-1005-1 G FB 1914-1010-1 G FB 1914-2005-1 G	<b>EUROPLUS endomysium gliadin (GAF-3X)</b>	IgA   IgGpa   IgA   IgGpa	2 BIOCHIPS per field: liver gliadin (GAF-3X) BIOCHIPS	monkey	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides) 10 x 05 (single slides) 10 x 10 (single slides) 20 x 05 (single slides)


**Diagnostics for Indirect Immunofluorescence: Systemic Autoantibodies**

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FA 1914-1005-2 A	<b>endomysium</b>	IgA	liver small intestine (2 BIOCHIPS per field)	monkey monkey	10 x 05 (test system)
FA 1914-1010-2 A					10 x 10 (test system)
FA 1914-2005-2 A					20 x 05 (test system)
FB 1914-1005-2 A					10 x 05 (single slides)
FB 1914-1010-2 A					10 x 10 (single slides)
FB 1914-2005-2 A					20 x 05 (single slides)
FA 1960-1005	<b>endothelial cells</b>	IgG	HUVEC	human	10 x 05 (test system)
FA 1960-1010					10 x 10 (test system)
FB 1960-1005					10 x 05 (single slides)
FB 1960-1010					10 x 10 (single slides)


**Diagnostics for Indirect Immunofluorescence: Further Antigens**

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields	
FV 2841-1005 A	<b>Saccharomyces cerevisiae</b>	IgA	fungal smear	Saccharomyces cerevisiae	10 x 05 (test system)	
FV 2841-1010 A					10 x 10 (test system)	
FV 2841-2005 A					20 x 05 (test system)	
FV 2841-1005 G					IgG	10 x 05 (test system)
FV 2841-1010 G						10 x 10 (test system)
FV 2841-2005 G						20 x 05 (test system)
FX 2841-1005		10 x 05 (single slides)				
FX 2841-1010		10 x 10 (single slides)				
FX 2841-2005		20 x 05 (single slides)				

For individual test kit controls please contact your respective sales representative.



# Infection diagnostics







# Bacteria

Bordetella · Borrelia · Treponema · Chlamydia




For more information on this subject scan the QR code or enter the Quick Link code **q008** at [www.euroimmun.com](http://www.euroimmun.com)

## Bordetella

■ **Clinical information:** *Bordetella pertussis* is the causative agent of whooping cough, a disease with 3 stages: 1. Catarrhal stage: mild flu-like symptoms; lasting 1 to 2 weeks; 2. Paroxysmal stage: fits of (staccato-like) coughing spasms with "whooping" sound when inhaling; lasting 2 to 3 weeks; 3. Convalescent stage: slow convalescence, which can take up to several months. Complications such as secondary pneumonia or otitis media are possible, especially in children under the age of 2 years. The disease is known in adults, but is rarely diagnosed, even though coughing adults can infect their surroundings. An infection confers specific immunity, which reduces after several years. The clinical progression of whooping cough depends mainly on the production of the different virulence factors (adhesins and toxins), such as filamentous haemagglutinin (FHA) or pertussis toxin (PT). PT is the only antigen that is exclusively produced by *B. pertussis*. FHA is found in all other *Bordetella* species and also in other bacteria.

■ **Diagnostics:** The method of detection for the diagnosis of *Bordetella* infection depends on the disease stage. Direct detection of the pathogen (culture, PCR) is particularly useful in the early stages of infection. Since the pathogen is often no longer detectable after around four weeks following infection, serology gains importance as the disease proceeds. Pathogen-specific antibodies of classes IgA and IgG can generally be detected from the paroxysmal stage. For antibody detection, international reference laboratories recommend test systems that are based on individual purified antigens. The use of antigen mixtures of PT and FHA is obsolete. The quantification of antibody titers should be performed in international units (IU/ml) according to the 1<sup>st</sup> International Standard of the WHO (1<sup>st</sup> IS NIBSC Code 06/140). The detection of anti-PT IgG is of particular importance for specific diagnosis of *B. pertussis* infection. A concentration of  $\geq 100$  IU/ml is considered a clear indicator of *B. pertussis* infection. If the anti-PT IgG concentration is below 40 IU/ml, acute *B. pertussis* infection is unlikely. In cases of unclear serological anti-PT IgG levels of between  $\geq 40$  and  $< 100$  IU/ml the investigation of further antibodies such as anti-PT IgA can provide additional information. Diagnosis can be confirmed if a significant change in the antibody concentration is found in two consecutive samples. It should be taken into account that a positive antibody result up to one year after vaccination is not a reliable indicator of acute infection.

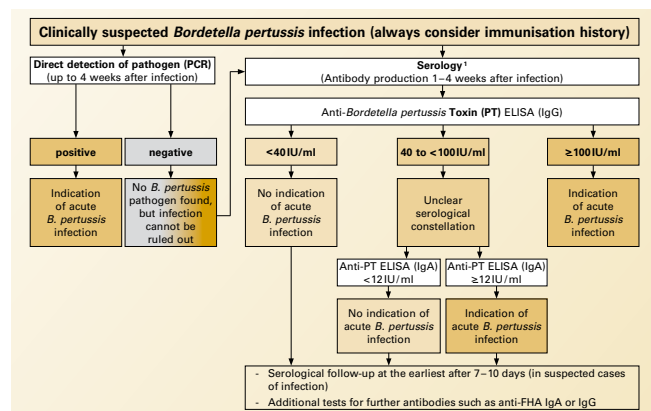

\*The clinical symptoms and age of the patient should always be taken into account.





## Product overview

Method	Substrate	Application	Order number	Page
ELISA	Highly purified pertussis toxin, PT	IgG ELISA: Most important serological test; specific for <i>B. pertussis</i> ; exclusion of <i>B. parapertussis</i> infections; quantification in IU/ml; interpretation according to 40/100 IU/ml limits	EI 2050-9601 G	197
	Highly purified pertussis toxin, PT	PT IgA; FHA IgA/G ELISA: useful for ambiguous anti-PT IgG titers in the range of $\geq 40$ to $< 100$ IU/ml; quantification in IU/ml	EI 2050-9601 A	197
	Highly purified filamentous haemagglutinin, FHA		EI 2050-9601-3 A/G	197
Blot	PT, FHA, ACT (adenylate cyclase toxin)	Additional qualitative test; antibodies against ACT can indicate a natural infection (ACT is currently not contained in acellular vaccines)	DN 2050-#### A/G	194



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q059** at [www.euroimmun.com](http://www.euroimmun.com)



# Bacteria

Bordetella · Borrelia · Treponema · Chlamydia




For more information on this subject scan the QR code or enter the Quick Link code **q009** at [www.euroimmun.com](http://www.euroimmun.com)

## Borrelia

■ **Clinical information:** Borrelia is the causative agent of Lyme borreliosis, a bacterial disease which is transmitted through bites from ticks of the genus Ixodes and is characterised by a variety of clinical symptoms. The most important human pathogenic Borrelia genospecies are *B. afzelii*, *B. burgdorferi* and *B. garinii*. Lyme borreliosis can manifest itself dermatologically, neurologically or through internal disorders. The radially spreading *erythema migrans* is a characteristic early symptom, which occurs a few days to several weeks after the infection. This is often accompanied by influenza-like general symptoms, such as fever, shivering, headaches and vomiting. The advanced stage of the disease is characterised by neurological (e.g. facial paresis), cardiac (e.g. myocarditis) and rheumatological (e.g. arthritis) manifestations. In chronic Lyme borreliosis involvement of the joints, epidermis (acrodermatitis chronica atrophicans) and central nervous system as well as fatigue are typically found.


■ **Diagnostics:** The diagnosis of Lyme disease is based on the patient anamnesis, clinical findings and the detection of antibodies against Borrelia antigens. For the serological diagnosis of anti-Borrelia-specific antibodies, the German Association for Hygiene and Microbiology (DGHM), the Robert Koch Institute and the CDC (Atlanta, Georgia) call for a two-stage strategy. Firstly, a sensitive screening test (ELISA, ChLIA or IIFT) is performed. Sera with a positive or borderline screening result are investigated further using an immunoblot to differentiate between Borrelia-specific and unspecific reactions. Since antibodies against Borrelia are first produced 2 to 6 weeks after infection, serological tests performed in the early stage of Lyme borreliosis can be negative. Early antibiotic treatment may also prevent antibody production. In suspected cases of neuroborreliosis, the presence of intrathecal synthesis of Borrelia-specific antibodies can be investigated by parallel analysis of a CSF/serum sample.

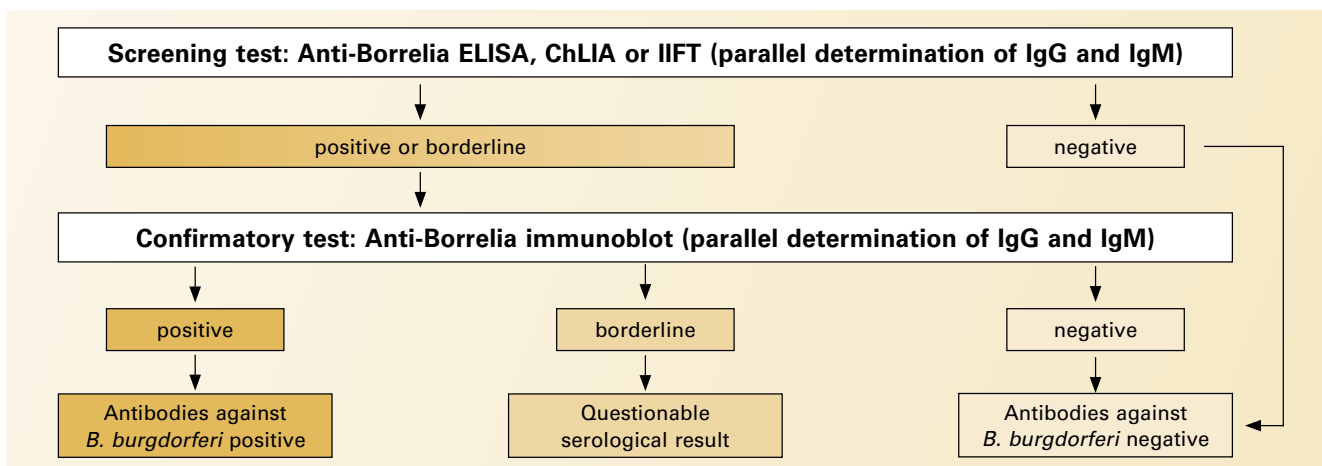



## Product overview

Method	Substrate	Application	Order number	Page
ELISA	Whole antigen, detergent extract of <i>B. burgdorferi</i> , <i>B. garinii</i> and <i>B. afzelii</i> plus recombinant VlsE	IgG ELISA: complete antigen spectrum incl. VlsE, high sensitivity	EI 2132-9601-2 G	197
	Whole antigen, detergent extract of <i>B. burgdorferi</i> , <i>B. garinii</i> and <i>B. afzelii</i>	IgM ELISA: complete antigen spectrum incl. OspC, high sensitivity	EI 2132-9601 M	197
	Mix of recombinant Borrelia antigens incl. VlsE (IgG) or dimeric OspC advanced (IgM)	Especially selected highly specific antigens, reduced cross reactivity	EI 2132-9601-5 G/M	197
ChLIA	IgG: VlsE of different Borrelia species, DbpA IgM: OspC advanced of different Borrelia species	Chemiluminescence tests for the random access instrument RA Analyzer 10	LI 2132-10010 G/M (control set: LR 2132-20210 G/M)	204
Blot	IgG: p18, p19, p20, p21, p58, OspC, p39, p41, p83, LBb, LBa, VlsE Bg, VlsE Bb, VlsE Ba IgM: OspC Bg, OspC Bb, OspC Ba, p39, p41, VlsE Bb	Line blots with diagnostically relevant Borrelia antigens incl. VlsE and OspC from different Borrelia species; simple evaluation	DN 2131-#### G/M	194
	OspC-adv Bsp, OspC-adv Bg, OspC-adv Bb, OspC-adv Ba, p39, p41, VlsE Bb	IgM line blot with rec. Borrelia antigens incl. dimeric OspC advanced	DN 2131-####-2 M	194
	IgG: p100, p41, p39, p18, OspC, VlsE Bg, VlsE Bb, VlsE Ba IgM: p39, p41, VlsE, OspC Ba, OspC Bb, OspC Bg, OspC Bsp	EUROMicroblot: line blots in microplate format; automatable with ELISA processors	KN 2131-9601 G/M	196

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 205).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **c060** at [www.euroimmun.com](http://www.euroimmun.com)



# Bacteria

Bordetella · Borrelia · Treponema · Chlamydia



For more information on this subject scan the QR code or enter the Quick Link code **q044** at [www.euroimmun.com](http://www.euroimmun.com)

## Treponema pallidum

■ **Clinical information:** *Treponema pallidum* is the pathogenic agent of syphilis (*lues*), a worldwide occurring, sexually or diaplacentally transmitted infection that is divided into 4 stages. 1. Primary stage: The typical primary manifestation is a clearly defined fibrous or crusted erosion at the site of infection which occurs about three weeks after infection. An ulcer or a hardening of the lesion can develop (hard chancre). Local lymph nodes become swollen within a week. 2. Secondary stage: In addition to a generalised swelling of the lymph nodes, 90% of patients show local or generalised skin disorders. Various organ disorders may develop, for example, keratitis, iritis, hepatitis, vasculitis, and myocardial disorders. Secondary syphilis is followed by a clinically silent stage (*syphilis latens*), which can last for years. 3. Tertiary stage: Typical manifestations are large papules and ulcers on the skin and mucous membranes, as well as organ or visceral syphilis, perivasculitis, cardiovascular syphilis, osteitis and periostitis. 4. Quaternary stage: Severe neurological disorders in the form of neurosyphilis can occur up to 30 years after the initial infection. Diaplacental transmission of the pathogen causes congenital syphilis.

■ **Diagnostics:** The diagnosis of syphilis is based on clinical findings according to the disease stage, pathogen detection (from the primary lesion) and serological detection of antibodies against *T. pallidum*. The focus of laboratory diagnostics lies in antibody detection, which has proven successful with a three-staged diagnostic procedure consisting of screening, confirmation and evaluation of the disease activity.

Screening can be performed using Treponema-specific agglutination tests (TPPA, TPHA) and polyvalent enzyme immunoassays. Useful confirmatory tests are ELISA, FTA-abs test and immunoblots. Due to blood vessel inflammation and tissue damage the activity of the infection correlates with the antibody titer against mitochondrial lipids (cardiolipin), which can be detected using the RPR (rapid plasma reagin) test or VDRL (venereal disease research laboratory) test.



## Product overview

Method	Substrate	Application	Order number	Page
ELISA	Antigen mixture of <i>T. pallidum</i> (p15, p17, p47 and TmpA)	Screening test; sensitive detection of <i>T. pallidum</i> -specific Ab (mixed conjugate IgG+IgM); very good correlation with TPHA/TPPA	EI 2111-9601 O	197
	Antigen mixture of <i>T. pallidum</i> (p15, p17, p47 and TmpA)	Confirmatory test; separate detection of <i>T. pallidum</i> -specific IgG or IgM antibodies	EI 2111-9601 G/M	197
Blot	Electrophoretically separated antigens of <i>T. pallidum</i> plus purified cardiolipin	Confirmatory test and information on disease activity by evaluation of the cardiolipin band	DY 2111-#### G/M	195
	<i>T. pallidum</i> -specific antigens (TpN15, TpN17, TmpA, TpN47)	Confirmatory test; separate detection of <i>T. pallidum</i> -specific antibodies by line blot	DN 2111-#### G/M	194
IIFT (FTA-Abs)	Bacterial smears of <i>T. pallidum</i>	Confirmatory test; unspecific cross-reacting antibodies are removed by pre-adsorption of samples	FI 2111-#### G/M	209
Parameter		Application	Order number	Page
EUROArray STI - 11		PCR-based direct detection of <i>Chlamydia trachomatis</i> , <i>Neisseria gonorrhoeae</i> , HSV-1, HSV-2, <i>Haemophilus ducreyi</i> , <i>Mycoplasma genitalium</i> , <i>M. hominis</i> , <i>T. pallidum</i> , <i>Trichomonas vaginalis</i> , <i>Ureaplasma parvum</i> and <i>Ureaplasma urealyticum</i>	MN 2830-####	302



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q101** at [www.euroimmun.com](http://www.euroimmun.com)



# Bacteria

Bordetella · Borrelia · Treponema · Chlamydia



For more information on this subject scan the QR code or enter the Quick Link code **q010** at [www.euroimmun.com](http://www.euroimmun.com)

## Chlamydia

■ **Clinical information:** The infectious agents *Chlamydia trachomatis*, *Chlamydia pneumoniae* and *Chlamydia psittaci* belong to the human pathogenic Chlamydia genus.


*Chlamydia trachomatis* can cause the following diseases: 1. Trachoma, a tropical eye infection (serotypes A-C); 2. Infections of the urogenital tract (serotypes D-K). Non-gonorrhoeal urethritis is one of the most common venereal diseases worldwide. Secondary effects of *C. trachomatis* infection can be reactive arthritis, secondary sterility or infertility. 3. Lymphogranuloma venereum (LGV), a rare venereal disease which occurs mainly in tropical areas (serotypes L1-L3).

*C. pneumoniae* mostly causes infections of the upper respiratory tract and pneumonia. Around half of infections proceed asymptotically. More than 50% of adults have been infected with *C. pneumoniae* and exhibit antibodies against the pathogen.

*C. psittaci* is the causative agent of psittacosis, an infection transmitted to humans by domesticated birds. In addition to flu-like symptoms, a life-threatening pneumonia can develop during the course of the infection, which is often accompanied by further organ manifestations.

■ **Diagnostics:** Pathogen detection (e.g. using PCR) is the method of choice for the diagnosis of acute urogenital *C. trachomatis* infection. In *sequelae* associated with *C. trachomatis* such as sterility or reactive arthritis, direct detection of the pathogen is mostly no longer possible. In these cases the investigation of IgA and IgG antibodies is of importance.

Since the diagnosis of *C. pneumoniae* infections in humans by means of symptoms or radiography is not entirely reliable, laboratory diagnostics play a significant role. Detection of the pathogen is useful in the diagnosis of acute infection, but often fails if the infection is older. The analysis of specific Chlamydia antibodies (IgA, IgG, IgM) can help with diagnosing primary infection and reinfection. A significant increase in the IgG antibody level or a seroconversion in two serum samples taken at an interval of several weeks indicates acute infection with *C. pneumoniae*.




Specific antibodies against Chlamydia antigens can be detected using MIF (micro-immunofluorescence) assay, ELISA or immunoblot. Since the three Chlamydia species have the same cell wall proteins (such as lipopolysaccharids, LPS) and are therefore very similar, cross-reactions cannot be ruled out. The inactivation of LPS antigens in the MIF minimises cross reactivity. Type-specific membrane proteins (MOMP: major outer membrane protein) are also suited for species-specific antibody detection.





## Product overview

Method	Substrate	Application	Order number	Page
ELISA	Native MOMP (major outer membrane protein) antigen of <i>C. trachomatis</i>	Species-specific detection by use of type-specific MOMP antigen	EI 2191-9601 A/G	198
	Cell lysate of <i>C. pneumoniae</i>	Genus-specific detection; sensitive detection of anti- <i>C. pneumoniae</i> Ab	EI 2192-9601 A/G/M	198
Blot	SDS extract of <i>C. trachomatis</i> plus membrane chips with antigens of <i>C. trachomatis</i> , <i>C. pneumoniae</i> and <i>C. psittaci</i>	Parallel detection of Ab against the three human pathogenic (HP) Chlamydia species <i>C. trachomatis</i> , <i>pneumoniae</i> and <i>psittaci</i>	DY 2190-1601-1 A/G	196
IFT (MIF)	Elementary bodies of <i>C. trachomatis</i> , <i>C. pneumoniae</i> , <i>C. psittaci</i> and control BIOCHIP with non-infected cells	Species-specific detection (cross-reacting LPS Ag are inactivated); simple evaluation due to use of optimised substrates; secure differentiation between unspecific and specific fluorescences by means of control BIOCHIP	FI 2191-####-3 A/G/M FR 2191-####-3 A/G/M (EUROPattern)	209
Parameter		Application	Order number	Page
EUROArray STI - 11		PCR-based direct detection of <i>C. trachomatis</i> , <i>N. gonorrhoeae</i> , <i>HSV-1</i> , <i>HSV-2</i> , <i>H. ducreyi</i> , <i>M. genitalium</i> , <i>M. hominis</i> , <i>T. pallidum</i> , <i>T. vaginalis</i> , <i>U. parvum</i> and <i>U. urealyticum</i>	MN 2830-####	302

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 205).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q061** at [www.euroimmun.com](http://www.euroimmun.com)



# Viruses

SARS-CoV-2 · EBV · HEV



For more information on this subject scan the QR code or enter the Quick Link code **q168** at [www.euroimmun.com](http://www.euroimmun.com)

## SARS-CoV-2

■ **Clinical information:** Severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2, previously called 2019-nCoV) belongs to the family of coronaviruses and, like SARS-CoV, is classified in the genus Betacoronavirus. At the end of 2019, it caused an infection wave that rapidly spread worldwide and was declared a pandemic by the WHO in March 2020. Just a few days after the first report about patients with pneumonia of unclear origin, SARS-CoV-2 was identified as the causative pathogen and the associated disease named COVID-19. SARS-CoV-2 is mainly transmitted via aerosols during speaking, breathing, coughing or sneezing or at close contact with an infected person. The incubation period is usually three to seven, maximally 14 days. The symptoms and severity of SARS-CoV-2 infection can vary significantly. The most common symptoms encompass fever, coughing, breathing difficulties and fatigue. Therefore, in the majority of patients, the infection resembles a cold with light fever, with irregular lung infiltrates. Some patients, especially older and chronically ill persons, develop acute respiratory distress syndrome.

■ **Diagnostics:** Suitable methods for the diagnosis of SARS-CoV-2 infections are the detection of viral RNA by reverse transcriptase polymerase chain reaction (RT-PCR) or of virus protein by means primarily in sample material from the upper (nasopharyngeal or oropharyngeal swab) or lower respiratory tract (bronchoalveolar lavage fluid, tracheal secretion, sputum, etc.). The PCR allows detection of the pathogen even in subclinical or asymptomatic courses already few days after virus contact and up to 14 after onset of possible symptoms. The determination of antibodies enables confirmation of SARS-CoV-2 infection in patients with typical symptoms and in suspected cases. It also contributes to monitoring and outbreak control. For significant serological results, two patient samples should be investigated, one from the acute phase (week 1 of the illness) and one from the convalescent phase (three to four weeks later).

EUROIMMUN offers the complete range of test systems for COVID-19 diagnostics: RT-PCR for acute diagnostics, serological tests for differentiated detection of antibodies of different immunoglobulin classes and against different SARS-CoV-2 antigens, and an interferon gamma release assay (IGRA) to measure the cellular immune response.



## Product overview

Method	Substrate	Application	Order number	Page
ELISA	S1 domain of the spike protein of SARS-CoV-2	Detection of IgA or IgG antibodies against SARS-CoV-2	EI 2606-#### A/G	200
	Modified nucleocapsid protein (NCP) of SARS-CoV-2	Detection of IgG antibodies against SARS-CoV-2	EI 2606-####-2 G	200
	S1 domain of the spike protein of SARS-CoV-2	Quantitative determination of IgG antibodies against SARS-CoV-2	EI 2606-9601-10 G	200
	S1 domain of the spike protein of SARS-CoV-2 and human ACE2 (liquid phase)	Surrogate virus neutralisation test (sVNT) in ELISA format	EI 2606-9601-4	200
IGRA	Based on the S1 domain of the spike protein of SARS-CoV-2	Set of SARS-CoV-2 stimulation tubes (to be combined with EQ 6841-9601)	ET 2606-3003	207
	Anti-interferon gamma antibody	Determination of the cellular immune response to SARS-CoV-2	EQ 6841-9601	207
Blot	Recombinant SARS-CoV-2 antigens: S1, S2, NP	Line blot for separate determination of IgG antibodies against antigens of SARS-CoV-2	DN 2606-####-1 G	195
Parameter	Sample material	Application	Order number	Page
EURORealTime SARS-CoV-2	RNA from throat swabs	Real-time PCR-based direct detection of SARS-CoV-2	MP 2606-####	303
EURORealTime SARS-CoV-2/ Influenza A/B	RNA from throat swabs	Real-time PCR-based direct detection of SARS-CoV-2 and influenza viruses A and B	MP 2606-####-20	303



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q168** at [www.euroimmun.com](http://www.euroimmun.com)



# Viruses

SARS-CoV-2 · EBV · HEV



For more information on this subject scan the QR code or enter the Quick Link code **q013** at [www.euroimmun.com](http://www.euroimmun.com)

## Epstein-Barr virus


■ **Clinical information:** Epstein-Barr virus (EBV) is the causative agent of infectious mononucleosis (glandular fever), a febrile disease usually accompanied by pharyngitis and lymphadenopathy, frequently by hepatosplenomegaly and more rarely by exanthema. Recent research results have also shown a connection between EBV infection and the pathogenesis of Burkitt's lymphoma and nasopharyngeal carcinoma (NPC). In pregnancy, EBV can cause infection of the placenta, leading to damage to the foetal heart, eyes and liver. In children, accompanying infections of the kidney have been observed with symptoms from microscopic haematuria to acute kidney failure.

■ **Diagnostics:** Infectious mononucleosis must be differentiated diagnostically from cytomegaly and toxoplasmosis and, in the case of atypical progress, also from infections with HIV and other pathogens.

The main goal of routine diagnostics is to differentiate between the stages of an EBV infection, for example primary or past infection. Infections are in most cases confirmed by serological detection of antibodies. Determination of the viral load by PCR is useful in immunosuppressed patients and in chronic active EBV infections.

During the course of an EBV infection the antibodies appear successively. In the early phase of the disease, IgM and IgG antibodies against EBV capsid antigen (EBV-CA) are detectable. A positive anti-EBV-CA (IgM) result is the classic marker of an acute infection. IgG antibodies against the early antigen (EA) occur somewhat later in the acute phase and decline to an undetectable concentration after three to six months. In contrast, the CA IgG antibody level persists lifelong. Around six to eight weeks after an infection, antibodies against Epstein-Barr nuclear antigen (EBNA) are produced. Their occurrence thus indicates a past infection.


Serologically difficult constellations, such as persistent anti-EBV-CA IgM antibodies, the absence of specific anti-EBV-CA IgM antibodies in acute infections or secondary loss of anti-EBNA IgG antibodies, can be clarified by measuring the avidity of anti-EBV-CA IgG antibodies and/or by the detection of further late-phase markers by immunoblot.





## Product overview

Method	Substrate	Application	Order number	Page
ELISA	Mixture of native EBV capsid antigens (EBV-CA)	IgG/IgA ELISA: complete Ag spectrum ensures high sensitivity and high specificity; avidity determination: exclusion of acute infection	EI 2791-9601 A/G EI 2791-9601-1 G	202 202
	Native EBV-CA gp125	IgM ELISA: optimal for the diagnosis of acute infection	EI 2791-9601 M	202
	Recombinant EBNA-1 antigen	High specificity for the late stage of the disease	EI 2793-9601 G	202
	Recombinant EBV early antigen D (EBV-EA-D)	Highly specific recombinant antigen	EI 2795-9601 A/G/M	202
ChLIA	Recombinant EBV capsid antigens (p18, p23, gp125)	IgG ChLIA: antigen spectrum ensures high sensitivity and specificity	LI 2791-10010 G (control set: LR 2791-20210 G)	204
	Recombinant EBV capsid antigens (p18, gp125)	IgM ChLIA: optimal for the diagnosis of acute infections	LI 2791-10010 M (control set: LR 2791-20210 M)	204
	Recombinant EBNA-1 antigen	IgG ChLIA: high specificity for the late phase of the disease	LI 2793-10010 G (control set: LR 2793-20210 G)	204
Blot	EBV Profile 2: separate EBV-CA gp125, EBV-CA p19, EBNA-1, p22, EA-D	Line blot with all relevant EBV antigens for the diagnosis and differentiation of early-stage and late-stage EBV infections	DN 2790-####-2 G/M	195
IIFT	BIOCHIP sequence: EBV-CA (avidity test, IgG, IgM), EBV-EA, EBNA; infected cells	IIFT is the gold standard for EBV diagnostics; BIOCHIP sequence contains all relevant antigens; avidity determination: exclusion of acute infection	FI 2799-####-1 X	229
	EUROPLUS sequence: EBV-CA (avidity test, IgG, IgM, gp125-Ag, p19-Ag), EBV-EA, EBNA; infected cells		FI 2799-####-21 X	229

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 205).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q066** at [www.euroimmun.com](http://www.euroimmun.com)



# Viruses

SARS-CoV-2 · EBV · HEV



For more information on this subject scan the QR code or enter the Quick Link code **q026** at [www.euroimmun.com](http://www.euroimmun.com)

## Hepatitis E virus

■ **Clinical information:** Hepatitis E virus (HEV) is the causative agent of hepatitis E, a worldwide distributed infectious disease. HEV is an uncoated RNA virus of the *Hepeviridae* family. Four human pathogenic genotypes of HEV have so far been described (1–4). While genotypes 1 and 2 are exclusively human pathogenic, genotypes 3 and 4 are found in humans and animals. The most common ways of infection include faecal-oral transmission through consumption of contaminated drinking water or food (endemic areas with low hygienic standards) and zoonotic transmission by the consumption of insufficiently cooked meat from infected animals, e.g. domestic or wild pigs (industrialised countries). Virus-contaminated blood products are also discussed as a potential source of infection for humans.

Infections with HEV usually proceed asymptotically or mildly with unspecific symptoms such as tiredness, loss of appetite, nausea, vomiting, headache and muscle and joint pains. If liver inflammation occurs, it is often self-limiting and heals without any complications. In rare cases hepatitis E can have a fulminant course with acute liver failure. Pregnant women with a history of severe disease courses are particularly at risk. Up to 20% of HEV infections are fatal for the expectant mother (lethality in hepatitis E infections in the total population: 0.5 to 4%).

■ **Diagnostics:** Since the clinical picture of hepatitis E resembles hepatitis A as well as other hepatitides, laboratory diagnostic methods are of major importance for diagnosis. Besides PCR detection of viral RNA in blood or stool (recommended method for very early phase of infection) the serological determination of antibodies of class IgA/IgG/IgM against hepatitis E virus is the most important tool for confirming HEV infections. Pathogen-specific antibodies are often detectable at or shortly after the onset of clinical symptoms. A positive IgA and/or IgM result and a significant IgG titer increase in a serum pair (taken at an interval of 8 to 14 days) indicate an acute infection. Anti-HEV IgA and IgM titers generally decrease rapidly after infection, while anti-HEV IgG titer often persist for more than 10 years.





## Product overview

Method	Substrate	Application	Order number	Page
ELISA	Recombinant target antigens of HEV genotypes 1 and 3	IgG ELISA; test for the quantitative determination of IgG antibodies against HEV	EI 2525-9601 G	199
		IgM ELISA: detection of HEV-specific antibodies of class IgM with high specificity and sensitivity	EI 2525-9601 M	199
		Screening ELISA for parallel determination of IgA, IgG and IgM antibodies against HEV	EI 2525-9601 P	199
Blot	Recombinant ORF2 antigens of the HEV genotypes 1, 2, 3 and 4	Line blot for determination of IgA, IgG or IgM antibodies against HEV	DN 2525-#### A/G/M	194



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q070** at [www.euroimmun.com](http://www.euroimmun.com)



# Funguses

## Aspergillus



For more information on this subject scan the QR code or enter the Quick Link code **q157** at [www.euroimmun.com](http://www.euroimmun.com)

# Aspergillus

■ **Clinical information:** Moulds of the genus *Aspergillus* are present in the air and soil, but also in biological waste and contaminated foods. Within the genus, which encompasses more than 300 species, some may lead to infections in humans, given the respective predisposition. Here, *Aspergillus fumigatus* plays an especially important role. Infections with other species such as *A. flavus*, *A. niger*, *A. terreus* were also described. Transmission occurs via inhalation of spores, of which humans inhale up to several hundred every day. In patients with an intact immune system, this intake does not lead to an infection since the spores can be controlled by the cellular immune system. In the beginning, a permanent load may cause hypersensitivity or allergic reactions (allergic bronchopulmonary aspergillosis, ABPA). With existing lung damage, e.g. destructed lung tissue due to tuberculosis, an aspergilloma, that is, a tumour-like growth may develop.

In patients with weakened immune system or immunosuppression, infections often lead to invasive aspergillosis. Initially, this manifests mainly in the respiratory tracts and the sinuses, but may also disseminate haematogenically and consequently affect organs such as the brain, liver and kidneys. This is usually accompanied by unspecific symptoms such as high fever and inflammation of the affected organs and may affect the central nervous system. Especially haemato-oncological and bone-marrow-transplanted patients are mostly affected. However, also other immune deficiencies, e.g. due to HIV infections or treatments with glucocorticoids, may favour an infection. In the last years, an increasing number of nosocomial infections were observed in patients in intensive care units. According to studies, up to 20% of the group of bone-marrow-transplanted patients were affected by an invasive fungal infection. Here, aspergilloses and candidiases are the most relevant infections. Depending on the manifestation, 50 to 90% of invasive aspergilloses are fatal.

■ **Diagnostics:** The laboratory diagnostic detection is based on cultivation or microscopy. However, cultivation is only successful in 50% of cases. The detection of *Aspergillus* antigen from body fluids is nowadays an established additional method. This enables sensitive *Aspergillus* detection already at an early stage. Due to this reason, detection of *Aspergillus* antigens was included in the guidelines of the European Organization for Research and Treatment of Cancer (EORTC) and the National Institute of Allergy and Infectious Diseases Mycoses Study Group (MSD) as a criterion of a “probable” invasive aspergillosis. Established test systems are based on the detection of polysaccharides from the cell wall.



## Product overview

Method	Substrate	Application	Order number	Page
Antigen ELISA	Antibodies against a glycosylated cell wall protein of <i>Aspergillus</i> (extracellular part)	Sensitive detection for the support to the diagnosis of acute aspergilloses	EQ 6911-9601	261
IIFT	<i>Candida albicans</i> smears	Separate detection of different antibodies classes against <i>Candida albicans</i>	FI 2861-#### A, G or M	228
Parameter		Application	Order number	Page
EUROArray Dermatomycosis		PCR-based molecular genetic direct detection of up to 50 dermatophytes and clear species identification of up to 23 dermatophytes and 6 yeasts/moulds	MN 2850-####	313



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q157** at [www.euroimmun.com](http://www.euroimmun.com)



# Special infection diagnostics

CSF diagnostics · TORCH · Tropical infections



For more information on this subject scan the QR code or enter the Quick Link code **q031** at [www.euroimmun.com](http://www.euroimmun.com)

## CSF diagnostics

■ **Clinical information:** The investigation of cerebrospinal fluid (CSF) is diagnostically decisive in acute or chronic inflammatory processes of the central nervous system (CNS). Acute CNS infections manifest themselves as meningitis (inflammation of the meninges), meningoencephalitis (inflammation of the brain or meninges) or encephalitis (inflammation of the brain). These infections can be caused by bacteria (e.g. *Borrelia*, *Treponema pallidum*), viruses (e.g. HSV, VZV, measles virus, TBE virus, EBV) or parasites (e.g. *Toxoplasma gondii*). CSF analysis also plays a major role in the differential diagnosis of non-infectious diseases such as multiple sclerosis (MS). The detection of intrathecal synthesis of antibodies against measles, rubella and/or varicella zoster viruses (MRZ reaction) is a specific indicator of MS.

■ **Diagnostics:** When determining an infection of the CNS it is necessary to differentiate between intrathecally produced antibodies and antibodies which have migrated from the blood into CSF. This is done by measuring the concentrations of pathogen-specific antibodies, corresponding immunoglobulin classes (total IgG, IgM) and albumin in both the CSF and serum of the patient. If an infection of the central nervous system is present, pathogen-specific antibodies accumulate in the CSF. If, however, the infection is not localised in the the brain, the distribution of pathogen-specific antibodies in CSF and serum is the same as that of total IgG. The intrathecal pathogen-specific antibody production is defined by the relative CSF/serum quotient  $CSQ_{rel}$  (synonym: antibody specificity index, AI). The quotient is calculated from the amount of specific IgG antibodies in total CSF IgG/IgM in proportion to the amount of pathogen-specific antibodies in total serum IgG/IgM. A  $CSQ_{rel} > 1.5$  indicates intrathecal synthesis of pathogen-specific antibodies.

In addition to the determination of specific antibodies, also the investigation of chemokine CXCL13 in CSF is useful for the diagnosis of neuroborreliosis. In patients with acute neuroborreliosis, in early stages of the disease, high concentrations of CXCL13 are frequently observed, often even before antibodies against *Borrelia* are detectable. CXCL13 determination can help to close the gap between infection and positive antibody test and to diagnose neuroborreliosis at an earlier stage. Moreover, CXCL13 used as activity marker helps to differentiate between acute and past neuroborreliosis. CXCL13 is also suitable as a marker for the disease course after treatment. Its concentration in CSF decreases with successful therapy. It needs to be taken into account that increased CXCL13 values can also be observed in other diseases, in particular in CNS lymphoma, HIV infections and neuro-lues.

■ **Evaluation software:** EUROIMMUN CSF software is a program for automatic calculation of CSF/serum quotients. For further information see page 84.





## Product overview

Method	Substrate	Application	Order number	Page
ELISA	Borrelia	Efficient standardised automation with uniform dilution and incubation conditions; 4-/6-point standard curve or recalibration with 1 calibrator (stored standard curve) for highest accuracy; very good reproducibility of results for the whole measurement range; excellent agreement with quality assessment results (INSTAND e.V.); automated calculation of results (EUROIMMUN CSF software); CSF/serum control pairs available for all ELISAs	EI 2132-9601-L G/M	197
	Measles virus		EI 2610-9601-L G	200
	Rubella virus		EI 2590-9601-L G	199
	Varicella zoster virus (VZV)		EI 2650-9601-L G	200
	Herpes simplex virus (HSV-1/2)		EI 2531-9601-1 L G	199
	Cytomegalovirus (CMV)		EI 2570-9601-L G	199
	Mumps virus		EI 2630-9601-L G	200
	Tick-borne encephalitis (TBE)		EI 2661-9601-L G/M	201
	Epstein-Barr virus (EBV-CA)		EI 2791-9601-L G	202
	<i>Treponema pallidum</i>		EI 2111-9601-L G	197
	<i>Toxoplasma gondii</i>	EI 2410-9601-L G	198	
Blot	Recombinant and native Borrelia antigens	Additional test for differentiated detection of antibodies in CSF and serum	DN 2131-#### G/M DN 2131-####-2 M	194
Antigen ELISA	Anti-CXCL13 antibody	Activity and therapy marker in neuroborreliosis	EQ 6811-9601-L	207
Parameter		Application	Order number	Page
EURORealTime HSV-1/2		PCR-based direct detection of HSV-1 and -2; quantification of virus DNA; differentiation between both types	MP 2530-####	303



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g078** at [www.euroimmun.com](http://www.euroimmun.com)



# Special infection diagnostics

CSF diagnostics · TORCH · Tropical infections




For more information on this subject scan the QR code or enter the Quick Link code **q043** at [www.euroimmun.com](http://www.euroimmun.com)

## TORCH

■ **Clinical information:** The term TORCH encompasses all infectious agents that can be transferred from mother to child in the uterus, during birth or after birth via vertical infection. It includes *Toxoplasma gondii*, rubella virus, cytomegalovirus (CMV), herpes simplex virus (HSV) and other pathogens such as *Chlamydia trachomatis*, parvovirus B19, *Treponema pallidum* and varicella zoster virus (VZV). Primary infections during pregnancy are especially feared, since they are associated with an increased risk of damage to the child.

■ **Diagnostics:** Nowadays, analysis of antibodies against TORCH parameters is an essential part of pre-, peri- and postnatal care. The tests allow the immune status of the mother to be established and the risks to an existing pregnancy assessed. The diagnostic procedure depends on the patient history, special risk factors and national regulations. TORCH tests are generally performed during the first trimester of pregnancy, but they can also be carried out on the newborn if an infection is suspected. The initial investigation of antibodies against TORCH pathogens is aimed at determining the immune status of the mother in order to be able to differentiate between acute primary and past infections or reactivations during the course of pregnancy. If diagnosed early, TORCH infections can in part be effectively treated, reducing the risk of birth defects or loss of the foetus. If there is no immunity against one of the TORCH pathogens, it is very important for the mother to avoid contact with known infection sources during pregnancy.








## Product overview

Method	Substrate	Application	Order number	Page
ELISA	Native whole antigen of <i>Toxoplasma gondii</i>	Complete ag spectrum; for sensitive determination of spec. IgG, IgM or IgAGM; avidity ELISA: exclusion of primary infections	EI 2410-9601 P	198
			EI 2410-9601 G/M	198
			EI 2410-9601-1 G	198
	Purified native antigens (IgG) and glycoproteins (IgM) of rubella virus	IgG ELISA: complete ag spectrum; IgM ELISA: highest specificity through the use of viral glycoproteins; Avidity ELISA: exclusion of primary infections	EI 2590-9601 G	199
			EI 2590-9601-1 G	199
			EI 2590-9601-2 M	199
Purified native antigens of cytomegalovirus	IgG, IgM ELISA: complete antigen spectrum; Avidity ELISA: exclusion of primary infections	EI 2570-9601 G/M	199	
		EI 2570-9601-1 G	199	
		EI 2570-9601-2 M	199	
Recombinant p52 (IgM) or glycoprotein B antigen (IgG) of cytomegalovirus	ELISA with reduced cross-reactivity (IgM) or for excluding primary infections (IgG)	EI 2570-9601-2 M	199	
		EI 2570-9601-3 G	199	
		EI 2570-9601-3 G	199	
Mixture of HSV-1 and -2 whole antigens	Determination of IgG or IgM antibodies against both HSV species	EI 2531-9601-1 G/M	199	
		EI 2531-9601-2 G	199	
		EI 2532-9601-2 G	199	
Glycoprotein C1 of HSV-1 or G2 of HSV-2	Type-specific IgG ELISA for HSV-1 and HSV-2	EI 2531-9601-2 G	199	
		EI 2532-9601-2 G	199	
		EI 2532-9601-2 G	199	
ChLIA	Glycoprotein G1 of HSV-1 or G2 of HSV-2, resp.	ChLIA for type-specific determination of IgG antibodies against HSV-1 or HSV-2	LI 2531-10010 G	204
			LI 2532-10010 G	204
			LR 2531-20210 G	204
			LR 2532-20210 G	204
Blot	Separate bands with native or recombinant antigens from different TORCH pathogens	Multiplex detection of IgG or IgM ab against up to 10 different TORCH antigens	DN 2410-1601-4 G/M	194
			DN 2410-####-11 G	194

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 205).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q100** at [www.euroimmun.com](http://www.euroimmun.com)



# Special infection diagnostics

CSF diagnostics · TORCH · Tropical infections




For more information on this subject scan the QR code or enter the Quick Link code **q045** at [www.euroimmun.com](http://www.euroimmun.com)

## Tropical infections and emerging diseases

■ **Clinical information:** The term tropical diseases encompasses a range of infectious diseases, which – as the name suggests – originate in tropical regions. However, they can also occur in other regions, for example, through transmission by returning travellers. Emerging diseases are infections that are new in a population, or are already known but have increased rapidly in incidence or regional distribution. In recent years, large epidemics have mostly been caused by mosquito-borne viruses such as Zika, dengue and chikungunya viruses. These viruses generally cause febrile diseases with unspecific flu-like symptoms. In the further course of disease, severe complications such as encephalitis or haemorrhaging can occur. Moreover, neurological abnormalities in newborns are associated with Zika virus infection. In addition to viral diseases, parasitic infections, for example with *Echinococcus*, *Plasmodium*, *Strongyloides*, *Trypanosoma* or *Schistosoma*, also play a role in humans. The symptoms of a parasitic infection are extremely variable and sometimes occur after months or years, as is the case with echinococcosis.

■ **Diagnostics:** The diagnosis of tropical infections is a particular challenge. Over the past years it has been observed that many new viruses and other pathogens have spread worldwide, introducing unknown diseases into previously unaffected regions. For these parameters there are often no commercial diagnostic test systems available. Antibody analysis is useful for testing travellers after trips to endemic areas and for screening large population groups. EUROIMMUN offers a wide range of products for the determination of specific antibodies against many pathogens.

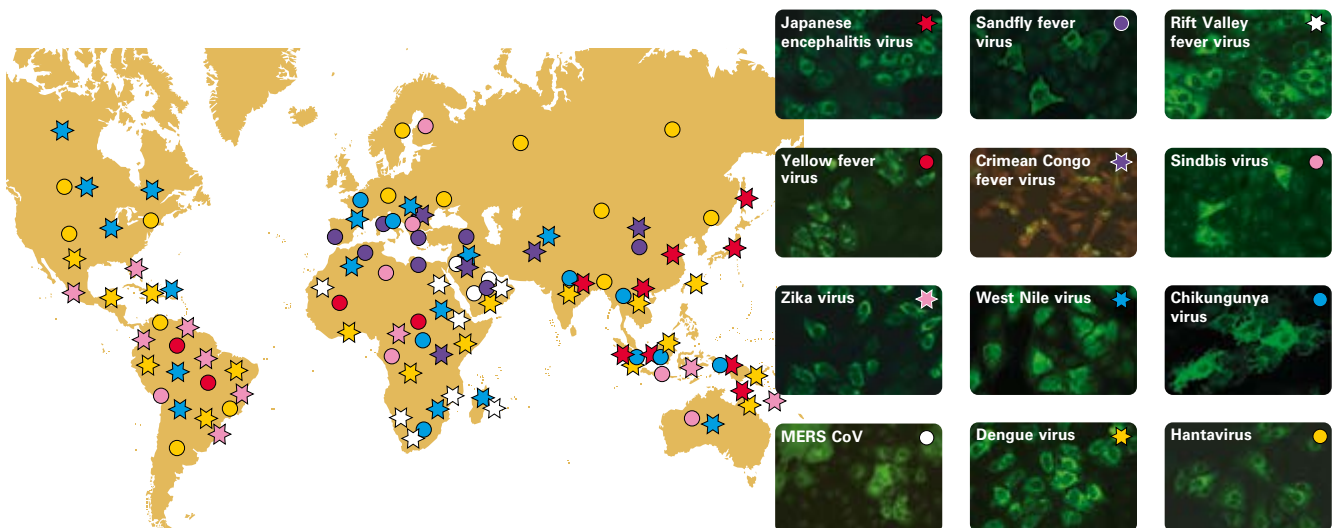



## Product overview

Method	Substrate	Application	Order number	Page
ELISA	Recombinant nonstructural protein (NS1) of Zika virus	Highly specific detection of Zika virus infection	EI 2668-9601 A/AM/G/M	201
	Preparation of dengue virus particles and rec. glycoprotein E of types 1-4	Monospecific detection of anti-dengue virus antibodies	EI 266a-9601-1 G/M	201
	Monoclonal mouse anti-dengue virus NS1 antibody	Early marker for acute dengue infections	EQ 266a-9601-1	207
	Recombinant viral structure protein from chikungunya virus	Highly specific test for the diagnosis of chikungunya fever	EI 293a-9601 G/M	202
	Purified native <i>Echinococcus multilocaris</i> vesicle fluid (EmVF)	Screening test for detection of alveolar and cystic echinococcosis	EI 2320-9601-1G	198
	Recombinant target antigens from all 5 human pathogenic Plasmodium species ( <i>P. falciparum</i> , <i>P. vivax</i> , <i>P. malariae</i> , <i>P. ovale</i> and <i>P. knowlesi</i> )	Identification of latent, asymptomatic and chronic Plasmodium infections	EI 2260-9601 G	198
Blot	Combination of whole antigen extract ( <i>Echinococcus multilocaris</i> vesicle fluid, EmVF) and specific single antigens	Differentiation between alveolar and cystic echinococcosis	DY 2321-1601-1 G	196
IFT	Flavivirus Mosaics: Zika virus, TBE virus, WNV, JEV, yellow fever virus, dengue virus types 1-4	Serological diagnosis of flavivirus infections; differential diagnostics	FI 2661-####-1 G/M FI 2661-####-2 G/M	211 211
	Arbovirus Fever Mosaics: Zika virus, chikungunya virus, dengue virus, JEV	For differential diagnosis of arbovirus infections, in particular Zika, dengue and chikungunya infections	FI 293a-####-1 G/M FI 2668-####-1 G/M FR 2668-####-1 G/M	214 211 211



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q102** at [www.euroimmun.com](http://www.euroimmun.com)



# Products for infection diagnostics





### Format

- 1601: 16 single test strips
- 1208: 12 microplate strips with 8 wells each
- 9601: 96 individual break-apart wells (12 microplate strips, 8 wells each)
- 1003: 10 slides with 3 fields each
- 1005: 10 slides with 5 fields each
- 2005: 20 slides with 5 fields each
- 1010: 10 slides with 10 fields each
- 1050: 10 slides with 50 fields each
- 1001: 10 slides to be incubated with 1 patient serum each
- 1002: 10 slides to be incubated with 2 patient sera each

**EI** **2132** - **9601** **-2** **G**

### Product code

### Immunoglobulin class

- A: IgA
- G: IgG
- M: IgM
- O: IgGM
- P: Polyvalent (IgAGM)
- X: Low-avid ab of class IgG
- H: High-avid ab of class IgG

### Product classification

- CL: Control for EUROLINE (infectious serology)..... page 192
- CW: Control for Westernblot/EUROLINE-WB (infectious serology) ..... page 193
- DN: Test system EUROLINE (infectious serology)..... page 194
- DY: Test system Westernblot/EUROLINE-WB (infectious serology) ..... page 195
- EI: Test system microplate ELISA (infectious serology)..... page 197
- LI: Test system chemiluminescence test (infectious serology) ..... page 204
- LR: Control set chemiluminescence test..... page 204
- Test system **ids** chemiluminescence test (infectious serology) ..... page 205
- Control set **ids** chemiluminescence test (infectious serology)..... page 206
- EQ: Test system microplate ELISA (infectious diseases, antigen determination)..... page 207
- ET: T-cell stimulation tube set (infectious diseases) ..... page 207
- CK: ELISA control (infectious CSF diagnostics) ..... page 208
- FI: Test system indirect immunofluorescence (infectious serology) ..... page 209
- FK: Single slides indirect immunofluorescence (infectious serology) ..... page 209
- FR: Test system for indirect immunofluorescence (EUROPattern): Infectious serology ..... page 209
- FS: Single slides for indirect immunofluorescence (EUROPattern): Infectious serology ..... page 209

For product orders the amount, product code and test name are required. **Test kits** comprise all reagents needed to perform the serological investigation. For diagnostics in indirect immunofluorescence, for example, these include slides, FITC-labelled antibodies against human immunoglobulin, positive and negative control sera (not available for some products) as well as embedding medium, cover glasses, sachets of PBS and Tween 20. EUROSORB for the determination of IgM class antibodies and sample buffer 3 (for anti-Borrelia IIFT only) are not included in the immunofluorescence test systems.

Substrates consisting of cell cultures and tissues which do not appear in this catalogue can be made to specification. In addition, BIOCHIP mosaics can be produced according to individual requirements. Apart from the customary package sizes and slide formats, special sizes are available as well. Quotations can be provided upon request.



### Controls for EUROLINE: Infectious Serology

Order No.	Control (Ready for use)	Ig Class	Format
CW2000-0001 ZA	negative control for infectious serology blot systems (IgA)	IgA	0.1 ml
CW2000-0001 ZG	negative control for infectious serology blot systems (IgG)	IgG	0.1 ml
CW2000-0001 ZM	negative control for infectious serology blot systems (IgM)	IgM	0.1 ml
CL 2050-0107 G	positive control serum: IgG, human, 50x concentrated for <i>Bordetella pertussis</i>	IgG	0.1 ml for EUROBlotOne
CL 2111-0107 G	positive control serum: IgG, human, 50x concentrated for <i>Treponema pallidum</i>	IgG	0.1 ml for EUROBlotOne
CL 2111-0107 M	positive control serum: IgM, human, 50x concentrated for <i>Treponema pallidum</i>	IgM	0.1 ml for EUROBlotOne
CL 2131-0107 G	positive control serum: IgG, human, 50x concentrated for <i>Borrelia</i>	IgG	0.1 ml for EUROBlotOne
CL 2131-0107 M	positive control serum: IgM, human, 50x concentrated for <i>Borrelia</i>	IgM	0.1 ml for EUROBlotOne
CL 2410-0107-4 G	positive control serum: IgG, human, 50x concentrated for TO.R.C.H. Profile	IgG	0.1 ml for EUROBlotOne
CL 2410-0107-4 M	positive control serum: IgM, human, 50x concentrated for TO.R.C.H. Profile	IgM	0.1 ml for EUROBlotOne
CL 2790-0107-12 G	positive control serum: IgG, human, 50x concentrated for EBV-Profil 2 G	IgG	0.1 ml for EUROBlotOne
CL 2790-0107-12 M	positive control serum: IgM, human, 50x concentrated for EBV-Profil 2 M	IgM	0.1 ml for EUROBlotOne





<b>Controls for Westernblot/EUROLINE-WB: Infectious Serology</b>			
<b>Order No.</b>	<b>Control (Ready for use)</b>	<b>Ig Class</b>	<b>Format</b>
CW2000-0001 ZA	negative control for infectious serology blot systems (IgA)	IgA	0.1 ml
CW2000-0001 ZG	negative control for infectious serology blot systems (IgG)	IgG	0.1 ml
CW2000-0001 ZM	negative control for infectious serology blot systems (IgM)	IgM	0.1 ml
CW2080-5001 A	antibodies against <i>Helicobacter pylori</i> IgA positive control	IgA	0.1 ml
CW2080-5001 G	antibodies against <i>Helicobacter pylori</i> IgG positive control	IgG	0.1 ml
CW2111-5001 G	antibodies against <i>Treponema pallidum</i> IgG positive control	IgG	0.1 ml
CW2111-5001 M	antibodies against <i>Treponema pallidum</i> IgM positive control	IgM	0.1 ml
CW2131-5001 G	antibodies against <i>Borrelia afzelii</i> IgG positive control (Westernblot/EUROLINE-WB)	IgG	0.1 ml
CW2131-5001 M	antibodies against <i>Borrelia afzelii</i> IgM positive control (Westernblot/EUROLINE-WB)	IgM	0.1 ml
CW2132-5001 G	antibodies against <i>Borrelia burgdorferi</i> IgG positive control	IgG	0.1 ml
CW2132-5001 M	antibodies against <i>Borrelia burgdorferi</i> IgM positive control	IgM	0.1 ml
CW2134-5001 G	antibodies against <i>Borrelia garinii</i> IgG positive control	IgG	0.1 ml
CW2134-5001 M	antibodies against <i>Borrelia garinii</i> IgM positive control	IgM	0.1 ml
CW2173-5001 A	antibodies against <i>Yersinia enterocolitica</i> IgA positive control (for diagnosing various forms of arthritis)	IgA	0.1 ml
CW2173-5001 G	antibodies against <i>Yersinia enterocolitica</i> IgG positive control (for diagnosing various forms of arthritis)	IgG	0.1 ml
CW2321-5001 G	antibodies against <i>Echinococcus</i> IgG positive control	IgG	0.1 ml
CW2531-5001 G	antibodies against Herpes simplex virus (HSV) IgG positive control	IgG	0.1 ml
CW2790-5001 G	antibodies against Epstein-Barr virus (EBV) IgG positive control	IgG	0.1 ml
CW2790-5001 M	antibodies against Epstein-Barr virus (EBV) IgM positive control	IgM	0.1 ml



## EUROLINE for Infectious Serology (Test Systems)

Order No.	Antibodies against	Ig Class	Substrate	Format
DL 0160-1601 G	EUROLINE validation	IgG	EUROLINE	16 strips
DN 2050-1601 A DN 2050-24001 A	<i>Bordetella pertussis</i> (FHA, PT, ACT separately)	IgA	EUROLINE	16 strips 240 strips
DN 2050-1601 G DN 2050-24001 G	<i>Bordetella pertussis</i> (FHA, PT, ACT separately)	IgG	EUROLINE	16 strips 240 strips
DN 2111-1601 G DN 2111-6401 G	<i>Treponema pallidum</i> (TpN15, TpN17, TmpA, TpN47 separately)	IgG	EUROLINE	16 strips 64 strips
DN 2111-1601 M DN 2111-6401 M	<i>Treponema pallidum</i> (TpN15, TpN17, TmpA, TpN47 separately)	IgM	EUROLINE	16 strips 64 strips
DN 2131-3201 G DN 2131-0510 G DN 2131-24001 G	EUROLINE <i>Borrelia</i> -RN-AT (p18, p19, p20, p21, p58, OspC (p25), p39, p83, LBb, LBa, VlsE Bg, VlsE Bb, VlsE Ba separately)	IgG	EUROLINE	32 strips 50 strips Immunoblot-PreQ 240 strips
DN 2131-3201 M DN 2131-0510 M DN 2131-24001 M	EUROLINE <i>Borrelia</i> -RN-AT (OspC Bg native, OspC Bb native, OspC Ba native, p39, VlsE Bb separately)	IgM	EUROLINE	32 strips 50 strips Immunoblot-PreQ 240 strips
DN 2131-3201-2 M DN 2131-0510-2 M DN 2131-24001-2 M	EUROLINE <i>Borrelia</i> -RN-AT-adv (OspC-adv Bsp, OspC-adv Bg, OspC-adv Bb, OspC-adv Ba, p39, VlsE Bb separately)	IgM	EUROLINE	32 strips 50 strips Immunoblot-PreQ 240 strips
DN 2173-1601 A DN 2173-6401 A	<i>Yersinia enterocolitica</i> Detection of antibodies against virulence factors of the <i>Yersinia enterocolitica</i> pathogen in human serum (for diagnosing various forms of arthritis).	IgA	EUROLINE	16 strips 64 strips
DN 2173-1601 G DN 2173-6401 G	<i>Yersinia enterocolitica</i> Detection of antibodies against virulence factors of the <i>Yersinia enterocolitica</i> pathogen in human serum (for diagnosing various forms of arthritis).	IgG	EUROLINE	16 strips 64 strips
DN 2410-1601-4 G DN 2410-6401-4 G	"TO.R.C.H. Profile" ( <i>Toxoplasma gondii</i> , Rubella virus, CMV, HSV-1, HSV-2 separately)	IgG	EUROLINE	16 strips 64 strips
DN 2410-1601-4 M DN 2410-6401-4 M	"TO.R.C.H. Profile" ( <i>Toxoplasma gondii</i> , ROP1, Rubella virus, CMV, HSV-1, HSV-2 separately)	IgM	EUROLINE	16 strips 64 strips
DN 2410-1601-11 G DN 2410-6401-11 G	"TO.R.C.H. 10" ( <i>Toxoplasma gondii</i> , Rubella virus, CMV, HSV-1, HSV-2, <i>Bordetella pertussis</i> , <i>Chlamydia trachomatis</i> , Parvovirus B19, <i>Treponema pallidum</i> , VZV separately)	IgG	EUROLINE	16 strips 64 strips
DN 2525-1601 A DN 2525-0510 A DN 2525-6401 A	EUROLINE Hepatitis E Virus (separat: GT1 ORF2, GT2 ORF2, GT3 ORF2, GT4 ORF2)	IgA	EUROLINE	16 stripes 50 stripes Immunoblot-PreQ 64 stripes
DN 2525-1601 G DN 2525-0510 G DN 2525-6401 G	EUROLINE Hepatitis E Virus (separat: GT1 ORF2, GT2 ORF2, GT3 ORF2, GT4 ORF2)	IgG	EUROLINE	16 stripes 50 stripes Immunoblot-PreQ 64 stripes
DN 2525-1601 M DN 2525-0510 M DN 2525-6401 M	EUROLINE Hepatitis E Virus (separat: GT1 ORF2, GT2 ORF2, GT3 ORF2, GT4 ORF2)	IgM	EUROLINE	16 stripes 50 stripes Immunoblot-PreQ 64 stripes
DN 2580-1601 G	Parvovirus B19 (VP1, VLP, VP2, NS1 separately)	IgG	EUROLINE	16 strips
DN 2580-1601 M	Parvovirus B19 (VP1, VLP, VP2, NS1 separately)	IgM	EUROLINE	16 strips



EUROLINE for Infectious Serology (Test Systems)				
Order No.	Antibodies against	Ig Class	Substrate	Format
DN 2606-1601-1 G DN 2606-0510-1 G DN 2606-6401-1 G	EUROLINE Anti-SARS-CoV-2 Profile ( IgG)	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips
DN 278h-1601-1 G	Hantavirus Profile 1 (PUUV, DOBV, HTNV separately)	IgG	EUROLINE	16 strips
DN 278h-1601-1 M	Hantavirus Profile 1 (PUUV, DOBV, HTNV separately)	IgM	EUROLINE	16 strips
DN 2790-1601-2 G DN 2790-0510-2 G DN 2790-6401-2 G	EBV Profile 2 (VCA gp125, VCA p19, EBNA-1, p22, EA-D separately)	IgG	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips
DN 2790-1601-2 M DN 2790-0510-2 M DN 2790-6401-2 M	EBV Profile 2 (VCA gp125, VCA p19, EBNA-1, p22, EA-D separately)	IgM	EUROLINE	16 strips 50 strips Immunoblot-PreQ 64 strips

Westernblot/EUROLINE-WB for Infectious Serology (Test Systems)				
Order No.	Antibodies against	Antigen and Antigen Source	Ig Class	Format
DY 2080-1601-1 A DY 2080-3001-1 A	EUROLINE-WB Helicobacter pylori	whole antigen of H. pylori, plus recombinant VacA and CagA antigen	IgA	16 strips 30 strips
DY 2080-1601-1 G DY 2080-3001-1 G	EUROLINE-WB Helicobacter pylori	whole antigen of H. pylori, plus recombinant VacA and CagA antigen	IgG	16 strips 30 strips
DY 2111-1601 G DY 2111-2401 G	Treponema pallidum	15 kDa, 17 kDa, 45 kDa (tmpA), 47 kDa	IgG	16 strips 24 strips
DY 2111-1601 M DY 2111-2401 M	Treponema pallidum	15 kDa, 17 kDa, 45 kDa (tmpA), 47 kDa	IgM	16 strips 24 strips
DY 2111-1601-1 G DY 2111-2401-1 G	EUROLINE-WB Treponema pallidum plus cardiolipin	15 kDa, 17 kDa, 45 kDa (tmpA), 47 kDa plus purified cardiolipin	IgG	16 strips 24 strips
DY 2111-1601-1 M DY 2111-2401-1 M	EUROLINE-WB Treponema pallidum plus cardiolipin	15 kDa, 17 kDa, 45 kDa (tmpA), 47 kDa plus purified cardiolipin	IgM	16 strips 24 strips
DY 2131-3001 G DY 2131-24001 G	Borrelia afzelii	whole antigen, SDS extract of Borrelia afzelii	IgG	30 strips 240 strips
DY 2131-3001 M DY 2131-24001 M	Borrelia afzelii	whole antigen, SDS extract of Borrelia afzelii	IgM	30 strips 240 strips
DY 2131-1601-1 G DY 2131-3001-1 G DY 2131-0148-1 G DY 2131-24001-1 G	EUROLINE-WB Borrelia	whole antigen, SDS extract of Borrelia afzelii plus VlsE	IgG	16 strips 30 strips 48 strips Immunoblot-PreQ 240 strips
DY 2131-1601-1 M DY 2131-3001-1 M DY 2131-0148-1 M DY 2131-24001-1 M	EUROLINE-WB Borrelia	whole antigen, SDS extract of Borrelia afzelii plus VlsE	IgM	16 strips 30 strips 48 strips Immunoblot-PreQ 240 strips
DY 2132-3001 G	Borrelia burgdorferi	whole antigen, SDS extract of Borrelia burgdorferi sensu stricto	IgG	30 strips
DY 2132-3001 M	Borrelia burgdorferi	whole antigen, SDS extract of Borrelia burgdorferi sensu stricto	IgM	30 strips



## Westernblot/EUROLINE-WB for Infectious Serology (Test Systems)

Order No.	Antibodies against	Antigen and Antigen Source	Ig Class	Format
DY 2133-3001 G * DY 2133-24001 G *	<b>Borrelia burgdorferi US</b>	whole antigen, SDS extract of <i>Borrelia burgdorferi</i>	IgG	30 strips 240 strips
DY 2133-3001-1 M * DY 2133-24001-1 M *	<b>Borrelia burgdorferi US EUROLINE-WB</b>	whole antigen, SDS extract of <i>Borrelia burgdorferi</i> plus flagellin	IgM	30 strips 240 strips
DY 2134-3001 G	<b>Borrelia garinii</b>	whole antigen, SDS extract of <i>Borrelia garinii</i>	IgG	30 strips
DY 2134-3001 M	<b>Borrelia garinii</b>	whole antigen, SDS extract of <i>Borrelia garinii</i>	IgM	30 strips
DY 2173-1601 A DY 2173-3001 A	<b>Yersinia enterocolitica</b> Detection of antibodies against virulence factors of the <i>Yersinia enterocolitica</i> pathogen in human serum (for diagnosing various forms of arthritis).	isolated virulence factors (release proteins, Yop) of <i>Yersinia enterocolitica</i>	IgA	16 strips 30 strips
DY 2173-1601 G DY 2173-3001 G	<b>Yersinia enterocolitica</b> Detection of antibodies against virulence factors of the <i>Yersinia enterocolitica</i> pathogen in human serum (for diagnosing various forms of arthritis).	isolated virulence factors (release proteins, Yop) of <i>Yersinia enterocolitica</i>	IgG	16 strips 30 strips
DY 2190-1601-1 A	<b>EUROLINE-WB Chlamydia, human pathogen</b>	<i>Chlamydia trachomatis</i> , <i>Chlamydia pneumoniae</i> , <i>Chlamydia psittaci</i>	IgA	16 strips
DY 2190-1601-1 G	<b>EUROLINE-WB Chlamydia, human pathogen</b>	<i>Chlamydia trachomatis</i> , <i>Chlamydia pneumoniae</i> , <i>Chlamydia psittaci</i>	IgG	16 strips
DY 2311-1601 G	<b>Toxocara</b>	<i>Toxocara</i> whole lysate	IgG	16 strips
DY 2321-1601-1 G	<b>EUROLINE-WB Echinococcus</b>	<i>Echinococcus multilocularis</i> and <i>Echinococcus granulosus</i>	IgG	16 strips
DY 2531-1601-1 G	<b>EUROLINE-WB Herpes simplex virus 1 (HSV-1) plus HSV-2 type-specific glycoprotein G2</b>	whole antigen, SDS extract of HSV-1 plus purified gG2	IgG	16 strips
DY 2531-1601-1 M	<b>EUROLINE-WB Herpes simplex virus 1 (HSV-1) plus HSV-2 type-specific glycoprotein G2</b>	whole antigen, SDS extract of HSV-1 plus purified gG2	IgM	16 strips
DY 2590-2401 G	<b>Rubella virus</b>	whole antigen	IgG	24 strips
DY 2790-1601-1 G	<b>EUROLINE-WB Epstein Barr virus (EBV)</b>		IgG	16 strips
DY 2790-1601-1 M	<b>EUROLINE-WB Epstein Barr virus (EBV)</b>		IgM	16 strips

## EUROMicroblot for Infectious Serology (Test Systems)

Order No.	Antibodies against	Ig Class	Substrate	Format
KN 2131-9601 G	<b>EUROMicroblot Anti Borrelia (IgG)</b>	IgG		1 x 96, separable
KN 2131-9601 M	<b>EUROMicroblot Anti Borrelia (IgM)</b>	IgM		1 x 96, separable

\* For research use only, not for in vitro diagnostic use in the sense of EU directive 98/79/EC.



Microplate ELISA for Infectious Serology (Test Systems)				
Order No.	Antibodies against	Ig Class	Calibration	Format
EI 2040-9601 G	diphtheria toxoid	IgG	0.01/0.1/1/2 IU/ml	96 x 01
EI 2050-9601 A	Bordetella pertussis toxin	IgA	2/10/25/50 IU/ml	96 x 01
EI 2050-9601 G	Bordetella pertussis toxin	IgG	5/25/100/200 IU/ml	96 x 01
EI 2050-9601 M	Bordetella pertussis incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2050-9601-3 A	Bordetella FHA	IgA	2/10/25/50 IU/ml	96 x 01
EI 2050-9601-3 G	Bordetella FHA	IgG	5/25/100/200 IU/ml	96 x 01
EI 2060-9601 G	tetanus toxoid	IgG	0,01/0,1/1/2/5 IU/ml	96 x 01
EI 2080-9601 A	Helicobacter pylori	IgA	semi-quantitative	96 x 01
EI 2080-9601 G	Helicobacter pylori	IgG	2/20/200 RU/ml	96 x 01
EI 2081-9601 A	Helicobacter pylori (CagA)	IgA	semi-quantitative	96 x 01
EI 2091-9601 A	Campylobacter jejuni	IgA	semi-quantitative	96 x 01
EI 2091-9601 G	Campylobacter jejuni	IgG	2/20/200 RU/ml	96 x 01
EI 2111-9601 G	Treponema pallidum	IgG	2/20/200 RU/ml	96 x 01
EI 2111-9601 M	Treponema pallidum incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2111-9601 O	Treponema pallidum Screen ELISA	IgGM	2/20/200 RU/ml	96 x 01
EI 2111-9601-L G	Treponema pallidum antibody determination in CSF	IgG	5/25/50/100 U	96 x 01
EI 2132-9601 M	Borrelia incl. IgG/RF absorbent	IgM	2/20/200 RU/ml	96 x 01
EI 2132-9601-2 G	Borrelia plus VlsE	IgG	2/20/200 RU/ml	96 x 01
EI 2132-9601-5 G	Borrelia Select: recombinant antigens with VlsE	IgG	2/20/200 RU/ml	96 x 01
EI 2132-9601-5 M	Borrelia Select: recombinant antigens with OspC advanced	IgM	2/20/200 RU/ml	96 x 01
EI 2132-9601-L G	Borrelia PLUS VlsE antibody determination in CSF	IgG	5/25/50/100/175/230 U	96 x 01
EI 2132-9601-L M	Borrelia antibody determination in CSF	IgM	5/25/50/100/175 U	96 x 01
EI 2132-9601-24 O	Lyme ELISA	IgGM	qualitative	96 x 01
EI 2150-9601 G	Legionella pneumophila	IgG	2/20/200 RU/ml	96 x 01
EI 2150-9601 M	Legionella pneumophila incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01



## Microplate ELISA for Infectious Serology (Test Systems)

Order No.	Antibodies against	Ig Class	Calibration	Format
EI 2173-9601 A	<i>Yersinia enterocolitica</i>	IgA	semi-quantitative	96 x 01
EI 2173-9601 G	<i>Yersinia enterocolitica</i>	IgG	2/20/200 RU/ml	96 x 01
EI 217a-9601-1 G	<i>Coxiella burnetii</i> phase 1	IgG	semi-quantitative	96 x 01
EI 217a-9601-2 G	<i>Coxiella burnetii</i> phase 2	IgG	semi-quantitative	96 x 01
EI 217a-9601-2 M	<i>Coxiella burnetii</i> phase 2	IgM	semi-quantitative	96 x 01
EI 2189-9601 G	<i>Brucella abortus</i>	IgG	2/20/200 RU/ml	96 x 01
EI 2189-9601 M	<i>Brucella abortus</i> incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2191-9601 A	<i>Chlamydia trachomatis</i>	IgA	semi-quantitative	96 x 01
EI 2191-9601 G	<i>Chlamydia trachomatis</i>	IgG	2/20/200 RU/ml	96 x 01
EI 2191-9601 M	<i>Chlamydia trachomatis</i> incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2192-9601 A	<i>Chlamydia pneumoniae</i>	IgA	semi-quantitative	96 x 01
EI 2192-9601 G	<i>Chlamydia pneumoniae</i>	IgG	2/20/200 RU/ml	96 x 01
EI 2192-9601 M	<i>Chlamydia pneumoniae</i> incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2202-9601 A	<i>Mycoplasma pneumoniae</i>	IgA	semi-quantitative	96 x 01
EI 2202-9601 G	<i>Mycoplasma pneumoniae</i>	IgG	2/20/200 RU/ml	96 x 01
EI 2202-9601 M	<i>Mycoplasma pneumoniae</i> incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2212-9601 G	<i>Trypanosoma cruzi</i>	IgG	2/20/200 RU/ml	96 x 01
EI 2260-9601 G	<i>Plasmodium</i>	IgG	semi-quantitative	96 x 01
EI 2290-9601 G	<i>Strongyloides</i>	IgG	semi-quantitative	96 x 01
EI 2300-9601 G	<i>Schistosoma</i>	IgG	semi-quantitative	96 x 01
EI 2300-9601 M	<i>Schistosoma</i> incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2311-9601 G	<i>Toxocara</i>	IgG	semi-quantitative	96 x 01
EI 2320-9601-1 G	<i>Echinococcus</i>	IgG	semi-quantitative	96 x 01
EI 2410-9601 A	<i>Toxoplasma gondii</i>	IgA	semi-quantitative	96 x 01
EI 2410-9601 G	<i>Toxoplasma gondii</i>	IgG	1/10/200 IU/ml	96 x 01
EI 2410-9601 M	<i>Toxoplasma gondii</i> incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2410-9601 P	<i>Toxoplasma gondii</i> Screen	IgAGM	semi-quantitative	96 x 01
EI 2410-9601-1 G	<i>Toxoplasma gondii</i> avidity determination	IgG	1/10/200 IU/ml	96 x 01
EI 2410-9601-L G	<i>Toxoplasma gondii</i> antibody determination in CSF	IgG	5/25/50/100 U	96 x 01





Microplate ELISA for Infectious Serology (Test Systems)				
Order No.	Antibodies against	Ig Class	Calibration	Format
EI 2525-9601 G	Hepatitis E virus (HEV)	IgG	0,2/1/10/25 IU/ml	96 x 01
EI 2525-9601 M	Hepatitis E virus (HEV)	IgM	semi-quantitative	96 x 01
EI 2525-9601 P	Hepatitis E virus (HEV)	IgAGM	semi-quantitative	96 x 01
EI 2531-9601-1 G	Herpes simplex virus (HSV-1/2 Pool)	IgG	2/20/200 RU/ml	96 x 01
EI 2531-9601-1 L G	Herpes simplex virus (HSV-1/2 Pool) antibody determination in CSF	IgG	5/25/50/100/175/230 U/ml	96 x 01
EI 2531-9601-1 M	Herpes simplex virus (HSV-1/2 Pool) incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2531-9601-2 G	Herpes simplex virus 1 (HSV-1)	IgG	2/20/200 RU/ml	96 x 01
EI 2532-9601-2 G	Herpes simplex virus 2 (HSV-2)	IgG	2/20/200 RU/ml	96 x 01
EI 2570-9601 G	Cytomegalovirus (CMV)	IgG	2/20/200 RU/ml	96 x 01
EI 2570-9601 M	Cytomegalovirus (CMV) incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2570-9601-1 G	Cytomegalovirus (CMV) avidity determination	IgG	2/20/200 RU/ml	96 x 01
EI 2570-9601-2 M	Cytomegalovirus (CMV) p52 incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2570-9601-3 G	Cytomegalovirus (CMV) gB	IgG	2/20/200 RU/ml	96 x 01
EI 2570-9601-L G	Cytomegalovirus (CMV) antibody determination in CSF	IgG	5/25/50/100 U	96 x 01
EI 2580-9601 G	Parvovirus B19	IgG	1/5/25/100 IU/ml	96 x 01
EI 2580-9601 M	Parvovirus B19 incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2590-9601 G	Rubella virus	IgG	1/10/50/200 IU/ml	96 x 01
EI 2590-9601-1 G	Rubella virus avidity determination	IgG	1/10/50/200 IU/ml	96 x 01
EI 2590-9601-2 M	Rubella virus glycoprotein incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2590-9601-L G	Rubella virus antibody determination in CSF	IgG	5/25/50/100/175/230 U	96 x 01
EI 2604-9601 G	MERS coronavirus	IgG	semi-quantitative	96 x 01



## Microplate ELISA for Infectious Serology (Test Systems)

Order No.	Antibodies against	Ig Class	Calibration	Format
EI 2606-9601 A EI 2606-9620 A	SARS-CoV-2	IgA	semi-quantitative	96 x 01 96 x 20
EI 2606-9601 G EI 2606-9620 G	SARS-CoV-2	IgG	semi-quantitative	96 x 01 96 x 20
EI 2606-9601-2 G EI 2606-9620-2 G	SARS-CoV-2 NCP	IgG	semi-quantitative	96 x 01 96 x 20
EI 2606-9601-4	SARS-CoV-2 NeutralISA	IgAGM		96 x 01
EI 2606-9601-10 G	SARS-CoV-2 QuantiVac	IgG	1/10/20/40/80/120 RU/mL	96 x 01
EI 2610-9601 G	Measles virus	IgG	50/250/1000/5000 IU/l	96 x 01
EI 2610-9601 M	Measles virus incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2610-9601-1 G	Measles virus avidity determination	IgG	50/250/1000/5000/5000 IU/l	96 x 01
EI 2610-9601-4 M	Measles virus NP: recombinant nucleoprotein incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2610-9601-L G	Measles virus antibody determination in CSF	IgG	5/25/50/100/175/230 U	96 x 01
EI 2630-9601 G	Mumps virus	IgG	2/20/200 RU/ml	96 x 01
EI 2630-9601 M	Mumps virus incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2630-9601-3 G	Mumps virus AT: strains "Enders" and "Jeryl Lynn"	IgG	2/20/200 RU/ml	96 x 01
EI 2630-9601-5 M	Mumps virus G5: native antigens, genotype "G5" incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2630-9601-L G	Mumps virus antibody determination in CSF	IgG	5/25/50/100 U	96 x 01
EI 2650-9601 A	Varicella zoster virus (VZV)	IgA	semi-quantitative	96 x 01
EI 2650-9601 G	Varicella zoster virus (VZV)	IgG	10/100/500/5000 IU/l	96 x 01
EI 2650-9601 M	Varicella zoster virus (VZV) incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2650-9601-1 G	Varicella zoster virus (VZV) avidity determination	IgG	10/100/500/5000 IU/l	96 x 01
EI 2650-9601-2 M	Varicella zoster virus (VZV) glycoprotein incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2650-9601-L A	Varicella zoster virus (VZV) antibody determination in CSF	IgA	5/25/50/100 U	96 x 01
EI 2650-9601-L G	Varicella zoster virus (VZV) antibody determination in CSF	IgG	5/25/50/100/175/230 U	96 x 01
EI 2661-9601 G	TBE virus	IgG	2/20/200 RU/ml	96 x 01



Microplate ELISA for Infectious Serology (Test Systems)				
Order No.	Antibodies against	Ig Class	Calibration	Format
EI 2661-9601 M	TBE virus incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2661-9601-1 G	TBE virus avidity determination	IgG	2/20/200 RU/ml	96 x 01
EI 2661-9601-9 G	TBE virus Vienna	IgG	15/150/300/1000 VIEU/ml	96 x 01
EI 2661-9601-L G	TBE virus antibody determination in CSF	IgG	5/25/50/100 U	96 x 01
EI 2661-9601-L M	TBE virus antibody determination in CSF	IgM	5/25/50/100 U	96 x 01
EI 2662-9601 G	West Nile virus (WNV)	IgG	2/20/200 RU/ml	96 x 01
EI 2662-9601 M	West Nile virus (WNV) incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2662-9601-1 G	West Nile virus (WNV) avidity determination	IgG	2/20/200 RU/ml	96 x 01
EI 2662-9601-2 G *	West Nile virus (WNV) NS1	IgG	2/20/200 RU/ml	96 x 01
EI 2663-9601 G	Japanese encephalitis virus (JEV)	IgG	2/20/200 RU/ml	96 x 01
EI 2663-9601 M	Japanese encephalitis virus (JEV)	IgM	semi-quantitative	96 x 01
EI 2667-9601 G	Usutu virus	IgG	2/20/200 RU/ml	96 x 01
EI 2668-9601 A	Zika virus (ZIKV)	IgA	semi-quantitative	96 x 01
EI 2668-9601 G	Zika virus (ZIKV)	IgG	2/20/200 RU/ml	96 x 01
EI 2668-9601 M	Zika virus (ZIKV) incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2668-9601 Q	Zika virus (ZIKV) incl. IgG/RF absorbent	IgAM	semi-quantitative	96 x 01
EI 266a-9601-1 G	Dengue virus (DENV) type 1-4	IgG	2/20/200 RU/ml	96 x 01
EI 266a-9601-1 M	Dengue virus (DENV) type 1-4 incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 266a-9601-2 G	Dengue virus NS1 (DENV) type 1-4	IgG	2/20/200 RU/ml	96 x 01
EI 2670-9601 A	Respiratory syncytial virus (RSV)	IgA	semi-quantitative	96 x 01
EI 2670-9601 G	Respiratory syncytial virus (RSV)	IgG	2/20/200 RU/ml	96 x 01
EI 2670-9601 M	Respiratory syncytial virus (RSV) incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2680-9601 A	Adenovirus	IgA	semi-quantitative	96 x 01
EI 2680-9601 G	Adenovirus	IgG	2/20/200 RU/ml	96 x 01

\* For research use only, not for in vitro diagnostic use in the sense of EU directive 98/79/EC.



## Microplate ELISA for Infectious Serology (Test Systems)

Order No.	Antibodies against	Ig Class	Calibration	Format
EI 2680-9601 M	Adenovirus incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2691-9601 A	Influenza virus type A	IgA	semi-quantitative	96 x 01
EI 2691-9601 G	Influenza virus type A	IgG	2/20/200 RU/ml	96 x 01
EI 2692-9601 A	Influenza virus type B	IgA	semi-quantitative	96 x 01
EI 2692-9601 G	Influenza virus type B	IgG	2/20/200 RU/ml	96 x 01
EI 2721-9601-1 A	Parainfluenza virus types 1 - 4 (Pool)	IgA	semi-quantitative	96 x 01
EI 2721-9601-1 G	Parainfluenza virus types 1 - 4 (Pool)	IgG	2/20/200 RU/ml	96 x 01
EI 2730-9601-1 A	Enterovirus	IgA	semi-quantitative	96 x 01
EI 2730-9601-1 G	Enterovirus	IgG	semi-quantitative	96 x 01
EI 2730-9601-1 M	Enterovirus incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 277c-9601 G	Toscana virus	IgG	2/20/200 RU/ml	96 x 01
EI 278h-9601-1 G	Hantavirus Pool 1 "Eurasia"	IgG	2/20/200 RU/ml	96 x 01
EI 278h-9601-1 M	Hantavirus Pool 1 "Eurasia" incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 278h-9601-2 G	Hantavirus Pool 2 "America"	IgG	2/20/200 RU/ml	96 x 01
EI 278h-9601-2 M	Hantavirus Pool 2 "America" incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2791-9601 A	Epstein-Barr virus capsid antigen (EBV-CA)	IgA	semi-quantitative	96 x 01
EI 2791-9601 G	Epstein-Barr virus capsid antigen (EBV-CA)	IgG	2/20/200 RU/ml	96 x 01
EI 2791-9601 M	Epstein-Barr virus capsid antigen (EBV-CA) incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 2791-9601-1 G	Epstein-Barr virus capsid antigen (EBV-CA) avidity determination	IgG	2/20/200 RU/ml	96 x 01
EI 2791-9601-L G	Epstein-Barr virus capsid antigen (EBV-CA) antibody determination in CSF	IgG	5/25/50/100 U	96 x 01
EI 2793-9601 G	Epstein-Barr virus nuclear antigen (EBNA-1)	IgG	2/20/200 RU/ml	96 x 01
EI 2795-9601 A	Epstein-Barr virus early antigen (EBV-EA)	IgA	semi-quantitative	96 x 01
EI 2795-9601 G	Epstein-Barr virus early antigen (EBV-EA)	IgG	2/20/200 RU/ml	96 x 01
EI 2795-9601 M	Epstein-Barr virus early antigen (EBV-EA) incl. IgG/RF absorbent	IgM	semi-quantitative	96 x 01
EI 279a-9601 G	Crimean Congo fever virus (CCHFV)	IgG	2/20/200 RU/ml	96 x 01



<b>Microplate ELISA for Infectious Serology (Test Systems)</b>				
<b>Order No.</b>	<b>Antibodies against</b>	<b>Ig Class</b>	<b>Calibration</b>	<b>Format</b>
El 279a-9601 M	<b>Crimean Congo fever virus (CCHFV) incl. IgG/RF absorbent</b>	IgM	semi-quantitative	96 x 01
El 293a-9601 G	<b>Chikungunya virus (CHIKV)</b>	IgG	2/20/200 RU/ml	96 x 01
El 293a-9601 M	<b>Chikungunya virus (CHIKV) incl. IgG/RF absorbent</b>	IgM	semi-quantitative	96 x 01
El 295c-9601 G	<b>Mayaro virus (MAYV)</b>	IgG	2/20/200 RU/ml	96 x 01
El 295c-9601 M	<b>Mayaro virus (MAYV)</b>	IgM	semi-quantitative	96 x 01



### Chemiluminescence Tests for Infectious Serology (Test Systems)

Order No.	Antibodies against	Ig Class	Calibration	Format
LI 2132-10010 G	<b>Borrelia</b>	IgG	quantitative	100 determinations for RA Analyzer 10
LI 2132-10010 M	<b>Borrelia</b>	IgM	quantitative	100 determinations for RA Analyzer 10
LI 2531-10010 G	<b>Herpes simplex virus 1 (HSV-1)</b>	IgG	quantitative	100 determinations for RA Analyzer 10
LI 2532-10010 G	<b>Herpes simplex virus 2 (HSV-2)</b>	IgG	quantitative	100 determinations for RA Analyzer 10
LI 2580-10010 G	<b>Parvovirus B19</b>	IgG	quantitative	100 determinations for RA Analyzer 10
LI 2580-10010 M	<b>Parvovirus B19</b>	IgM	quantitative	100 determinations for RA Analyzer 10
LI 2606-10010-1 G	<b>SARS-CoV-2 RBD</b>	IgG	quantitative	100 determinations for RA Analyzer 10
LI 2791-10010 G	<b>Epstein-Barr virus capsid antigen (EBV-CA)</b>	IgG	quantitative	100 determinations for RA Analyzer 10
LI 2791-10010 M	<b>Epstein-Barr virus capsid antigen (EBV-CA)</b>	IgM	quantitative	100 determinations for RA Analyzer 10
LI 2793-10010 G	<b>Epstein-Barr virus nuclear antigen 1 (EBNA-1)</b>	IgG	quantitative	100 determinations for RA Analyzer 10

### Control Sets for Chemiluminescence Tests

Order No.	Control Set (Ready for use)	Ig Class	Format
LR 2132-20210 G	<b>Control set Borrelia</b>	IgG	2 x 0.5 ml control 1/2
LR 2132-20210 M	<b>Control set Borrelia</b>	IgM	2 x 0.5 ml control 1/2
LR 2531-20210 G	<b>Control set Herpes simplex virus 1 (HSV-1)</b>	IgG	2 x 0.5 ml control 1/2
LR 2532-20210 G	<b>Control set Herpes simplex virus 2 (HSV-2)</b>	IgG	2 x 0.5 ml control 1/2
LR 2580-20210 G	<b>Control set Parvovirus B19</b>	IgG	2 x 0.5 ml control 1/2
LR 2580-20210 M	<b>Control set Parvovirus B19</b>	IgM	2 x 0.5 ml control 1/2
LR 2606-20210-1 G	<b>Control set Anti-SARS-CoV-2 RBD ChLIA (IgG)</b>	IgG	2 x 0.5 ml control 1/2
LR 2791-20210 G	<b>Control set Epstein-Barr virus capsid antigen (EBV-CA)</b>	IgG	2 x 0.5 ml control 1/2
LR 2791-20210 M	<b>Control set Epstein-Barr virus capsid antigen (EBV-CA)</b>	IgM	2 x 0.5 ml control 1/2
LR 2793-20210 G	<b>Control set Epstein-Barr virus nuclear antigen 1 (EBNA-1)</b>	IgG	2 x 0.5 ml control 1/2





IDS Chemiluminescence Tests for Infectious Serology (Test Systems)		
IDS Order No.	Description	Format
IS-ID6101	IDS Tetanus IgG	100 determinations, calibrators incl.
IS-ID6201	IDS Borrelia Burgdorferi IgG	100 determinations, calibrators incl.
IS-ID6202	IDS Borrelia Burgdorferi IgM	100 determinations, calibrators incl.
YB500032	TGS TOXO IgG	100 determinations, calibrators incl.
YB500033	TGS TOXO IgM	100 determinations, calibrators incl.
YB500034	TGS TOXO IgG Avidity	50 determinations, calibrators incl.
IS-ID5701	IDS HSV 1/2 IgM	100 determinations, calibrators incl.
IS-ID5601	IDS HSV-1 IgG	100 determinations, calibrators incl.
IS-ID5602	IDS HSV-2 IgG	100 determinations, calibrators incl.
YB500035	TGS CMV IgG	100 determinations, calibrators incl.
YB500036	TGS CMV IgM	100 determinations, calibrators incl.
YB500037	TGS CMV IgG Avidity	50 determinations, calibrators incl.
IS-ID6301	IDS Parvovirus B19 IgG	50 determinations, calibrators incl.
IS-ID6302	IDS Parvovirus B19 IgM	50 determinations, calibrators incl.
YB500038	TGS Rubella IgG	100 determinations, calibrators incl.
YB500039	TGS Rubella IgM	100 determinations, calibrators incl.
YB500047	TGS Rubella IgG Avidity	50 determinations, calibrators incl.
CVCL100G	TGS COVID-19 IgG	100 determinations
CVCL100M	TGS COVID-19 IgM	100 determinations
IS-ID5901	IDS Measles IgG	50 determinations, calibrators incl.
IS-ID6001	IDS Measles IgM	50 determinations, calibrators incl.
IS-ID5902	IDS Mumps IgG	50 determinations, calibrators incl.
IS-ID6002	IDS Mumps IgM	50 determinations, calibrators incl.
IS-ID5903	IDS VZV IgG	50 determinations, calibrators incl.
IS-ID6003	IDS VZV IgM	50 determinations, calibrators incl.
IS-ID5801	IDS EBV VCA IgG	100 determinations, calibrators incl.
IS-ID5802	IDS EBV VCA IgM	100 determinations, calibrators incl.
IS-ID5803	IDS EBV EBNA-1 IgG	100 determinations, calibrators incl.
IS-ID5804	IDS EBV EA IgG	50 determinations, calibrators incl.



## IDS Control Sets for Chemiluminescence Tests

IDS Order No.	Description	Format
IS-ID6130	IDS Tetanus IgG Control Set	2 concentrations
IS-ID6230	IDS Borrelia Burgdorferi Control Set	2 concentrations
YB500040	TGS TOXO Control Set	2 concentrations
YB500041	TGS TOXO Avidity Control Set	2 concentrations
IS-ID5730	IDS HSV 1/2 IgM Control Set	2 concentrations
IS-ID5630	IDS HSV 1/2 IgG Control Set	2 concentrations
YB500042	TGS CMV Control Set	2 concentrations
YB500043	TGS CMV Avidity Control Set	2 concentrations
IS-ID6330	IDS Parvovirus B19 Control Set	2 concentrations
YB500044	TGS Rubella Control Set	2 concentrations
YB500048	TGS Rubella Avidity Control Set	2 concentrations
CVCLCSGM	TGS COVID-19 Control Set	2 concentrations
IS-ID5930	IDS MMV IgG Control Set	2 concentrations
IS-ID6030	IDS MMV IgM Control Set	2 concentrations
IS-ID5830	IDS EBV Control Set	2 concentrations




**Microplate ELISA for the Determination of Infectious Diseases, Antigen Detection (Test Systems)**

Order No.	Analyte	Calibration	Format
EQ 2606-9601	SARS-CoV-2 Antigen	semi-quantitative	96 x 01
EQ 266a-9601-1	Dengue virus NS1 antigen detection (DENV)	1/10/100 RU/ml	96 x 01
EQ 6811-9601-L	CXCL13 determination in CSF	0-500 pg/ml	96 x 01
EQ 6841-9601	Quan-T-Cell ELISA To be used in combination with ET 2606	12-400 mIU/ml	96 x 01
EQ 6911-9601	Aspergillus antigen	0/20/50/125/312.5/625 pg/ml	96 x 01

**T-Cell Stimulation Tube Sets for the Determination of Infectious Diseases**

Order No.	Analyte	Calibration	Format
ET 2606-3003	Quan-T-Cell SARS-CoV-2 To be used in combination with EQ 6841	–	30 x 03



### ELISA Controls for Infectious CSF Diagnostics

Order No.	Control (Ready for use)	Ig Class	Format
CK2111-0220-L G	CSQ pair of controls anti-Treponema pallidum (IgG)	IgG	2 x 2 ml, ready for use
CK2132-0220-L G	CSQ pair of controls anti-Borrelia (IgG)	IgG	2 x 2 ml, ready for use
CK2132-0220-L M	CSQ pair of controls anti-Borrelia (IgM)	IgM	2 x 2 ml, ready for use
CK2410-0220-L G	CSQ pair of controls anti-Toxoplasma gondii (IgG)	IgG	2 x 2 ml, ready for use
CK2531-0220-1 L G	CSQ pair of controls anti-HSV-1/2 Pool (IgG)	IgG	2 x 2 ml, ready for use
CK2570-0220-L G	CSQ pair of controls anti-Cytomegalovirus (IgG)	IgG	2 x 2 ml, ready for use
CK2590-0220-L G	CSQ pair of controls anti-Rubella virus (IgG)	IgG	2 x 2 ml, ready for use
CK2610-0220-L G	CSQ pair of controls anti-Measles virus (IgG)	IgG	2 x 2 ml, ready for use
CK2630-0220-L G	CSQ pair of controls anti-Mumps virus (IgG)	IgG	2 x 2 ml, ready for use
CK2650-0220-L G	CSQ pair of controls anti-VZV (IgG)	IgG	2 x 2 ml, ready for use
CK2661-0220-9 L G	CSQ pair of controls anti-TBE virus Vienna (IgG)	IgG	2 x 2 ml, ready for use
CK2661-0220-L G	CSQ pair of controls anti-TBE virus (IgG)	IgG	2 x 2 ml, ready for use
CK2661-0220-L M	CSQ pair of controls anti-TBE virus (IgM)	IgM	2 x 2 ml, ready for use
CK2791-0220-L G	CSQ pair of controls anti-EBV-CA (IgG)	IgG	2 x 2 ml, ready for use



Diagnostics for Indirect Immunofluorescence: Infectious Serology					
Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FI 2050-1005-1 G FI 2050-1010-1 G	<b>Bordetella pertussis</b> <b>Bordetella parapertussis</b>	IgG	bacterial smears (2 BIOCHIPS per field)	B. pertussis B. parapertussis	10 x 05 (test system) 10 x 10 (test system)
FI 2111-1005 G FI 2111-1010 G FI 2111-1005 M FI 2111-1010 M	<b>Treponema pallidum (FTA-ABS)</b>	IgG IgM	bacterial smear verification BIOCHIP (2 BIOCHIPS per field)	T. pallidum	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FI 2112-1005 G FI 2112-1010 G FI 2112-1005 M FI 2112-1010 M	<b>Treponema pallidum (FTA-ABS)</b>	IgG IgM	bacterial smears verification BIOCHIP (3 BIOCHIPS per field)	T. pallidum T. phagedenis	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FI 2136-1005-1 G FI 2136-1010-1 G FI 2136-1005-1 M FI 2136-1010-1 M	<b>EUROPLUS</b> <b>Borrelia afzelii</b> <b>Borrelia burgdorferi (USA)</b> <b>OspC antigen</b> <b>VlsE antigen</b>	IgG IgM	4 BIOCHIPS per field: bacterial smear bacterial smear OspC BIOCHIPS VlsE BIOCHIPS	B. afzelii B. burgd. (USA) B. burgdorferi recombinant	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FI 2141-1005-1 G FI 2141-1010-1 G	<b>Listeria monocytogenes 1/2a and 4b</b>	IgG	bacterial smears (2 BIOCHIPS per field)	Listeria monocytogenes 1/2a and 4b	10 x 05 (test system) 10 x 10 (test system)
FI 2191-1005-3 A FI 2191-1010-3 A FI 2191-1005-3 G FI 2191-1010-3 G FI 2191-1005-3 M FI 2191-1010-3 M	<b>Anti-Chlamydia MIF</b> <b>Chlamydia trachomatis</b> <b>Chlamydia pneumoniae</b> <b>Chlamydia psittaci</b>	IgA EB IgG EB IgM EB	4 BIOCHIPS per field: elementary bodies and non-infected cells	EU 40 EU 40 EU 40	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FR 2191-1005-3 A FR 2191-1010-3 A FR 2191-1005-3 G FR 2191-1010-3 G FR 2191-1005-3 M FR 2191-1010-3 M	<b>Anti-Chlamydia MIF EUROPattern</b> <b>Chlamydia trachomatis</b> <b>Chlamydia pneumoniae</b> <b>Chlamydia psittaci</b>	IgA EB IgG EB IgM EB	4 BIOCHIPS per field: elementary bodies and non-infected cells	EU 40 EU 40 EU 40	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FI 2191-1005-80 A FI 2191-1005-80 G FI 2191-1005-80 M	<b>Chlamydia trachomatis</b>	IgA EB IgG EB IgM EB	elementary bodies (MIF) non-infected cells (2 BIOCHIPS per field)	EU 40 EU 40	10 x 05 (test system) 10 x 05 (test system) 10 x 05 (test system)
FI 2192-1005-80 A FI 2192-1005-80 G FI 2192-1005-80 M	<b>Chlamydia pneumoniae</b>	IgA EB IgG EB IgM EB	elementary bodies (MIF) non-infected cells (2 BIOCHIPS per field)	EU 40 EU 40	10 x 05 (test system) 10 x 05 (test system) 10 x 05 (test system)
FR 2192-1005-80 A FR 2192-1005-80 G FR 2192-1005-80 M	<b>Chlamydia pneumoniae EUROPattern</b>	IgA EB IgG EB IgM EB	elementary bodies (MIF) non-infected cells (2 BIOCHIPS per field)	EU 40 EU 40	10 x 05 (test system) 10 x 05 (test system) 10 x 05 (test system)
FI 219b-1005 G FI 219b-1010 G FI 219b-1005 M FI 219b-1010 M	<b>Bartonella henselae</b>	IgG IgM EB	infected cells infected and non-infected cells (2 BIOCHIPS per field)	EU 70	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FI 219b-1005-1 G FI 219b-1010-1 G FI 219b-1005-1 M FI 219b-1010-1 M	<b>Bartonella henselae</b> <b>Bartonella quintana</b>	IgG IgM EB	infected cells infected cells (2 BIOCHIPS per field) infected and non-infected cells (4 BIOCHIPS per field)	EU 70 EU 70 EU 70 EU 38	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FR 219b-1005-1 G FR 219b-1010-1 G FR 219b-2010-1 M	<b>Bartonella henselae EUROPattern</b> <b>Bartonella quintana EUROPattern</b>	IgG PI IgM EB	infected cells infected cells (2 BIOCHIPS per field) infected and non-infected cells (4 BIOCHIPS per field)	EU 70 EU 70 EU 70 EU 38	10 x 05 (test system) 10 x 10 (test system) 20 x 10 (test system)



## Diagnostics for Indirect Immunofluorescence: Infectious Serology

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FI 2201-1005-1 G FI 2201-1010-1 G FI 2201-1005-1 M FI 2201-1010-1 M	<b>Mycoplasma hominis</b> <b>Ureaplasma urealyticum</b>	IgG EB  IgM EB	infected cells infected cells non-infected cells (3 BIOCHIPS per field)	EU 38 EU 38 EU 38	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FR 2201-1005-1 G FR 2201-1010-1 G	<b>Mycoplasma hominis EUOPattern</b> <b>Ureaplasma urealyticum EUOPattern</b>	IgG EB	infected cells infected cells non-infected cells (3 BIOCHIPS per field)	EU 38 EU 38 EU 38	10 x 05 (test system) 10 x 10 (test system)
FI 2231-1005 G FI 2231-1010 G FI 2231-1005 M FI 2231-1010 M	<b>Leishmania donovani</b> <b>(promastigote)</b>	IgG  IgM	protozoan smear	Leishmania donovani	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FI 2300-1005 G	<b>Schistosoma</b> <b>mansoni</b>	IgG	frozen sections	Schistosoma mansoni, adult	10 x 05 (test system)
FI 2410-1005 G FI 2410-1010 G FI 2410-1005 M FI 2410-1010 M	<b>Toxoplasma</b> <b>gondii</b>	IgG  IgM	protozoan smear	Toxoplasma gondii	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FI 2536-1005 G FI 2536-1010 G FI 2536-2005 G FI 2536-2010 G FI 2536-1005 M FI 2536-1010 M FI 2536-2005 M FI 2536-2010 M	<b>HHV-6</b>	IgG    IgM	infected cells	EU 30	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FR 2536-1005 G FR 2536-1010 G FR 2536-2005 G FR 2536-2010 G FR 2536-1005 M FR 2536-1010 M FR 2536-2005 M FR 2536-2010 M	<b>HHV-6 EUOPattern</b>	IgG EB    IgM EB	infected cells	EU 30	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 20 x 10 (test system)
FI 2601-1010 G FI 2601-1010 M	<b>SARS coronavirus</b>	IgG IgM	infected and non- infected cells (2 BIOCHIPS per field)	EU 14	10 x 10 (test system) 10 x 10 (test system)
FI 2604-1005 G FI 2604-1010 G FI 2604-1005 M FI 2604-1010 M	<b>MERS coronavirus</b>	IgG  IgM	infected and non- infected cells (2 BIOCHIPS per field)	EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FI 2620-1005 G * FI 2620-1010 G *	<b>Bornavirus (BoDV)</b>	IgG	infected and uninfected cells (2 BIOCHIPS per field)	EU 14	10 x 05 (test system) 10 x 10 (test system)
FI 2650-1005 G FI 2650-1010 G FI 2650-1005 M FI 2650-1010 M	<b>Varicella zoster virus</b> <b>(VZV)</b>	IgG  IgM	infected cells	EU 168	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FI 2661-1005 G FI 2661-1010 G FI 2661-1005 M FI 2661-1010 M	<b>TBE virus (TBEV)</b>	IgG  IgM	infected and non- infected cells (2 BIOCHIPS per field)	EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)

\* For research use only, not for in vitro diagnostic use in the sense of EU directive 98/79/EC.





## Diagnostics for Indirect Immunofluorescence: Infectious Serology

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FI 2661-1005-1 G FI 2661-1010-1 G FI 2661-1005-1 M FI 2661-1010-1 M	<b>Flavivirus Mosaic 1</b> TBE virus (TBEV) West Nile virus (WNV) Japanese encephalitis virus (JEV) Yellow fever virus (YFV)	IgG  IgM	4 BIOCHIPS per field: infected cells infected cells infected cells infected cells	EU 14 EU 14 EU 14 EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FI 2661-1005-2 G FI 2661-2005-2 G FI 2661-1005-2 M FI 2661-2005-2 M	<b>Flavivirus Profile 2</b> upper row: TBE virus (TBEV) West Nile virus (WNV) Japanese encephalitis virus (JEV) Yellow fever virus (YFV) bottom row: Dengue virus types 1 - 4 (DENV)	IgG  IgM	 infected cells infected cells infected cells infected cells  infected cells	 EU 14 EU 14 EU 14 EU 14  EU 14	10 x 05 (test system) 20 x 05 (test system) 10 x 05 (test system) 20 x 05 (test system)   10 x 05 (test system)
FI 2662-1005 G FI 2662-1010 G FI 2662-1005 M FI 2662-1010 M	West Nile virus (WNV)	IgG  IgM	infected and non- infected cells (2 BIOCHIPS per field)	EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FI 2663-1005 G FI 2663-1005 M	Japanese encephalitis virus (JEV)	IgG IgM	infected and non- infected cells (2 BIOCHIPS per field)	EU 14	10 x 05 (test system) 10 x 05 (test system)
FI 2664-1005-2 G * FI 2664-1010-2 G * FI 2664-1005-2 M * FI 2664-1010-2 M *	<b>Arbovirus Mosaic America 2</b> St. Louis encephalitis virus (SLEV) La crosse virus (LACV) Eastern equine encephalitis virus (EEEV) Western equine encephalitis virus (WEEV)	IgG  IgM	4 BIOCHIPS per field: infected cells infected cells infected cells infected cells	EU 14 EU 14 EU 14 EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FI 2665-1005 G FI 2665-1010 G FI 2665-1005 M FI 2665-1010 M	Yellow fever virus (YFV)	IgG  IgM	infected and non- infected cells (2 BIOCHIPS per field)	EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FR 2665-1005 G FR 2665-1005 M	Yellow fever virus (YFV) EUOPattern	IgG PI IgM PI	infected and non- infected cells (2 BIOCHIPS per field)	EU 14	10 x 05 (test system) 10 x 05 (test system)
FI 2666-1005-2 G * FI 2666-1005-2 M *	<b>Arbovirus Mosaic Australia 2</b> Murray Valley encephalitis virus (MVEV) Ross River virus (RRV) Barmah forest virus (BFV)	IgG IgM	4 BIOCHIPS per field: infected cells infected cells infected cells non-infected cells	EU 14 EU 14 EU 14 EU 14	10 x 05 (test system) 10 x 05 (test system)
FI 2668-1005 G FI 2668-1010 G FI 2668-1005 M FI 2668-1010 M	Zika virus (ZIKV)	IgG  IgM	infected and non- infected cells (2 BIOCHIPS per field)	EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FR 2668-1005 G FR 2668-1010 G FR 2668-1005 M FR 2668-1010 M	Zika virus (ZIKV) EUOPattern	IgG PI IgM PI	infected and non- infected cells (2 BIOCHIPS per field)	EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FI 2668-1005-1 G FI 2668-1010-1 G FI 2668-1005-1 M FI 2668-1010-1 M	<b>Arbovirus Fever Mosaic 2</b> Zika virus (ZIKV) Chikungunya virus (CHIKV) Dengue virus types 1 - 4 (DENV)	IgG  IgM	6 BIOCHIPS per field: infected cells infected cells infected cells	EU 14 EU 14 EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FR 2668-1005-1 G FR 2668-1010-1 G FR 2668-1005-1 M FR 2668-1010-1 M	<b>Arbovirus Fever Mosaic 2 EUOPattern</b> Zika virus (ZIKV) Chikungunya virus (CHIKV) Dengue virus types 1 - 4 (DENV)	IgG PI  IgM PI	6 BIOCHIPS per field: infected cells infected cells infected cells	EU 14 EU 14 EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)

\* For research use only, not for in vitro diagnostic use in the sense of EU directive 98/79/EC.



## Diagnostics for Indirect Immunofluorescence: Infectious Serology

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FI 2668-1005-3 G FI 2668-1005-3 M	<b>Arbovirus Profile 3</b> upper row : Zika virus (ZIKV) Chikungunya virus (CHIKV) Dengue virus types 1 - 4 (DENV) bottom row: TBE virus (TBEV) West Nile virus (WNV) Japanese encephalitis virus (JEV) Yellow fever virus (YFV)	IgG IgM	infected cells infected cells infected cells infected cells infected cells infected cells infected cells	EU 14 EU 14 EU 14 EU 14 EU 14 EU 14 EU 14	10 x 05 (test system) 10 x 05 (test system)
FI 266a-1005-1 G FI 266a-1010-1 G FI 266a-2005-1 G FI 266a-1005-1 M FI 266a-1010-1 M FI 266a-2005-1 M	<b>Mosaic Dengue virus</b> types 1 - 4 (DENV)	IgG IgM	4 BIOCHIPS per field: infected cells	EU 14	10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system) 10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system)
FR 266a-1005-1 G FR 266a-1010-1 G FR 266a-1005-1 M FR 266a-1010-1 M	<b>Mosaic Dengue virus</b> types 1 - 4 (DENV) EUROPattern	IgG PI IgM PI	4 BIOCHIPS per field: infected cells	EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FI 2730-1005-2 G FI 2730-2005-2 G FI 2730-2010-2 G FI 2730-1005-2 M FI 2730-2005-2 M FI 2730-2010-2 M	<b>Mosaic Coxsackie virus A types</b> types A7, A9, A16, A24	IgG IgM	4 BIOCHIPS per field: infected cells	EU 38	10 x 05 (test system) 20 x 05 (test system) 20 x 10 (test system) 10 x 05 (test system) 20 x 05 (test system) 20 x 10 (test system)
FR 2730-2010-2 G FR 2730-2010-2 M	<b>Coxsackie virus screen (types A) EUROPattern</b> types A7, A9, A16, A24	IgG PI IgM PI	4 BIOCHIPS per field: infected cells	EU 38	20 x 10 (test system) 20 x 10 (test system)
FI 2730-2005-3 G FI 2730-2005-3 M	<b>Mosaic Coxsackie virus B types</b> types B1, B2, B3, B4, B5, B6	IgG IgM	6 BIOCHIPS per field: infected cells	EU 38	20 x 05 (test system) 20 x 05 (test system)
FR 2730-2010-3 G FR 2730-2010-3 M	<b>Coxsackie virus screen (types B) EUROPattern</b> types B1, B2, B3, B4, B5, B6	IgG PI IgM PI	6 BIOCHIPS per field: infected cells	EU 38	20 x 10 (test system) 20 x 10 (test system)
FI 277a-1005-1 G FI 277a-1010-1 G FI 277a-1005-1 M FI 277a-1010-1 M	<b>Sandfly fever virus Mosaic 1</b> types Sicilian, Naples, Toscana, Cyprus	IgG IgM	4 BIOCHIPS per field: infected cells	EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FR 277a-1005-1 G FR 277a-1005-1 M	<b>Sandfly fever virus Mosaic 1</b> EUROPattern types Sicilian, Naples, Toscana, Cyprus	IgG PI IgM PI	4 BIOCHIPS per field: infected cells	EU 14	10 x 05 (test system) 10 x 05 (test system)
FI 278h-1005-1 G FI 278h-1010-1 G FI 278h-1005-1 M FI 278h-1010-1 M	<b>Hantavirus Mosaic 1</b> types Hantaan (HTNV), Sin Nombre (SNV), Puumala (PUUV), Dobrava (DOBV), Seoul (SEOV), Saaremaa (SAAV)	IgG IgM	6 BIOCHIPS per field: infected cells	EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)
FR 278h-1005-1 G FR 278h-1005-1 M	<b>Hantavirus Mosaic 1 EUROPattern</b> types Hantaan (HTNV), Sin Nombre (SNV), Puumala (PUUV), Dobrava (DOBV), Seoul (SEOV), Saaremaa (SAAV)	IgG PI IgM PI	6 BIOCHIPS per field: infected cells	EU 14	10 x 05 (test system) 10 x 05 (test system)
FI 278h-1005-2 G FI 278h-1010-2 G FI 278h-1005-2 M FI 278h-1010-2 M	<b>Hantavirus Mosaic 2 Eurasia</b> types Hantaan (HTNV), Puumala (PUUV), Dobrava (DOBV), Seoul (SEOV), Saaremaa (SAAV)	IgG IgM	6 BIOCHIPS per field: infected and non- infected cells	EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)



Diagnostics for Indirect Immunofluorescence: Infectious Serology					
Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FI 278m-1005-3 G FI 278m-1005-3 M	Hantavirus Mosaic 3: America types Sin Nombre (SNV), Andes (ANDV)	IgG IgM	2 BIOCHIPS per field: infected cells	EU 14	10 x 05 (test system) 10 x 05 (test system)
FR 278m-1005-3 G FR 278m-1005-3 M	Hantavirus Mosaic 3: America types Sin Nombre (SNV), Andes (ANDV) EUROPattern	IgG PI IgM PI	2 BIOCHIPS per field: infected cells	EU 14	10 x 05 (test system) 10 x 05 (test system)
FI 2791-1005 G FI 2791-1010 G FI 2791-2010 G FI 2791-1005 M FI 2791-1010 M FI 2791-2005 M	Epstein-Barr virus capsid antigen (EBV-CA)	IgG EB   IgM EB	expressing cells	P3HR1	10 x 05 (test system) 10 x 10 (test system) 20 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system) 20 x 05 (test system)
FR 2791-1005 G FR 2791-1010 G FR 2791-2010 G FR 2791-1010 M	Epstein-Barr virus capsid antigen (EBV-CA) EUROPattern Anti-EBV-CA IIFT EUROPattern (IgM)	IgG PI   IgM PI	expressing cells	P3HR1	10 x 05 (test system) 10 x 10 (test system) 20 x 10 (test system) 10 x 10 (test system)
FI 2793-1010 C	Epstein-Barr virus nuclear antigen (EBNA, complement-fixing antibodies)	C3c EB	expressing cells	Raji	10 x 10 (test system)
FR 2793-1010 C	Epstein-Barr virus nuclear antigen (EBNA) EUROPattern	C3c PI	expressing cells	Raji	10 x 10 (test system)
FI 2795-1005 G FI 2795-1010 G	Epstein-Barr virus early antigen (EBV-EA)	IgG EB	expressing cells	EU 33	10 x 05 (test system) 10 x 10 (test system)
FR 2795-1005 G FR 2795-1010 G	Epstein-Barr virus early antigen (EBV-EA) EUROPattern	IgG PI	expressing cells	EU 33	10 x 05 (test system) 10 x 10 (test system)
FI 2799-1001-1 X FI 2799-1002-1 X FI 2799-2001-1 X FI 2799-2002-1 X	BIOCHIP Sequence EBV fields A and B: EBV-CA (IgG) field C: EBV-CA (IgM) field D: EBV-EA field E: EBNA format 1001: per slide one patient format 1002: per slide two patients	avidity test	expressing cells expressing cells expressing cells expressing cells	P3HR1 P3HR1 EU 33 Raji	10 x 01 (test system) 10 x 02 (test system) 20 x 01 (test system) 20 x 02 (test system)
FI 2799-1001-21 X FI 2799-1002-21 X FI 2799-2001-21 X FI 2799-2002-21 X	EUROPLUS BIOCHIP Sequence EBV field A: EBV-CA (IgG), gp125 ag, p19 ag field B: EBV-CA (IgG) field C: EBV-CA (IgM), gp125 ag, p19 ag field D: EBV-EA field E: EBNA format 1001: per slide one patient format 1002: per slide two patients	avidity test	expr. cells, gp125/p19/ag-free BIOCHIP expressing cells expressing cells expr. cells, gp125/p19/ag-free BIOCHIP expressing cells	P3HR1, native/rec. EU 120 P3HR1 P3HR1, native/rec. EU 120 EU 33 Raji	10 x 01 (test system) 10 x 02 (test system) 20 x 01 (test system) 20 x 02 (test system)
FI 279a-1005-2 G FI 279a-1010-2 G FI 279a-2010-2 G FI 279a-1005-2 M FI 279a-1010-2 M FI 279a-2010-2 M	Crimean Congo fever virus Mosaic 2 CCHFV-GPC CCHFV-N	IgG EB   IgM EB	3 BIOCHIPS per field: transfected cells transfected cells control transfection	EU 90 EU 90 EU 90	10 x 05 (test system) 10 x 10 (test system) 20 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system) 20 x 10 (test system)
FI 280a-1005 G FI 280a-1010 G FI 280a-1005 M FI 280a-1010 M	Rift Valley fever virus (RVFV)	IgG   IgM	infected and non-infected cells (2 BIOCHIPS per field)	EU 14	10 x 05 (test system) 10 x 10 (test system) 10 x 05 (test system) 10 x 10 (test system)



## Diagnostics for Indirect Immunofluorescence: Infectious Serology

Order No.	Antibodies against	Ig Class	Substrate	Species	Format Slides x Fields
FI 291a-1005 G *	<b>Sindbis virus (SINV)</b>	IgG	infected and non- infected cells	EU 14	10 x 05 (test system)
FI 291a-1010 G *					10 x 10 (test system)
FI 291a-1005 M *		IgM	(2 BIOCHIPS per field)		10 x 05 (test system)
FI 291a-1010 M *					10 x 10 (test system)
FI 293a-1005 G	<b>Chikungunya virus (CHIKV)</b>	IgG	infected and non- infected cells	EU 14	10 x 05 (test system)
FI 293a-1010 G					10 x 10 (test system)
FI 293a-2005 G					20 x 05 (test system)
FI 293a-1005 M		IgM	(2 BIOCHIPS per field)		10 x 05 (test system)
FI 293a-1010 M					10 x 10 (test system)
FI 293a-2005 M					20 x 05 (test system)
FR 293a-1005 G	<b>Chikungunya virus (CHIKV) EUROPattern</b>	IgG PI	infected and non- infected cells	EU 14	10 x 05 (test system)
FR 293a-1010 G					10 x 10 (test system)
FR 293a-1005 M		IgM PI	(2 BIOCHIPS per field)		10 x 05 (test system)
FR 293a-1010 M					10 x 10 (test system)
FI 293a-1005-1 G	<b>Arbovirus Fever Mosaic 1</b> <b>Chikungunya virus (CHIKV)</b> <b>Japanese encephalitis virus (JEV)</b> <b>Dengue virus types 1 - 4 (DENV)</b>	IgG	6 BIOCHIPS per field: infected cells	EU 14	10 x 05 (test system)
FI 293a-1010-1 G					10 x 10 (test system)
FI 293a-1005-1 M		IgM	infected cells		10 x 05 (test system)
FI 293a-1010-1 M					10 x 10 (test system)

\* For research use only, not for in vitro diagnostic use in the sense of EU directive 98/79/EC.  
For individual test kit controls please contact your respective sales representative.





# Allergy diagnostics







# Specific IgE

Inhalation · Food · Atopy · Anti-CCD absorbent



For more information on this subject scan the QR code or enter the Quick Link code **q002** at [www.euroimmun.com](http://www.euroimmun.com)

## Inhalation

■ **Clinical information:** In the case of inhalation allergies, the allergens enter the body through the air and through the mucous membranes, leading to measurable IgE concentrations against a specific allergen source. Seasonal allergens (pollen from trees, grasses and herbs) play a role, as do also indoor allergens (house dust mites, domestic animals and mould spores) which occur the whole year round. The symptoms generally occur shortly after contact with the allergen. These allergies are therefore called immediate type reactions, which can be found in more than 15% of the population in industrialised countries. If a systemic allergic reaction occurs, serious, even life-threatening reactions can result (anaphylactic shock). Typical allergic reactions are rhinitis, conjunctivitis and allergic asthma. Allergic rhinitis is increasing worldwide, with a prevalence of 10 to 40% in various regions.

■ **Diagnostics:** A confirmed allergy diagnosis demands an extensive patient anamnesis and various diagnostic methods (in vivo and in vitro tests), depending on the patient's clinical symptoms. In vitro diagnostics are based on the detection of total and specific IgE (sIgE) in serum or plasma. In individual cases, provocation tests can be additionally performed to help with the diagnosis. The results of the various diagnostic methods are of equal value and complement each other. All individual results must always be interpreted within the context of the anamnesis and the clinical findings.



Various **inhalation profiles** (EUROLINE) are available for the clarification of inhalation allergies. Depending on the test system, these permit semi-quantitative or quantitative in vitro determination of human IgE antibodies against the most frequent inhalation allergens in serum or plasma. Moreover, **country-specific inhalation profiles** are available, which offer different allergen compositions optimised with regard to regional relevance.


In addition, the total IgE concentration in the serum can be determined using the Total IgE ELISA to allow differentiation between allergic and intrinsic asthma, between allergic and vasomotor rhinitis and between atopic and seborrhoeic dermatitis.



## Product overview

Method	Substrate	Application	Order number	Page
EUROLINE*	Inhalation (g1, g3, g6, g12, t2, t3, t4, t7, w1, w6, w9, d1, d2, e1, e2, e3, m1, m2, m3, m6, CCD)	Efficient screening for sIgE against the most important inhalation allergens	DP 3110-1601 E	233
	Paediatric Inhalation (g6, g12, t2, t3, t4, w6, w8, w9, d1, d2, e1, e2, e3, e6, e82, e84, m1, m2, m3, m6, CCD)	Efficient screening for sIgE against inhalation allergens relevant in childhood	DP 3111-1601 E	233
ELISA	Total IgE	ELISA for quantitative determination of human IgE in serum	EV 3840-9601 E	146

\* Further profiles from page 233

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 239).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g074** at [www.euroimmun.com](http://www.euroimmun.com)



# Specific IgE

Inhalation ·  Food · Atopy · Anti-CCD absorbent



For more information on this subject scan the QR code or enter the Quick Link code **q003** at [www.euroimmun.com](http://www.euroimmun.com)

## Food

■ **Clinical information:** In food allergies, the IgE-induced immune reaction can lead to symptoms such as burning or itching in the oral cavity, nausea, gastrointestinal spasms, diarrhoea and skin rashes within a short period after ingesting the food. Severe reactions can also result in asthma attacks, breathlessness, increased heart rate or in panic attacks and confusion. In rare cases, an anaphylactic shock can occur. Foods that most frequently cause allergic reactions include nuts and peanuts, soy, wheat, fish, milk and eggs. With a prevalence of 5 to 10%, primary allergic sensitisations to foods play an important role, particularly in babies and infants. Food allergies in adults occur with a prevalence of 1 to 5%.

■ **Diagnostics:** Various food allergy profiles (EUROLINE) are available for the clarification of food allergies. These enable semi-quantitative in vitro determination of human IgE antibodies against the most frequent food allergens in serum or plasma. Moreover, country-specific food allergy profiles are available which have been developed with regard to the regional eating habits.

In addition, the total IgE concentration in the serum can be determined using the Total IgE ELISA.






## Product overview

Method	Substrate	Application	Order number	Page
EUROLINE*	Food (f1, f75, f2, f45, f4, f5, f9, f13, f14, f17, f20, f49, f84, f237, f25, f31, f35, f85, f3, f23, CCD)	Efficient screening for IgE antibodies against the most important food allergens	DP 3410-1601 E	234
	Food "Gulf" (f1, f75, f2, f105, f4, f14, f45, fs36, f13, f92, f33, f44, f93, f25, f31, f48, f83, f88, f3, f23, CCD)	Efficient screening for sIgE against the relevant regional food allergens	DP 3416-1601 E	235
	Food "Turkey 1" (f1, f75, f2, f169, f78, f4, f79, f9, f14, f10, f13, f17, f144, u87, f222, f73, f33, f44, f49, f92, f84, f146, f328, f25, f31, f35, f48, f95, f97, f122, f132, fs14, fs10, fs43, f83, CCD)		DP 3420-1601-11 E	235
ELISA	Total IgE	ELISA for quantitative determination of human IgE in serum	EV 3840-9601 E	146

\* Further profiles from page 233

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 239).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g081** at [www.euroimmun.com](http://www.euroimmun.com)



# Specific IgE

Inhalation · Food · Atopy · Anti-CCD absorbent



For more information on this subject scan the QR code or enter the Quick Link code **q001** at [www.euroimmun.com](http://www.euroimmun.com)

## Atopy

■ **Clinical information:** Atopy is a genetic predisposition to allergic hypersensitivity reactions which can have various clinical manifestations. The allergens responsible for the reaction enter the body either through the air and the mucous membranes (in the case of inhalation allergies), or through food ingestion (in the case of food allergies). However, allergic reactions to foods of plant origin can also be caused by cross-reacting IgE antibodies. These reactions, termed cross-allergies, are based on the structural similarity between proteins which are present in both the food as well as in the corresponding inhalation allergens of plant origin. An example of this is the phenomenon known as "oral allergy syndrome" (OAS). Accordingly, patients with a primary birch pollen allergy can also develop allergic reactions to apple, celery, hazelnut, potato or kiwi. Multiple sensitisations to allergens of different origin are therefore not uncommon.

■ **Diagnostics:** Various **atopy profiles** (EUROLINE) are available for the clarification of multiple sensitisations. These permit the simultaneous in vitro determination of human IgE antibodies against the most frequent inhalation and food allergens in serum or plasma. Moreover, **country-specific profiles** are available which take into account the characteristics of the regional allergen exposure.

In addition, the total IgE concentration in the serum can be determined using the Total IgE ELISA.








## Product overview

Method	Substrate	Application	Order number	Page
EUROLINE*	Atopy (g6, g12, t3, w6, d1, e1, e2, e3, m2, m6, f1, f2, f3, f4, f9, f14, f17, f31, f35, f49, CCD)	Efficient screening for sIgE antibodies against the most important inhalation and food allergens	DP 3710-1601 E	237
	Paediatrics (gx, t3, w6, d1, d2, e1, e2, e3, m2, m3, m6, f1, f75, f2, f3, f76, f77, f78, e204, f4, f9, f14, f13, f17, f31, f35, f49, CCD)	Efficient screening for sIgE against inhalation and food allergens relevant in childhood	DP 3712-1601 E	237
ELISA	Total IgE	ELISA for quantitative determination of human IgE in serum	EV 3840-9601 E	146

\* Further profiles from page 233

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 239).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g053** at [www.euroimmun.com](http://www.euroimmun.com)



# Specific IgE

Inhalation · Food · Atopy · Anti-CCD absorbent



For more information on this subject scan the QR code or enter the Quick Link code **q161** at [www.euroimmun.com](http://www.euroimmun.com)

## Anti-CCD absorbent

■ **Background:** Anti-CCD absorbent is an additional reagent designed for the incubation with blot-based allergy profiles. The absorbent eliminates anti-CCD IgE antibodies from patient serum, which increases the specificity of test results if these antibodies are present in the sample.

Anti-CCD IgE antibodies are directed against sugar structures on proteins and can be detected in around 25% of allergy patients as well as in non-allergic individuals. They generally have no clinical relevance.


In extract-based in vitro allergy diagnostics, these antibodies complicate the interpretation of positive results because the following cases cannot be differentiated:

- positive reaction caused by IgE antibodies against peptide epitopes
- positive reaction caused by anti-CCD IgE antibodies
- positive reaction caused by a combination of the two antibody types

Differentiation between the described reactions is possible if the absorbent is used and the anti-CCD IgE antibodies are eliminated.

■ **Indication:** The anti-CCD absorbent is useful if the patient sample demonstrably contains IgE antibodies against CCD structures. This is indicated by a positive CCD band on the incubated allergy profile. In this case, the serum should be retested using the anti-CCD absorbent.

■ **Test principle:** The patient sample is incubated with anti-CCD absorbent for 60 minutes at room temperature according to the instructions provided with the reagent. Afterwards, the sample can be tested directly using the desired allergy profiles.



## Product overview

Method	Substrate	Application	Order number	Page
EUROLINE	Anti-CCD absorbent	Increases the specificity of test results in allergy profiles, if the patient sample contains anti-CCD IgE antibodies	ZD 3001_0101 ZD 3001_0401	306



# Molecular allergy diagnostics

DPA-Dx (Defined partial allergen diagnostics) · Insect venoms



For more information on this subject scan the QR code or enter the Quick Link code **q039** at [www.euroimmun.com](http://www.euroimmun.com)

## DPA-Dx (Defined partial allergen diagnostics)


■ **Indication:** Allergy sufferers frequently exhibit specific IgE antibodies to various allergen sources. Such multiple sensitisation patterns are often caused by **cross-reactions** of IgE antibodies against single, structurally similar proteins (components) from the allergen sources.

In defined partial allergen diagnostics (DPA-Dx), in contrast to classic extract-based allergy diagnostics, single purified allergen components are used. This approach allows identification of the components responsible for the sensitisation and enables, for example:

- Assessment of the risk of a severe systemic reaction to the allergen
- Differentiation of a primary sensitisation from cross-reactivity. In the latter the patient should be advised about the allergen sources that could trigger a reaction.
- Selection of a specific immunotherapy (SIT) for the patient
- Evaluation of the likelihood of tolerance induction

■ **Diagnostics:** Use of DPA-Dx systems is especially relevant for the differential diagnosis of inhalation, food and insect venom allergies.

**Inhalation allergy:** In allergy patients with multiple pollen sensitisations, DPA-Dx offers the possibility to differentiate between primary and cross sensitisations. This differentiation delivers important information for the targeted selection of suitable immunotherapy. For the analysis of multiple pollen sensitisations, allergen components of birch (Bet v 1 (t215), Bet v 2 (t216), Bet v 4 (t220) and Bet v 6 (t225)) and grasses (Phl p 1 (g205), Phl p 5 (g215), Phl p 7 (g210) and Phl p 12 (g212)) have been defined as markers for primary or cross sensitisation.

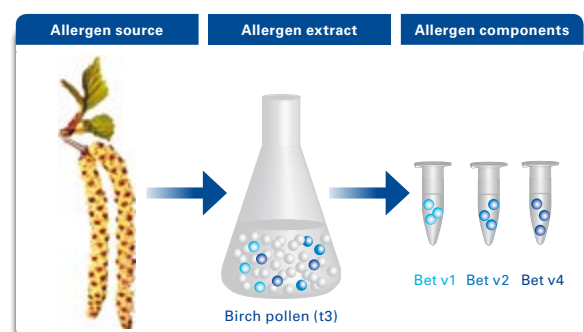

**Food allergy:** In the area of food allergies, allergen components allow assessment of the risk of a severe reaction and evaluation of the possible development of tolerance. Moreover, primary allergies can be differentiated from pollen-associated food allergies. This allows a targeted statement concerning therapy and food elimination.




Insect venom allergy: 50% of insect venom allergy sufferers show a double sensitisation to bee and wasp venom in extract-based allergy diagnostics. In these cases it is necessary to determine if the patient has a genuine primary sensitisation to both venoms or if the result is due to cross-reactivity. The use of species-specific components in DPA-Dx provides diagnostic clarification, enabling selection of a suitable immunotherapy.

## Product overview

Method	Substrate	Application	Order number	Page
EUROLINE*	DPA-Dx Pollen 1 (t3, g6, t215, t216, t220, t225, g205, g215, g210, g212, CCD)	Component-resolved differential diagnostics for multiple pollen sensitisations (birch, timothy grass)	DP 3210-1601-1 E	233
	DPA-Dx Paediatrics 1 (f427, f424, f423, f422, f356, f323, f233, f232, e204, f334, f78, f77, f76, t215, CCD)	Component-resolved differential diagnostics for food allergies (milk, egg, peanut) in infants	DP 3812-1601-1 E	238
	DPA-Dx Peanut 1 (t215, f422, f423, f424, f427, f429, f444, f445, CCD)	Component-resolved differential diagnostics for peanut allergies	DP 3511-1601-1 E	236
	DPA-Dx Insect Venoms 2 (i1, i208, i211, i213, i216, i3, i209, CCD)	Component-resolved differential diagnostics for insect venom allergies	DP 3850-1601-2 E	238

\* Further profiles from page 233

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 239).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g079** at [www.euroimmun.com](http://www.euroimmun.com)



# Molecular allergy diagnostics

DPA-Dx (Defined partial allergen diagnostics) · Insect venoms



For more information on this subject scan the QR code or enter the Quick Link code **q028** at [www.euroimmun.com](http://www.euroimmun.com)

## Insect venoms

■ **Clinical information:** Localised pain, swelling, itching and redness occur as normal reactions to an insect bite. However, insect venoms can also cause allergic reactions which manifest within minutes or not until hours later. The faster the symptoms occur, the more severe the allergic reaction. With further insect bites, the symptoms can continuously worsen.

According to estimations, around 1 to 7% of the population in Central Europe react to insect venoms. In persons who are allergic to insect venoms, severe systemic reactions can occur, which manifest with the formation of urtica, swelling, itching and redness at sites other than the puncture, swelling of the throat and tongue, difficulty in breathing, nausea, gastrointestinal cramps, diarrhoea, neurological deficiencies with confusion, dizziness and gait disorder, as well as raised pulse and fall in blood pressure. In the worst case, the reaction leads to a life-threatening anaphylactic shock.



■ **Diagnostics:** In suspected cases of insect venom allergy, differential diagnostics is recommended for exact identification of the allergy-inducing species. Specific IgE antibodies against bee and wasp venom, as the most common insect venoms, can be detected with the help of multiparameter tests. Besides the previously used natural **insect venom extracts**, recombinant **species-specific allergy components** (defined partial allergen diagnostics, DPA-Dx) are also available for a refined serological diagnosis. Using the EUROLINE DPA-Dx Insect Venoms 2, antibodies against the natural insect venom extracts and against specific molecular antigens for bee and wasp venom (rApi m1, rApi m2, rApi m10, rVes v1 and rVes v5), as well as against CCD (cross-reactive carbohydrate determinant) as a marker for cross-reactivity between the insect venoms can be determined simultaneously in one process. The detection of a primary sensitisation to bee or wasp venom, or of a genuine double sensitisation with comparison to a cross-reaction is made with this test.

In addition, the total IgE concentration in the serum can be determined using the Total IgE ELISA.






## Product overview

Method	Substrate	Application	Order number	Page
EUROLINE*	Insect Venoms (i1, i3, CCD)	Extract-based differentiation of bee and wasp venom allergies	DP 3720-1601 E	237
	DPA-Dx Insect Venoms 2 (i1, i208, i211, i213, i216, i3, i209, CCD)	Component-resolved differential diagnostics for insect venom allergies	DP 3850-1601-2 E	238
ELISA	Total IgE	ELISA for quantitative determination of human IgE in serum	EV 3840-9601 E	146

\* Further profiles from page 233

In addition to EUROIMMUN products, you will also find innovative test systems from Immunodiagnostic Systems  for this indication in the following product lists (page 239).



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q075** at [www.euroimmun.com](http://www.euroimmun.com)



# Products for allergy diagnostics



### Format

- 0501: 5 slides to be incubated with 1 patient serum each
- 0502: 5 slides to be incubated with 2 patient sera each
- 1001: 10 slides to be incubated with 1 patient serum each
- 1601: 16 single test strips



### Product classification

- DE: Test system EUROASSAY (allergy diagnostics) ..... page 232
- DP: Test system EUROLINE (allergy diagnostics) ..... page 233
- Test system chemiluminescence test (allergy diagnostics) ..... page 239
- Control set chemiluminescence test (allergy diagnostics) ..... page 241

For product orders the amount, product code and test name are required. **Test kits** comprise all reagents needed to perform the serological investigation.

Test systems which do not appear in this catalogue can be made to specification. Apart from the customary package sizes and slide formats, special sizes are available as well. Quotations can be provided upon request.



## EUROASSAY for Allergy Diagnostics (Test Systems)

Order No.	Antibodies against	Ig Class	Substrate	Format
DE 3110-1001 E	inhalation (g1, g3, g6, g12, t2, t3, t4, t7, w1, w8, w6, w9, d1, d2, es4, e2, e3, e6, e1, e82, e84, m1, m2, m3, m6, CCD)	IgE	EUROASSAY strip with allergens	10 x 01
DE 3110-1001-2 E	inhalation 2 (t3, t4, t15, t2, gx2, g12, d1, w6, w1, d2, e1, e2, m6, m2, t7, t11, t23, g6, i6, d70, w21, w9, d71, e3, u85, d72, m3, m1, CCD)	IgE	EUROASSAY strip with allergens	10 x 01
DE 3210-0501-1 E	DPA-Dx pollen 1 (t3, g6, t215, t216, t220, t225, g205, g215, g210, g212, CCD)	IgE	EUROASSAY strip with allergens	05 x 01
DE 3410-1001 E	food (f1, f75, f2, f78, f45, f4, f5, f9, f14, f10, f13, f17, f20, f84, f95, f237, f25, f31, f35, f85, f3, f23, f49, CCD)	IgE	EUROASSAY strip with allergens	10 x 01
DE 3410-1001-2 E	food 2 (f47, f26, f75, f90, f10, f78, f89, u87, f35, f95, f329, f84, f24, f20, f1, f13, f5, f2, f14, f4, f25, f85, f31, f33, f92, f49, f17, f3, CCD)	IgE	EUROASSAY strip with allergens	10 x 01
DE 3712-1001 E	pediatrics/atopy (g6, g12, t3, w6, d1, d2, e1, e2, e3, m2, m3, m6, f1, f75, f3, f2, f76, f77, f78, e204, f4, f9, f14, f13, f17, f31, f35, f49, CCD)	IgE	EUROASSAY strip with allergens	10 x 01
DE 3712-1001-2 E	pediatrics/atopy 2 (t3, t4, t15, t2, gx2, g12, d1, w6, w1, d2, e1, e2, m6, m2, f1, f13, f5, f2, f14, f4, f25, f85, f31, f33, f92, f49, f17, f3, CCD)	IgE	EUROASSAY strip with allergens	10 x 01
DE 3812-1001-1 E	DPA-Dx pediatrics 1 (t215, f76, f77, f78, f334, e204, f232, f233, f323, f356, f422, f423, f424, f427, CCD)	IgE	EUROASSAY strip with allergens	10 x 01
DE 3850-0501-3 E	DPA-Dx insect venoms 3 (i1, i3, i75, i208, i213, i216, i209, i211, CCD)	IgE	EUROASSAY strip with allergens	05 x 01

Allergy diagnostics





EUROLINE for Allergy Diagnostics (Test Systems)				
Order No.	Antibodies against	Ig Class	Substrate	Format
DP 3110-1601 E DP 3110-6401 E DP 3110-1601 SE DP 3110-6401 SE	inhalation (g1, g3, g6, g12, t2, t3, t4, t7, w1, w6, w9, d1, d2, e1, e2, e3, m1, m2, m3, m6, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01 64 x 01 16 x 01 64 x 01
DP 3110-1601-1 E	inhalation 2 (g6, g12, t2, t3, t4, w6, w9, d1, d2, e1, e2, e3, e6, e82, e84, es4, m1, m2, m3, m6, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3110-1601-3 E	inhalation 3 (t3, t4, t7, t9, t11, t15, t23, g2, g3, g6, g8, g12, g101, u85, w1, w6, w9, w21, e1, e5, e3, e82, m3, m5, m6, i6, d1, d2, d70, d201, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3111-1601 E	pediatric inhalation (g6, g12, t2, t3, t4, w6, w8, w9, d1, d2, e1, e2, e3, e6, e82, e84, m1, m2, m3, m6, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3112-1601 E	Mediterranean inhalation (g2, g6, t3, t4, t9, t11, t23, t210, w1, w6, w9, w19, d1, d2, d70, e1, e2, e3, m2, m6, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3112-1601-2 E	Mediterranean inhalation 2 (d1, d2, d70, d71, d201, e1, e2, e3, m2, m3, m6, i6, g2, g3, g5, g6, g8, g12, t2, t3, t4, t9, t11, t23, w1, w6, w9, w10, w11, w19, w21, u85, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3113-1601 E	inhalation "South East Asia" (ts19, t19, t223, u85, gs1, ds1, i6, u134, e1, e2, es172, e6, e71, e82, e84, ms1, ms4, m5, m12, m45, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3116-1601-2 E	inhalation "China 2" (ds1, h1, i6, e1, e2, ms1, ts20, u80, w1, w6, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3118-1601 E	inhalation "Gulf" (g6, g12, t2, t3, t7, t9, w1, w6, d1, d2, i6, e1, e2, e3, e17, m1, m2, m3, m5, m6, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3119-1601-11 E	inhalation "Turkey 1" (gs12, gs15, gs21, g12, ts23, ts24, t9, t70, ws18, ws19, ws20, d1, d2, i6, es2, es172, e1, e2, e3, e4, e80, e81, e84, ms11, ms12, m1, m2, m3, m6, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3120-1601 E	inhalation "India" (g6, g12, g20, t18, w4, w27, w29, ds1, d2, i6, e1, e2, e11, e85, m3, m37, u81, u126, u129, u140, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3120-1601-2 E	inhalation "India 2" (g2, g6, g10, g12, g20, t18, t20, w6, w10, w13, w14, w27, w29, ds1, d2, i6, m1, m2, m3, m4, m5, m6, m11, m16, m37, e1, e2, e11, e85, u81, u126, u129, u140, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3122-1601-2 E	inhalation "France 2" (t3, t7, t9, t11, t23, t15, g6, g2, g101, g8, g12, w9, w6, w21, w1, e1, e5, e82, m3, m6, i6, d1, d2, d70, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3123-1601-2 E	inhalation "Lebanon 2" (g6, g2, g12, g101, w7, w19, w21, ws24, t2, t3, t7, t9, t16, t23, ts32, m1, m2, m3, m5, m6, d1, d2, e1, e2, e3, e85, es170, es172, u85, u140, i1, i3, i6, i71, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3124-1601 E	inhalation "Screen South Africa" (ts19, ts29, gs1, ws21, e1, e2, hs12, ms1, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01



## EUROLINE for Allergy Diagnostics (Test Systems)

Order No.	Antibodies against	Ig Class	Substrate	Format
DP 3126-1601 E	inhalation "Mexico" (g2, g5, g6, g10, g14, t3, t7, t19, t210, t20, t14, t15, w1, w4, w6, w8, w10, w11, w14, w15, w100, d1, d2, h1, i6, e1, e2, es4, m1, m2, m3, m6, m20, m5, m11, m14, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3127-1601-1 E	inhalation "Ukraine 1" (d1, d2, e1, e2, e3, e6, e82, e84, t2, t3, t4, t7, g6, g12, w6, w9, m1, m2, m3, m6, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3128-1601 E	inhalation trees (t1, t2, t3, t4, t5, t7, t15, t12, t14, t16, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3129-1601 E	inhalation grass and weeds (g1, g3, g6, g12, w1, w6, w9, w10, w103, w203, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3130-1601 E	inhalation animals (e1, e2, e3, e6, e71, e73, e82, e84, es7, es172, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3131-1601 E	inhalation indoor allergens (ds1, es2, i6, e7, m1, m2, m3, m5, m6, m37, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3132-1601 E	inhalation "Maghreb" (g2, g3, g6, g8, g12, t3, t5, t7, t9, t11, t15, t18, t19, t23, w1, w4, w6, w7, w9, w10, w21, d1, d2, i6, e1, e2, e3, m3, m5, m6, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3133-1601-1 E	inhalation "Iran 1" (e1, e2, e3, e4, e81, es2, es172, g1, g3, g12, g14, g16, w6, w9, w10, w11, w14, w17, w28, w100, t1, t15, t16, t70, ts22, ts26, i1, i6, h1, d1, d2, m1, m2, m3, m6, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3135-1601-1 E	inhalation "Venezuela 1" (g2, g5, g10, w6, w8, w9, w14, e1, e2, e78, e85, e86, e111, u85, m1, m2, m3, m5, m6, d1, d2, d201, i1, i2, i3, i4, i70, i71, i100, p1, p2, p4, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3138-1601-1 E	inhalation "Iraq 1" (e1, e2, e3, e4, e81, es2, es172, g1, g3, g12, g14, g16, w6, w9, w10, w11, w14, w17, w28, w100, t1, t15, t16, t70, ts22, ts26, i1, i6, h1, d1, d2, m1, m2, m3, m6, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3139-1601-1 E	inhalation "Central Africa 1" (d1, d2, d70, d201, e1, e2, e7, e80, m1, m2, m3, m5, m6, i6, u85, u140, g2, g6, w1, t102, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3210-1601-1 E	DPA-Dx pollen 1 (t3, g6, t215, t216, t220, t225, g205, g215, g210, g212, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3211-1601-1 E	DPA-Dx pollen "Southern Europe 1" (t3, t9, t23, g6, w21, m6, t215, t226, w211, g205, g215, g210, g212, t224, t231, t235, m229, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3410-1601 E DP 3410-6401 E DP 3410-1601 SE DP 3410-6401 SE	food (f1, f75, f2, f45, f4, f5, f9, f13, f14, f17, f20, f49, f84, f237, f25, f31, f35, f85, f3, f23, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01 64 x 01 16 x 01 64 x 01
DP 3410-1601-1 E	food 2 (f1, f75, f2, f78, f4, f5, f14, f10, f13, f17, f20, f49, f84, f95, f25, f31, f35, f85, f3, f23, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01





## EUROLINE for Allergy Diagnostics (Test Systems)

Order No.	Antibodies against	Ig Class	Substrate	Format
DP 3410-1601-3 E	food 3 (f13, f17, f20, f158, f12, f14, f89, f96, f25, f47, f48, f85, f49, f84, f92, f95, f26, f27, f83, f3, f23, f24, f40, f4, f8, f9, f10, f45, f2, f78, f218, f1, f75, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3411-1601 E	food "South East Asia 1" (f1, f75, f2, f4, f9, f10, f14, f13, f17, f63, f64, f83, fs10, fs14, f23, f24, f80, f234, f105, f336, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3414-1601-2 E	food "China 2" (f1, f2, f13, f14, f23, f24, fs33, fs34, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3415-1601-2 E	food "Middle East 2" (f2, f169, f245, f233, f13, f17, f20, f144, f253, f256, f10, f361, f36, f9, f4, f292, fs82, fs83, fs43, f83, f12, f14, f132, f159, fx20, f33, f49, f92, f97, f237, fs48, f50, f72, f93, f96, f191, f329, f25, f35, f38, f47, f244, f262, fx15, fs77, fs78, f273, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3416-1601 E	food "Gulf" (f1, f75, f2, f105, f4, f14, f45, fs36, f13, f92, f33, f44, f93, f25, f31, f48, f83, f88, f3, f23, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3420-1601-11 E	food "Turkey 1" (f1, f75, f2, f169, f78, f4, f79, f9, f14, f10, f13, f17, f144, u87, f222, f73, f33, f44, f49, f92, f84, f146, f328, f25, f31, f35, f48, f95, f97, f122, f132, fs14, fs10, fs43, f83, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3421-1601 E	food "India" (f2, f75, f168, f4, f9, f14, f13, f36, f49, f50, f35, f38, f48, f244, f83, f89, f74, f240, f23, f24, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3421-1601-2 E	food "India 2" (f1, f75, f2, f168, f360, f4, f79, f7, f9, f14, f13, f33, f36, f49, f50, f12, f25, f35, f38, f47, f48, f159, f212, f244, f262, f370, f364, f367, f27, f83, f88, f89, f74, f105, f240, fs81, f3, f23, f24, f371, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3422-1601-2 E	food "France 2" (f20, f17, f25, f12, f13, f14, f85, f92, f96, f49, f84, f89, f27, f26, f24, f23, f40, f3, f45, f10, f4, f2, f75, f1, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3423-1601-3 E	food "Lebanon 3" (f23, f24, f40, f41, fs79, f45, f1, f2, f76, f77, f78, f334, e204, f4, f9, f10, f12, f13, f14, f20, fs39, f44, f49, f84, f95, fs80, f25, f31, f35, f47, f48, f86, f96, f159, f292, f273, fs78, f27, f83, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3424-1601 E	food "Screen South Africa" (f1, f2, f4, f13, f14, fs36, f3, fs12, fs58, fs53, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3425-1601 E	food "Mexico" (f1, f75, f2, f78, f95, f96, f44, fs32, f4, f7, f9, f45, f13, f14, f20, fs35, f12, f15, f49, f292, f25, f31, f35, f92, f216, f191, f263, f105, f284, f83, f26, f27, fs27, f24, f40, fs12, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3426-1601-2 E	food "Ukraine 2" (f4, f6, f9, f11, f13, f361, f45, f47, f73, f81, fs32, f25, f35, f26, f27, f83, f3, f40, f41, f206, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3427-1601 E	food dairy products and nuts (f1, f2, f75, f78, f13, f256, f17, f20, f73, f336, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3428-1601 E	food flour and meat (f4, f5, f7, f9, f26, f27, f83, f79, f3, f24, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3429-1601 E	food vegetables (f10, f14, f86, f25, f31, f35, f85, f46, f244, f292, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01



## EUROLINE for Allergy Diagnostics (Test Systems)

Order No.	Antibodies against	Ig Class	Substrate	Format
DP 3430-1601 E	food fruits (f44, f49, f84, f92, f95, f97, f122, f237, f329, fs32, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3431-1601 E	food "Maghreb" (f1, f75, f2, f78, f4, f9, f10, f12, f13, f14, f17, f20, f33, f44, f49, f92, f25, f35, f47, f48, f85, f45, f73, f27, f83, f3, f40, f41, f23, f24, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3432-1601-1 E	food "Iran 1" (f1, f75, f2, f78, f4, f5, f9, fs13, f10, f13, f14, f17, f20, f144, f256, f79, f44, f49, f50, f84, f92, f93, f95, f97, f87, fs32, f25, f35, f46, f47, f85, f262, f83, fs28, f24, fs12, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3433-1601-1 E	food "Venezuela 1" (f1, f232, f233, f75, f2, f76, f77, f78, f105, f4, f5, f6, f7, f9, f14, f292, f79, f13, f17, f20, f256, f3, f24, f37, f40, f41, f308, f155, f45, f25, f31, f35, f32, f33, f44, f49, f72, f92, f26, f27, f83, f81, f205, f218, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3436-1601-1 E	food "Iraq 1" (f1, f75, f2, f78, f4, f5, f9, fs13, f10, f13, f14, f17, f20, f144, f256, f79, f44, f49, f50, f84, f92, f93, f95, f97, f87, fs32, f25, f35, f46, f47, f85, f262, f83, fs28, f24, fs12, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3439-1601-1 E	food "Central Africa 1" (f2, fs84, f245, f45, f83, fs43, f3, fs85, f4, f10, f13, fs86, f14, f235, fs87, f25, f35, f262, fs912, fs88, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3510-1601-1 E DP 3510-1601-1 SE	DPA-Dx milk 1 (f2, f76, f77, f78, f334, e204, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01 16 x 01
DP 3511-1601-1 E	DPA-Dx peanuts 1 (t215, f422, f423, f424, f429, f445, f444, f427, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3702-1601-1 E	atopy "Chile 1" (d1, d2, e1, e2, es2, g2, g4, g5, m2, m3, m6, t11, t14, t15, t19, w9, w100, f1, f75, f78, f2, f40, f41, fs12, f4, f9, f13, f14, f25, f33, f49, f92, f83, f96, f105, f292, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3702-1601-2 E	atopy "Chile 2" (d1, d2, e1, e2, es2, gs2, m5, i6, t1, t7, t11, t14, t19, ts30, ws23, f1, f2, f4, f6, f7, f13, f17, f36, f256, f14, f74, f105, f292, f26, f27, f83, f88, f3, f40, f41, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3703-1601-1 E	atopy "Ukraine 1" (d1, d2, e1, e2, IgE, h1, is6, m6, g6, g12, ts3, t7, w1, w6, f1, f2, f14, f95, f23, fs59, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3703-1601-2 E	atopy "Ukraine 2" (d1, d2, e1, e2, e3, g6, t3, w6, m2, m3, f1, f75, f2, f3, f4, f13, f14, f31, f35, f49, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3704-1601-1 E	atopy "Venezuela 1" (f1, f75, f3, f24, f40, f308, f4, f5, f6, f7, f9, f14, f292, f79, f13, f17, f20, f2, f76, f77, f78, f105, f218, f25, f32, f33, f44, f49, f72, f26, f27, f83, f155, f45, u85, d1, d2, d201, e1, e2, e85, m1, m2, m3, m5, m6, g2, w8, i1, i3, i70, i71, i100, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3706-1601-1 E	atopy "Caribbean 1" (g6, g12, t3, t20, w6, e1, e2, e3, d1, m2, m6, f1, f2, f79, f4, f9, f14, f13, f31, f35, f292, f49, f362, f64, f3, f24, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3707-1601-1 E	atopy "Indonesia 1" (g2, g6, gs1, t19, t223, u85, d1, d2, d4, d72, d73, d201, e1, e2, e3, e204, es2, u134, i1, i6, m5, ms1, f4, f79, f13, f14, f17, f20, f45, f336, f1, f2, f76, f77, f78, fs10, f3, f40, f41, f23, f24, f80, f157, f63, f64, f83, f88, f81, f25, f47, f44, f84, f74, f105, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01



## EUROLINE for Allergy Diagnostics (Test Systems)

Order No.	Antibodies against	Ig Class	Substrate	Format
DP 3709-1601-1 E	atopy "Thailand 1" (g2, g6, g10, e1, e2, e84, d1, d2, i6, i100, m2, m3, m6, u85, f1, f75, f2, f3, f23, f24, f41, f177, f234, f258, f232, f233, f76, f77, f78, f4, f79, f13, f423, f427, f14, f36, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3709-1601-2 E	atopy "Thailand 2" (d1, d2, e1, e2, e71, e82, e84, e85, e86, u81, u85, g2, g6, g10, t18, t19, i6, i100, m1, m2, m3, m6, f1, f75, f2, f4, f10, f13, f14, f20, f158, f31, f35, f45, f336, f23, f24, f234, f40, f41, f3, f436, f324, f37, f258, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3710-1601 E	atopy (g6, g12, t3, w6, d1, e1, e2, e3, m2, m6, f1, f2, f3, f4, f9, f14, f17, f31, f35, f49, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3710-1601-4 E	atopy 4 (f13, f17, f12, f14, f4, f85, f96, f26, f3, f24, f1, f2, f49, f84, f95, t3, t7, t9, t11, t15, t23, g6, w1, w6, w9, w21, e1, e5, m3, m6, d1, d2, i6, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3710-1601-13 E	Atopy: 13 (d1, d2, d4, t2, t3, t4, t15, gs2, w6, w9, e1, e2, e3, m1, m2, m3, m6, f13, f17, f20, f144, f158, f256, f4, f5, f11, f99, f10, f14, f1, f75, f2, f76, f77, f78, f3, f84, f49, f25, w1, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3712-1601 E DP 3712-6401 E DP 3712-1601 SE DP 3712-6401 SE	pediatrics (gx, t3, w6, d1, d2, e1, e2, e3, m2, m3, m6, f1, f75, f2, f3, f76, f77, f78, e204, f4, f9, f14, f13, f17, f31, f35, f49, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01 64 x 01 16 x 01 64 x 01
DP 3713-1601 E DP 3713-6401 E	atopy "China" (ts20, w1, w6, ds1, h1, e1, e2, i6, ms1, u80, f1, f2, f13, f14, f27, f88, fs33, f24, f23, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01 64 x 01
DP 3713-1601-5 E	atopy "China 5" (ds1, h1, i6, e1, e2, ms1, w1, w6, f1, f2, f13, f14, f23, f24, fs33, u80, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3713-1601-7 E	atopy "China 7" (ds1, h1, i6, e1, e2, ms1, w1, w6, f1, f2, fs33, u80, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3715-1601-3 E	atopy "South East Asia 3" (ts20, w1, w6, ds1, h1, e1, e2, i6, ms1, u80, f1, f2, f13, f14, f27, f88, fs33, fs34, f24, f23, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3716-1601 E	atopy "Peru" (e1, e2, e3, e7, e11, e82, e84, es172, i1, i3, i6, m1, m2, m3, m6, t18, u85, w29, w28, d1, d2, f75, f79, f1, f2, f23, f206, f13, f14, f104, f105, f26, fs32, f44, f49, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3717-1601-2 E	"Mix France 2" (f85, f14, f13, f12, f4, f24, f3, f2, f1, f17, f49, f84, t3, t7, t9, t15, t23, g6, w9, w6, w21, w1, e1, e5, m3, m6, d1, d2, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3718-1601 E DP 3718-1601 SE	atopy "Lithuania" (w6, w9, w103, w203, t3, t4, t11, g6, gs21, e1, e2, e3, e4, e82, es2, ds1, ms1, m5, f73, f245, f2, f81, f13, f14, f17, f256, f4, f12, f15, f44, fs32, f26, f27, f83, f49, f3, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01 16 x 01
DP 3720-1601 E	insect venoms (i1, i3, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01



## EUROLINE for Allergy Diagnostics (Test Systems)

Order No.	Antibodies against	Ig Class	Substrate	Format
DP 3790-1601 E	<b>atopy screen</b> (d1, d2, i1, i3, i6, h1, e1, e2, e3, m1, m2, m3, m6, g1, g3, g6, g12, t2, t3, t4, t7, t23, w1, w6, w9, u85, f25, f31, f35, f85, f1, f75, f2, f3, f23, f24, e204, f76, f77, f78, f27, f88, f45, f4, f5, f9, f14, f10, f13, f17, f20, f49, f84, f237, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3812-1601-1 E	<b>DPA-Dx pediatrics 1</b> (t215, f76, f77, f78, f334, e204, f232, f233, f323, f356, f422, f423, f424, f427, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3812-1601-2 E	<b>DPA-Dx pediatrics 2</b> (f76, f77, f78, f334, e204, f232, f233, f323, f356, f422, f423, f424, f429, f445, f444, f427, t215, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3850-1601-2 E	<b>DPA-Dx insect venoms 2</b> (i1, i208, i213, i216, i3, i209, i211, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3850-1601-3 E	<b>DPA-Dx insect venoms 3</b> (i1, i3, i75, i208, i213, i216, i209, i211, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01
DP 3851-1601-1 E	<b>DPA-Dx insect venoms "Southern Europe 1"</b> (i1, i3, i75, i77, i208, i213, i216, i210, i209, i220, i211, CCD)	IgE	membrane strip with allergens (EUROLINE)	16 x 01



## IDS Chemiluminescence Test for Allergy Diagnostics (Test Systems)

IDS Order No.	Description	Format
IS-1TIGE900	IDS Total / Specific IgE Reagent Kit	50 / 200 determinations
IS-1D001	IDS Specific IgE (D001) House dust mite	50 determinations
IS-1D002	IDS Specific IgE (D002) House dust mite	50 determinations
IS-1D202	IDS Specific IgE (D202) rDer p 1	20 determinations
IS-1D203	IDS Specific IgE (D203) rDer p 2	20 determinations
IS-1D205	IDS Specific IgE (D205) rDer p 10	20 determinations
IS-1E001	IDS Specific IgE (E001) Cat dander	50 determinations
IS-1E003	IDS Specific IgE (E003) Horse dander	50 determinations
IS-1E005	IDS Specific IgE (E005) Dog dander	50 determinations
IS-1E094	IDS Specific IgE (E094) nFel d 1	20 determinations
IS-1E101	IDS Specific IgE (E101) nCan f 1	20 determinations
IS-1F001	IDS Specific IgE (F001) Egg white	50 determinations
IS-1F002	IDS Specific IgE (F002) Cow's Milk	50 determinations
IS-1F003	IDS Specific IgE (F003) Fish (cod)	50 determinations
IS-1F013	IDS Specific IgE (F013) Peanut	50 determinations
IS-1F014	IDS Specific IgE (F014) Soybean	50 determinations
IS-1F017	IDS Specific IgE (F017) Hazelnut	50 determinations
IS-1F020	IDS Specific IgE (F020) Almond	50 determinations
IS-1F037	IDS Specific IgE (F037) Mussel	50 determinations
IS-1F075	IDS Specific IgE (F075) Egg yolk	50 determinations
IS-1F076	IDS Specific IgE (F076) Alpha-lactalbumin	50 determinations
IS-1F077	IDS Specific IgE (F077) Beta-lactoglobulin	50 determinations
IS-1F078	IDS Specific IgE (F078) Casein	50 determinations
IS-1F084	IDS Specific IgE (F084) Kiwi	50 determinations
IS-1F202	IDS Specific IgE (F202) Cashew nut	50 determinations
IS-1F203	IDS Specific IgE (F203) Pistachio	50 determinations
IS-1F233	IDS Specific IgE (F233) nGal d 1	20 determinations
IS-1F245	IDS Specific IgE (F245) Hen's Egg	50 determinations
IS-1F256	IDS Specific IgE (F256) Walnut	50 determinations
IS-1F351	IDS Specific IgE (F351) rPen a 1	20 determinations
IS-1F423	IDS Specific IgE (F423) rAra h 2	20 determinations
IS-1F427	IDS Specific IgE (F427) rAra h 9	20 determinations
IS-1F428	IDS Specific IgE (F428) rCor a 1	20 determinations
IS-1F434	IDS Specific IgE (F434) rMal d 1	20 determinations



## IDS Chemiluminescence Test for Allergy Diagnostics (Test Systems)

IDS Order No.	Description	Format
IS-1G001	IDS Specific IgE (G001) Sweet vernal grass	50 determinations
IS-1G002	IDS Specific IgE (G002) Bermuda grass	50 determinations
IS-1G003	IDS Specific IgE (G003) Cocksfoot	50 determinations
IS-1G004	IDS Specific IgE (G004) Meadow fescue	50 determinations
IS-1G005	IDS Specific IgE (G005) Rye-grass	50 determinations
IS-1G006	IDS Specific IgE (G006) Timothy grass	50 determinations
IS-1G007	IDS Specific IgE (G007) Common reed	50 determinations
IS-1G008	IDS Specific IgE (G008) Meadow grass	50 determinations
IS-1G012	IDS Specific IgE (G012) Cultivated rye	50 determinations
IS-1G013	IDS Specific IgE (G013) Velvet grass	50 determinations
IS-1G014	IDS Specific IgE (G014) Cultivated oat	50 determinations
IS-1G015	IDS Specific IgE (G015) Cultivated wheat	50 determinations
IS-1G201	IDS Specific IgE (G201) Barley	50 determinations
IS-1G205	IDS Specific IgE (G205) rPhl p 1	20 determinations
IS-1G213	IDS Specific IgE (G213) rPhl p 1, rPhl p 5b	20 determinations
IS-1G215	IDS Specific IgE (G215) rPhl p 5b	20 determinations
IS-1GX03	IDS Specific IgE (GX03) Grass mix 3	50 determinations
IS-1I001	IDS Specific IgE (I001) Honey bee	50 determinations
IS-1I003	IDS Specific IgE (I003) Wasp	50 determinations
IS-1K082	IDS Specific IgE (K082) Latex	50 determinations
IS-1M003	IDS Specific IgE (M003) Aspergillus fumigatus	50 determinations
IS-1M006	IDS Specific IgE (M006) Alternaria alternata	50 determinations
IS-1M229	IDS Specific IgE (M229) rAlt a 1	20 determinations
IS-1T002	IDS Specific IgE (T002) Alder	50 determinations
IS-1T003	IDS Specific IgE (T003) Common silver birch	50 determinations
IS-1T004	IDS Specific IgE (T004) Hazel	50 determinations
IS-1T009	IDS Specific IgE (T009) Olive	50 determinations
IS-1T025	IDS Specific IgE (T025) European ash	50 determinations
IS-1T215	IDS Specific IgE (T215) rBet v 1	20 determinations
IS-1T216	IDS Specific IgE (T216) rBet v 2	20 determinations
IS-1T224	IDS Specific IgE (T224) rOle e 1	20 determinations
IS-1W001	IDS Specific IgE (W001) Common ragweed	50 determinations
IS-1W006	IDS Specific IgE (W006) Mugwort	50 determinations








IDS Chemiluminescence Test for Allergy Diagnostics (Test Systems)			ids <sup>®</sup>
IDS Order No.	Description	Format	
IS-1W009	IDS Specific IgE (W009) Plantain	50 determinations	
IS-1W230	IDS Specific IgE (W230) nAmb a 1	20 determinations	
IS-1W231	IDS Specific IgE (W231) nArt v 1	20 determinations	

IDS Control Sets for Chemiluminescence Tests			ids <sup>®</sup>
IDS Order No.	Description	Format	
IS-1F003-30	IDS Positive Specific IgE Control (F003) Cod	1 concentration	
IS-1G006-30	IDS Positive Specific IgE Control (G006) Timothy Grass	1 concentration	
IS-1SIGE930	IDS Negative Specific IgE Control (F003/G006) Cod/Timothy Grass	1 concentration	
IS-1TIGE930	IDS Total IgE Control Set	3 concentrations	



# Antigen detection





# Neurodegenerative diseases

Beta-amyloid, tau protein · Neurofilaments




For more information on this subject scan the QR code or enter the Quick Link code **q032** at [www.euroimmun.com](http://www.euroimmun.com)

## Beta-amyloid, tau proteins

■ **Clinical information:** Alzheimer's disease, which was first described in 1906, is with 60 to 70% the most common cause of dementia in old age. The prevalence doubles for around every five years of age – 30% of persons over 90 suffer from this disease. In contrast to the age-dependent, sporadic form of Alzheimer's, the familial, genetically caused form can also occur in young adults from 30 years of age. The disease is divided into three consecutive phases: the preclinical stage, the MCI (mild cognitive impairment) stage and the dementia stage. In Alzheimer's disease neurofibrillary tangles accumulate in the nerve cells (in particular in the cortical and limbic brain regions). Outside of the nerve cells, deposits of beta-amyloid ( $A\beta$ ) in the form of so-called **neuritic plaques** are observed. These contain predominantly the peptides beta-amyloid 1-40 ( $A\beta$ 1-40) and beta-amyloid 1-42 ( $A\beta$ 1-42). The intracellular **neurofibrillary tangles** consist of hyperphosphorylated tau proteins.

■ **Diagnostics:** Definitive diagnosis of Alzheimer's disease can only be established by brain autopsy to detect the neuropathological changes (plaques and neurofibrillary tangles). In vivo diagnosis (probable Alzheimer's disease) is based primarily on clinical identification of dementia syndrome and exclusion of possible reversible causes (e.g. endocrinopathies, vitamin deficiency diseases, chronic infections, etc.).

Clinical diagnosis is unreliable, particularly in the early disease stages, and requires additional measurable biomarkers with high diagnostic reliability. The concentrations of soluble  $A\beta$ 1-42 and phosphorylated tau protein (pTau(181)) in the **cerebrospinal fluid (CSF)** reflect the Alzheimer's-specific neuropathological changes in the brain. The CSF of persons who will later develop Alzheimer's disease exhibits a significant **decrease in the  $A\beta$ 1-42 concentration** already 5 to 10 years before the start of cognitive changes. In contrast, the **concentrations of total tau and pTau(181)** in the CSF **increase** when patients show advanced neurodegeneration and cognitive impairment. Thus, discrimination from healthy persons is possible. The **ratio  $A\beta$ 1-42/ $A\beta$ 1-40** in CSF can, in addition, contribute to the differentiation of Alzheimer's disease from vascular dementia (see figure).



Imaging techniques such as MRT, SPECT, or PET (amyloid detection) can also be used to support early and differential diagnostics. Results from CSF-based neurochemical analyses and results from imaging procedures should only be assessed in the context of all available diagnostic information.



## Product overview

Method	Analyte	Sample material	Application	Order number	Page
ELISA	Beta-amyloid (1-40)	CSF	Quantitative detection of beta-amyloid (1-40)	EQ 6511-9601-L	260
	Beta-amyloid (1-40)*	Plasma		EQ 6511-9601	260
	Beta-amyloid (1-42)	CSF	Quantitative detection of beta-amyloid (1-42)	EQ 6521-9601-L	260
	Beta-amyloid (1-42)*	Plasma		EQ 6521-9601	260
	Total tau	CSF	Quantitative detection of total tau protein	EQ 6531-9601-L	260
	Phospho tau	CSF	Specific detection of threonine 181 phosphorylated tau protein (pTau(181))	EQ 6591-9601-L	261
	BACE-1*	CSF	Quantitative detection of BACE-1	EQ 6541-9601-L	261
	Neurogranin*	CSF	Quantitative detection of truncated neurogranin P75	EQ 6551-9601-L	261
	Alpha-synuclein*	CSF	Quantitative detection of alpha-synuclein	EQ 6545-9601-L	261
ChLIA	Beta-amyloid (1-40)	CSF	Quantitative detection of beta-amyloid (1-40)	LQ 6511-10100-L (control set: LR 6511-20210-L)	263
	Beta-amyloid (1-42)	CSF	Quantitative detection of beta-amyloid (1-42)	LQ 6521-10100-L (control set: LR 6521-20210-L)	263
	Total tau	CSF	Quantitative detection of total-tau protein	LQ 6531-10100-L (control set: LR 6531-20210-L)	263
	Phospho tau	CSF	Quantitative detection of threonine 181 phosphorylated tau protein (pTau(181))	LQ 6591-10100-L (control set: LR 6591-20210-L)	263

\* For research use only, not for in vitro diagnostic use in the sense of EU directive 98/79/EC.



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q083** at [www.euroimmun.com](http://www.euroimmun.com)



# Neurodegenerative diseases

Beta-amyloid, tau protein · Neurofilaments



For more information on this subject scan the QR code or enter the Quick Link code **q160** at [www.euroimmun.com](http://www.euroimmun.com)

## Neurofilaments

■ **Clinical information:** Neurofilaments (Nf) are intermediary filaments consisting of the neurofilament light chain (Nf-L), medium chain (Nf-M) and heavy chain (pNf-H). Nf-M and pNf-H, in particular, are subject to considerable posttranslational modifications (phosphorylation, O-glycosylation). Neurofilaments are expressed exclusively in neurons. As the most important structural elements, they are involved, among other things, in axonal transport.

■ **Diagnostics:** Neurofilaments are released in case of neuroaxonal damage, which leads to an increase in the concentration of Nf-subunits in the CSF and blood. CSF and blood Nf levels correlate with each other. However, measurement in the CSF is diagnostically more conclusive since the CSF concentration is 10 times higher than that in blood. In rapidly progressing neurodegenerative diseases, such as amyotrophic lateral sclerosis (ALS) or Creutzfeldt-Jakob disease (CJD), the Nf levels are approximately ten times higher than those in healthy individuals.

The concentration of Nf in the CSF and blood of ALS patients is already significantly increased at an early, pre-diagnostic stage of the disease. The Nf level correlates with the degree of degeneration of the motor neurons. Furthermore, Nf is a prognostic biomarker for the life expectancy of ALS patients. While high concentrations are associated with an unfavourable and rapid disease course, patients who live longer generally exhibit lower Nf values. In studies comparing Nf-L and pNf-H in ALS diagnosis, a higher sensitivity and specificity were observed for pNf-H.





## Product overview

Method	Analyte	Sample material	Application	Order number	Page
ELISA	Neurofilament (pNf-H)	CSF and serum	Quantitative detection of phosphorylated neurofilament heavy chain (pNf-H)	EQ 6561-9601	261
	Neurofilament (pNf-H) highly sensitive	Serum and plasma		EQ 6562-9601	261



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g083** at [www.euroimmun.com](http://www.euroimmun.com)



# Kidney markers

 Uromodulin · Soluble CD163 (sCD163)



For more information on this subject scan the QR code or enter the Quick Link code **q125** at [www.euroimmun.com](http://www.euroimmun.com)

## Uromodulin

■ **Clinical information:** In the human body, uromodulin is exclusively produced in the kidneys by the tubule cells of the thick ascending limb of Henle's loop and secreted both into the lumen of the tubule and the blood stream. In the distal tubule lumen, uromodulin is present polymerised to the epithelium, offering protection against kidney stone formation. Due to its polymer structure, the uromodulin which is secreted via the urine is only to a small extent suitable for measurement. Uromodulin in serum, on the other hand, is exclusively present as a monomer and therefore can be more reliably quantified.

Moreover, uromodulin concentrations in urine only have a weak association with the estimated glomerular filtration rate (eGFR). In contrast, the uromodulin in serum (sUmod) correlates strongly with the eGFR.

The sUmod concentration allows identification of early stages of chronic kidney insufficiency already in the symptom-free phase as opposed to established glomerular markers, such as creatinine and cystatin C. A decrease of sUmod concentration in progressing kidney insufficiency shows a loss in function and integrity of the kidney parenchyma.

Based on the sUmod level, also long-term complications can be deduced. Epidemiological studies show that low sUmod concentrations are associated with an increased overall mortality, cardiovascular morbidity, heart insufficiency and the progression of kidney insufficiency. With respect to transplantations, low sUmod concentrations are predicative for long-term function loss of the transplant.

■ **Diagnostics:** Serum uromodulin presents a sensitive marker of tubular function with a large potential for the prediction and early recognition of decreasing kidney function. This applies especially to diseases in which mainly the kidney tubules are damaged.



## Product details

Analyte	Sample material	Application	Order number	Page
Uromodulin	Serum/plasma	Sensitive marker for a loss in kidney function	EQ 6821-9601	261



# Kidney markers

Uromodulin · Soluble CD163 (sCD163)



For more information on this subject scan the QR code or enter the Quick Link code **q162** at [www.euroimmun.com](http://www.euroimmun.com)

## Soluble CD163 (sCD163)

■ **Clinical information:** CD163 is a membrane protein that is produced exclusively on the cells of the immune system, i.e. monocytes and macrophages. If these come into contact with inflammation-promoting stimuli, for instance, bacterial molecules, CD163 is enzymatically cleaved off of the immune cell membrane, which results in the formation of soluble CD163 (sCD163). In glomerulonephritis, macrophages migrate into the tissue and release sCD163 into the urine via the Bowman's capsule. The biomarker can then be measured in the urine.

The more serious the inflammation, the more macrophages migrate into the tissue. This means that the concentration of sCD163 in urine directly provides information about the severity of the glomerulonephritis. The sCD163 level correlates with the disease activity. The higher its concentration, the more severe the inflammation.

■ **Diagnostics:** The sCD163 ELISA is particularly suited for monitoring patients with diagnosed AAV with renal involvement. Contrary to systemic inflammation markers, the sCD163 level is a specific indicator of renal inflammation and reacts quickly under treatment or in case of fluctuations in the inflammatory activity.

If, during regular testing, the sCD163 concentrations increase again after having been normal for some time, this can point to a renewed outbreak of the kidney inflammation. The treatment can then be adjusted at an early stage, preventing irreversible kidney damage in the patient.



## Product details

Analyte	Sample material	Application	Order number	Page
sCD163	Urine	Sensitive marker that reflects the inflammation in the glomeruli (glomerulonephritis) depending on the migrated M2 macrophages.	EQ 6851-9601-U	261



# Inflammatory bowel diseases



For more information on this subject scan the QR code or enter the Quick Link code **q127** at [www.euroimmun.com](http://www.euroimmun.com)

## Calprotectin

■ **Clinical information:** Calprotectin is a calcium- and zinc-binding protein which is produced by neutrophil granulocytes and monocytes and has bactericidal and fungicidal properties. In the case of an inflammatory intestinal disease, granulocytes move into the gut lumen where they release calprotectin, which is secreted with stool. The calprotectin concentration in stool shows the extent of an inflammation in the intestine.

■ **Diagnostics:** The non-invasive determination of calprotectin levels in stool is useful for:

Differential diagnostic delimitation of an irritable colon (irritable bowel syndrome) from acute and chronic inflammations of the intestine (e.g. viral or bacterial infections, Crohn's disease, ulcerative colitis). The calprotectin level in stool is increased in chronic inflammatory bowel diseases (CIBD) and malignant intestinal tumors with an inflammatory component, but not in intestinal polyps, benign intestinal tumors, and irritable colon.

Monitoring the disease course and therapy response in patients with CIBD. With successful treatment, the originally increased calprotectin level decreases significantly. In the case of a relapse, it increases again. The level correlates very well with the histological and endoscopic findings. Owing to the non-invasive calprotectin determination, patients can be spared biopsies and other complicated procedures.





## Product details

Method	Analyte	Sample material	Application	Order number	Page
ELISA	Calprotectin	Stool	Ideally suited for differentiation of chronic inflammatory bowel disease and irritable bowel syndrome and for monitoring the disease course	EQ 6831-9601 W	261
ChLIA	Calprotectin	Stool		LQ 6831-10010 W (control set: LR 6831-20210 W)	263
Additional material				Order number	
Stool dosage tubes (SDT), prefilled with extraction buffer, 45 pieces				ZE 6010-4501	
Stool dosage tubes (SDT), not prefilled with extraction buffer, 100 pieces				ZE 6010-0100-1	



# IDS products

Bone turnover markers · calcium metabolism



For more information on this subject scan the QR code or enter the Quick Link code **q076** at [www.euroimmun.com](http://www.euroimmun.com)

## Bone turnover markers

■ **Clinical information:** Bone is a metabolically active organ that undergoes continuous remodelling throughout life. Bone turnover markers are products derived from the bone remodelling process which are released as a result of the action of the cells involved (osteoblasts and osteoclasts). Depending on their involvement in the remodelling process, they are categorised into bone formation or resorption markers.



■ **Diagnostics:** Osteoporosis is the most common bone metabolism disorder. It is characterised by a weakening of the bone structure. According to the recommendation of a consensus group of the International Osteoporosis Foundation (IOF), osteoporosis therapy can be monitored using bone turnover markers. Their targeted determination makes it possible to assess whether the patient is responding to the treatment. A useful approach would be to establish baseline levels before starting therapy and measure serum levels after three months and every 12 months thereafter. Subsequent yearly measurements, preferably at the same time as DXA controls, will help to identify patients developing poor adherence.

Similarly, according to the Canadian Consensus Conference on Osteoporosis, analysis of bone turnover markers can be used to quickly assess adherence and effectiveness of drug therapies. According to the organisation, bone mineral density (BMD) should not be considered the only indicator of treatment success, as therapy is not necessarily associated with a significant increase in BMD.

In addition to osteoporosis, there are many other conditions affecting bone, such as chronic kidney disease (CKD) and other metabolic bone diseases. Utilisation of the bone turnover markers in these cases can be beneficial to support clinicians in the management of patients.



## Product details

Method	Analyte	Sample material	Application	Order number	Page
ELISA	Serum CrossLaps <sup>®</sup> (CTX-I)	Serum/plasma	Detection of C-terminal telopeptides of type I collagen – a marker of bone resorption	AC-02F1	262
	Urine CrossLaps <sup>®</sup> (CTX-I)	Urine		AC-03F1	262
	Alpha CrossLaps <sup>®</sup> (CTX-I)	Urine		AC-04F1	262
	Urine BETA CrossLaps <sup>®</sup> (CTX-I)	Urine		AC-05F1	262
	N-MID <sup>®</sup> Osteocalcin	Serum/plasma	Detection of N-MID osteocalcin – a marker of bone formation	AC-11F1	262
	Ostase <sup>®</sup> (BAP)	Serum	Detection of bone-specific alkaline phosphatase – a marker of bone formation	AC-20F1	262
ChLIA	CrossLaps <sup>®</sup> (CTX-I)	Serum/plasma	Detection of C-terminal telopeptides of type I collagen – a marker of bone resorption	IS-3000 IS-3030 (control set)	264 265
	N-MID <sup>®</sup> Osteocalcin	Serum/plasma	Detection of N-MID osteocalcin – a marker of bone formation	IS-2900 IS-2930 (control set)	264 265
	Ostase <sup>®</sup> (BAP)	Serum/plasma	Detection of bone-specific alkaline phosphatase – a marker of bone formation	IS-2800 IS-2830 (control set)	264 265
	BoneTRAP <sup>®</sup> (TRAcP 5b)	Serum/plasma	Tartrate-resistant acid phosphatase – a marker of bone resorption	IS-4100 IS-4130 (control set)	264 265
	Intact PINP	Serum/plasma	Intact N terminal propeptide of type I procollagen – a marker of bone formation	IS-4000 IS-4030 (control set)	264 265



# IDS products

Bone turnover markers · calcium metabolism



For more information on this subject scan the QR code or enter the Quick Link code **q076** at [www.euroimmun.com](http://www.euroimmun.com)

## Calcium metabolism

■ **Clinical information:** Calcium metabolism or calcium homeostasis is the regulation of calcium levels within the body. An important aspect of this is the maintenance of circulating calcium levels in the blood within a narrow range. The body maintains very tight control over the calcium circulating in the blood at any given time. The equilibrium is maintained by an interplay of calcium absorbed from the intestines, movement of calcium into and out of the bones, and the kidney's reclamation and excretion of calcium into the urine. The body regulates calcium through the parathyroid hormone (PTH), vitamin D, and, to a lesser extent, calcitonin.



If the serum calcium level falls, the parathyroid glands release parathyroid hormone (PTH) into the blood and this signals cells in bone (osteoclasts) to release calcium from the bone surfaces. PTH also signals the kidney to reclaim more calcium before it is excreted in the urine and stimulates synthesis of the active form of vitamin D, calcitriol (1,25-dihydroxy vitamin D).

Vitamin D<sub>3</sub> is made in the skin from 7-dehydrocholesterol under the influence of UV light. Vitamin D<sub>2</sub> (ergocalciferol) is derived from the plant sterol ergosterol. Vitamin D<sub>3</sub> and D<sub>2</sub> are converted to 25-hydroxy vitamin D (25-OH vitamin D) in the liver, then to the active form 1,25-dihydroxy vitamin D mostly by the kidneys.

■ **Diagnostics:** The determination of the total amount of circulating 25-OH vitamin D is particularly suitable for assessing the vitamin D supply status or for determining vitamin D insufficiency.

Because 1,25-dihydroxy vitamin D is the active form of vitamin D, it is often mistakenly assumed that the determination of 1,25-dihydroxy vitamin D allows accurate assessment of the vitamin D status and the detection of vitamin D deficiency. However, 1,25-dihydroxy vitamin D has little or no relationship to vitamin D stores. It is primarily regulated by PTH. The PTH concentration in turn depends on calcium and thus also on 25-OH vitamin D. The 1,25-dihydroxy vitamin D blood tests are useful in patients with kidney disease.

Elevated PTH levels, as can occur in vitamin D deficiency due to lowered calcium levels, stimulate bone resorption due to the maturation of osteoclasts that digest the bone matrix, which can lead to an increased risk of fractures, osteopenia, and osteoporosis. Increased levels of PTH can also cause demineralisation of the skeleton, e.g. osteomalacia, because of the increased renal loss of phosphorus. It is therefore necessary for individuals to maintain sufficient levels of 25-OH vitamin D to avoid elevations in PTH.




## Product details

Method	Analyte	Sample material	Application	Order number	Page
ELISA	25-OH vitamin D	Serum/plasma	ELISA with an analytical specificity of 100 % for 25-OH vitamin D <sub>2</sub> and D <sub>3</sub>	EQ 6411-9601	261
	Intact parathyroid hormone (iPTH)	Serum/plasma	Specific detection by combination of N and C terminus-specific antibodies	EQ 6421-9601	260
	1,25-Dihydroxy vitamin D	Serum/plasma	Detection of 1,25-(OH) <sub>2</sub> vitamin D	AC-62F1	262
ChLIA	25-OH vitamin D	Serum/plasma	Fully automated detection of total 25-OH vitamin D – a CDC VDSCP certified test	IS-2500N IS-2530N (control set)	263
	1,25-Dihydroxy vitamin D	Serum	Fully automated detection of 1,25-(OH) <sub>2</sub> vitamin D	IS-2000 IS-2030 (control set)	264 265
	1,25-Dihydroxy vitamin D	Serum/plasma	Semi-automated detection of 1,25-(OH) <sub>2</sub> vitamin D	IS-2400 IS-2430 (control set)	264 265
	Intact PTH	Serum/plasma	Fully automated detection of intact PTH	IS-3200 IS-3230 (control set)	264 265



# Products for antigen detection

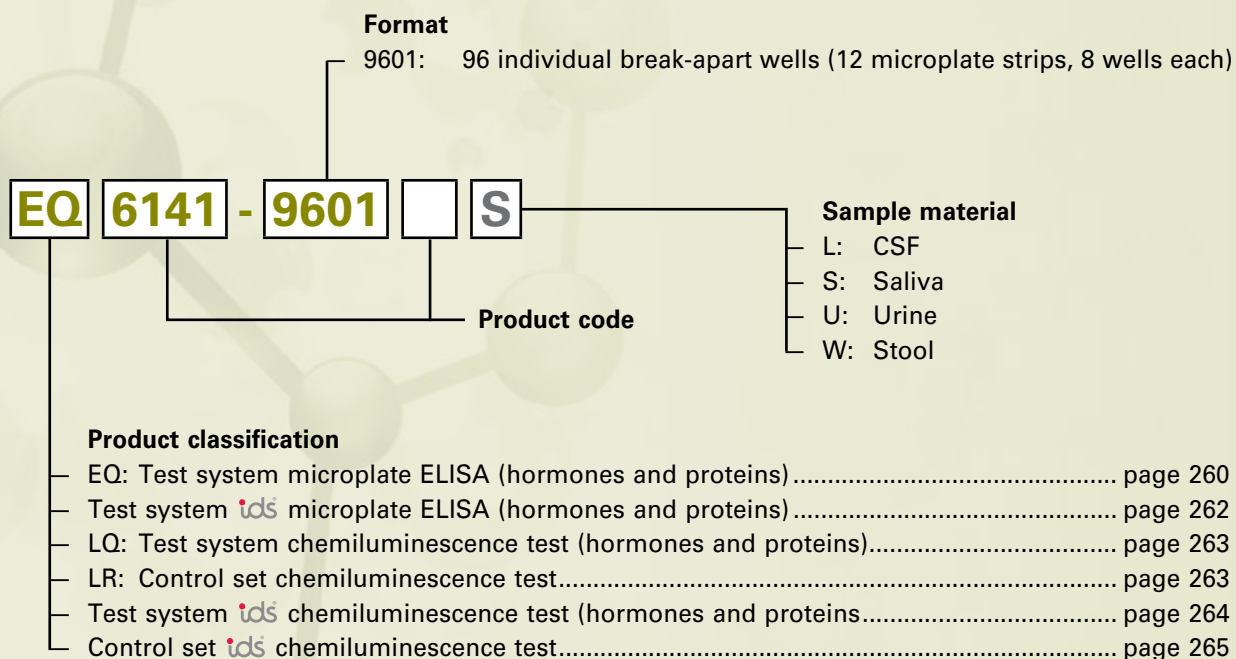

Antigen detection

For product orders the amount, product code and test name are required. **Test kits** comprise all reagents needed to perform the investigation.




**Microplate ELISA for the Determination of Hormones and Proteins (Test Systems)**

Order No.	Analyte	Calibration	Format
EQ 1016-9601	free triiodothyronine (FT3)	0/2/4/8/16/40 pg/ml	96 x 01
EQ 1016-9601-9	reverse triiodothyronine (RT3)	0/0.02/0.1/0.4/1/2 ng/ml	96 x 01
EQ 1017-9601	free thyroxine (FT4)	0/2/6/20/80 pg/ml	96 x 01
EQ 2606-9601	SARS-CoV-2 Antigen	semi-quantitative	96 x 01
EQ 266a-9601-1	Dengue virus NS1 antigen detection (DENV)	1/10/100 RU/ml	96 x 01
EQ 6141-9601 S	cortisol determination in saliva	0/0.3/1/3/10/30 ng/ml	96 x 01
EQ 6143-9601	aldosterone	0/15/50/200/500/1000 pg/ml	96 x 01
EQ 6151-9601	free testosterone	0/0.1/1/5/20/60 pg/ml	96 x 01
EQ 6151-9601-1	total testosterone	0/0.08/0.42/1.67/5/16.7 ng/ml	96 x 01
EQ 6152-9601-1	Dihydrotestosteron	0/25/100/250/500/1000/2500 pg/ml	96 x 01
EQ 6153-9601	androstenedione	0/0.1/0.3/1/3/10 ng/ml	96 x 01
EQ 6154-9601	dehydroepiandrosterone (DHEA)	0/0.2/1/5/15/40 ng/ml	96 x 01
EQ 6155-9601	dehydroepiandrosterone sulfate (DHEA-S)	0/0,005/0,02/0,1/0,5/2,5/10 µg/ml	96 x 01
EQ 6156-9601	3alpha-androstanediol glucuronid (3alpha-adiol G)	0/0.25/1/3/10/50 ng/ml	96 x 01
EQ 6160-9601-1	total estrogens	0-2500 pg/ml	96 x 01
EQ 6163-9601	17-OH-progesterone	0/0.15/0.5/1.5/3/7.5/20 ng/ml	96 x 01
EQ 6164-9601	pregnenolone	0/0.1/0.4/1.6/6.4/25.6 ng/ml	96 x 01
EQ 6165-9601-1	estrone	0/20/60/200/600/2000 pg/ml	96 x 01
EQ 6167-9601	Free Estriol ELISA	0/0,05/0,25/1/5/30 ng/ml	96 x 01
EQ 6179-9601	sex hormone-binding globulin (SHBG)	0/3.3/12.5/55/160/295 nmol/l	96 x 01
EQ 6411-9601	25-OH vitamin D	0/4/10/25/60/120 ng/ml	96 x 01
EQ 6421-9601	intact PTH	0-500 pg/ml	96 x 01
EQ 6431-9601	calcitonin	0-500 pg/ml	96 x 01
EQ 6444-9601	leptin	0/1/5/10/20/50/100 ng/ml	96 x 01
EQ 6446-9601	adiponectin	0/2/5/10/25/50 ng/ml	96 x 01
EQ 6511-9601 *	beta-amyloid (1-40) determination in plasma	0-75 pg/ml	96 x 01
EQ 6511-9601-L	beta-amyloid (1-40) determination in CSF	0-900 pg/ml	96 x 01
EQ 6521-9601 *	beta-amyloid (1-42) determination in plasma	0-40 pg/ml	96 x 01
EQ 6521-9601-L	beta-amyloid (1-42) determination in CSF	0-1800 pg/ml	96 x 01
EQ 6531-9601-L	total tau determination in CSF	0-1500 pg/ml	96 x 01


\* For research use only, not for in vitro diagnostic use in the sense of EU directive 98/79/EC.


**Microplate ELISA for the Determination of Hormones and Proteins (Test Systems)**

Order No.	Analyte	Calibration	Format
EQ 6541-9601-L *	<b>BACE-1</b> determination in CSF	0-12000 pg/ml	96 x 01
EQ 6545-9601-L *	<b>alpha-synuclein</b> determination in CSF	0-6000 pg/ml	96 x 01
EQ 6551-9601-L *	<b>neurogranin</b> determination in CSF	0-1300 pg/ml	96 x 01
EQ 6561-9601	<b>neurofilament (pNf-H)</b> determination in CSF and serum	0/0,125/0,5/2/5/10 ng/ml	96 x 01
EQ 6562-9601	<b>neurofilament (pNf-H)</b> highly sensitive determination in serum and plasma	0/20/50/200/500/1000 pg/ml	96 x 01
EQ 6591-9601-L	<b>pTau(181)</b> determination in CSF	0-200 pg/ml	96 x 01
EQ 6811-9601-L	<b>CXCL13</b> determination in CSF	0-500 pg/ml	96 x 01
EQ 6821-9601	<b>uromodulin</b> determination in serum	0/25/50/100/200/400 ng/ml	96 x 01
EQ 6825-9602	<b>Plasma Renin Activity (PRA)</b>	0/0,2/0,5/1,5/4/10/25/60 ng/ml	96 x 02
EQ 6831-9601 W	<b>calprotectin</b> determination in stool	0/15/60/240/960/2100 µg/g	96 x 01
EQ 6841-9601	<b>Quan-T-Cell ELISA</b> To be used in combination with ET 2606	12-400 mIU/ml	96 x 01
EQ 6851-9601-U	<b>sCD163</b> determination in urine	0-12 ng/ml	96 x 01
EQ 6911-9601	<b>Aspergillus antigen</b>	0/20/50/125/312.5/625 pg/ml	96 x 01

\* For research use only, not for in vitro diagnostic use in the sense of EU directive 98/79/EC.


**IDS Microplate ELISA for the Determination of Hormones and Proteins (Test Systems)**

IDS Order No.	Description	Format	
AC-57SF1	25-Hydroxy Vitamin D S EIA	96 x 01	
AC-62F1	1,25-Dihydroxy Vitamin D EIA	96 x 01	
AC-20F1	Ostase® BAP EIA	96 x 01	
AC-02F1	Serum CrossLaps® (CTX-I) ELISA	96 x 01	
AC-03F1	Urine CrossLaps® (CTX-I) EIA	96 x 01, determination in urine	
AC-04F1	Urine Alpha CrossLaps® (CTX-I) EIA	96 x 01, determination in urine	
AC-05F1	Urine BETA CrossLaps® (CTX-I) ELISA	96 x 01, determination in urine	
SB-TR201A	BoneTRAP® (TRAcP 5b) ELISA	96 x 01	
AC-11F1	N-MID® Osteocalcin ELISA	96 x 01	
AC-10F1	Urine CartiLaps® (CTX-II) EIA	96 x 01, determination in urine	
AN-14-1006-71	Human COMP® ELISA	96 x 01	



### Chemiluminescence Tests for the Determination of Hormones and Proteins (Test Systems)

Order No.	Analyte	Calibration	Format
LQ 6511-10010-L	beta-amyloid (1-40) determination in CSF	0-20000 pg/ml	100 determinations for RA Analyzer 10
LQ 6521-10010-L	beta-amyloid (1-42) determination in CSF	0-2000 pg/ml	100 determinations for RA Analyzer 10
LQ 6531-10010-L	Total Tau determination in CSF	0-2000 pg/ml	100 determinations for RA Analyzer 10
LQ 6591-10010-L	pTau (181) determination in CSF	0-400 pg/ml	100 determinations for RA Analyzer 10
LQ 6831-10010 W	calprotectin determination in stool	0-1000 µg/g	100 determinations for RA Analyzer 10

### Control Sets for Chemiluminescence Tests

Order No.	Control Set (Ready for use)	Format
LR 6511-20210-L	Control set beta-amyloid (1-40) determination in CSF	2 x 0.5 ml control 1/2
LR 6521-20210-L	Control set beta-amyloid (1-42) determination in CSF	2 x 0.5 ml control 1/2
LR 6531-20210-L	Control set Total Tau determination in CSF	2 x 0.5 ml control 1/2
LR 6591-20210-L	Control set pTau (181) determination in CSF	2 x 0.5 ml control 1/2
LR 6831-20210 W	Control set calprotectin determination in stool	2 x 0.5 ml control 1/2



## IDS Chemiluminescence Tests for the Determination of Hormones/Proteins (Test Systems)

IDS Order No.	Description	Format
IS-4600	IDS Cortisol	100 determinations
IS-4900	IDS Salivary Cortisol	100 determinations, calibrators incl.
IS-3300	IDS Aldosterone	100 determinations, calibrators incl.
IS-4500N	IDS ACTH	100 determinations
IS-5300	IDS Free Testosterone	100 determinations, calibrators incl.
IS-5000	IDS Total Testosterone	100 determinations, calibrators incl.
IS-5100	IDS 17-OH Progesterone	100 determinations, calibrators incl.
IS-5600	IDS SHBG	100 determinations, calibrators incl.
IS-3700	IDS human Growth Hormone (hGH)	100 determinations, calibrators incl.
IS-3900	IDS Insulin-like Growth Factor-I (IGF-I)	100 determinations, calibrators incl.
IS-4400	IDS Insulin-like Growth Factor Binding Protein-3 (IGFBP-3)	100 determinations, calibrators incl.
IS-4700	IDS Inaktif MGP (dp-uc MGP)	100 determinations, calibrators incl.
IS-2500N	IDS 25 VitD S	100 determinations
IS-2000	IDS 1,25 VitD Xp	100 determinations, calibrators incl.
IS-2400	IDS 1,25-Dihydroxy Vitamin D	100 determinations, calibrators incl.
IS-2800	IDS Ostase® BAP	100 determinations, calibrators incl.
IS-3000	IDS CTX-I (CrossLaps®)	100 determinations, calibrators incl.
IS-4100	IDS TRAcP 5b (BoneTRAP®)	100 determinations, calibrators incl.
IS-2900	IDS N-MID® Osteocalcin	100 determinations, calibrators incl.
IS-3200	IDS Intact PTH	100 determinations, calibrators incl.
IS-4000	IDS Intact PINP	100 determinations, calibrators incl.
IS-3400	IDS Direct Renin	100 determinations, calibrators incl.
IS-5900	IDS ACE	100 determ., calibrators/controls incl.
IS-6000	IDS Calprotectin	100 determinations



Antigen  
detection



IDS Control Sets for Chemiluminescence Tests			ids®
IDS Order No.	Description	Format	
IS-4620	IDS Cortisol Calibrator Set	6 concentration levels	
IS-4630	IDS Cortisol Control Set	2 concentration levels	
IS-4930	IDS Salivary Cortisol Control Set	3 concentration levels	
IS-3330	IDS Aldosterone Control Set	3 concentration levels	
IS-4520N	IDS ACTH Calibrator Set	6 concentration levels	
IS-4530N	IDS ACTH Control Set	3 concentration levels	
IS-5030	IDS Total Testosterone Control Set	3 concentration levels	
IS-5330	IDS Free Testosterone Control Set	3 concentration levels	
IS-5130	IDS 17-OH Progesterone Control Set	3 concentration levels	
IS-5630	IDS SHBG Control Set	3 concentration levels	
IS-3930	IDS Insulin-like Growth Factor-I (IGF-I) Control Set	3 concentration levels	
IS-4430	IDS Insulin-like Growth Factor Binding Protein-3 (IGFBP-3) Control Set	3 concentration levels	
IS-4730	IDS Inaktif MGP (dp-uc MGP) Control Set	3 concentration levels	
IS-2520N	IDS 25 VitD S Calibrator Set	6 concentration levels	
IS-2530N	IDS 25 VitD S Control Set	2 concentration levels	
IS-2030	IDS 1,25 VitD Xp Control Set	2 concentration levels	
IS-2430	IDS 1,25-Dihydroxy Vitamin D Control Set	2 concentration levels	
IS-2830	IDS Ostase® BAP Control Set	3 concentration levels	
IS-3030	IDS CTX-I (CrossLaps®) Control Set	3 concentration levels	
IS-4130	IDS TRAcP 5b (BoneTRAP®) Control Set	3 concentration levels	
IS-2930	IDS N-MID® Osteocalcin Control Set	3 concentration levels	
IS-3230	IDS Intact PTH Control Set	3 concentration levels	
IS-4030	IDS Intact PINP Control Set	3 concentration levels	
IS-3430	IDS Direct Renin Control Set	3 concentration levels	
IS-6020	IDS Calprotectin Calibrator Set	5 concentration levels	
IS-6030	IDS Calprotectin Control Set	2 concentration levels	



# Molecular genetic diagnostics







# Molecular genetics

ApoE · F V / II / MTHFR · HLA-B27 · HLA-B57:01 · HLA-Cw6 · HLA-DQ2/8 · HFE · LCT



For more information on this subject scan the QR code or enter the Quick Link code **q142** at [www.euroimmun.com](http://www.euroimmun.com)

## ApoE

■ **Clinical information:** The molecular genetic determination of the APOE alleles  $\epsilon 2$ ,  $\epsilon 3$  and  $\epsilon 4$  is used in particular for the differential diagnosis and/or early identification of Alzheimer's disease (AD) and type III hyperlipoproteinaemia.

Apolipoprotein E (ApoE) is a component of lipoproteins in blood and plays an important role in fat metabolism, but also in blood coagulation, the immune response, and the protection from oxidative processes. ApoE binds to the amyloid  $\beta$  peptide, which plays a central role in neurodegeneration in Alzheimer's patients. There are three different APOE alleles:  $\epsilon 2$ ,  $\epsilon 3$  and  $\epsilon 4$ . From these alleles, three different isoforms of the ApoE protein (E2, E3 and E4) are produced, which differ in the amino acids at positions 112 and 158.

The APOE allele  $\epsilon 4$  occurs in Alzheimer's patients around three times more frequently than in the normal population (36.7% versus 13.7%). In contrast, the APOE allele  $\epsilon 2$  is rarer in Alzheimer's patients than in the normal population (3.9% versus 8.4%). Correspondingly, carriers of an APOE  $\epsilon 4$  allele have an increased risk of developing Alzheimer's disease, while the APOE allele  $\epsilon 2$  is associated with a reduced risk. In families with the late form of Alzheimer's disease, the disease risk and the average age of disease onset is strongly dependent on the  $\epsilon 4$  gene dosage: 20% and 84 years for non  $\epsilon 4$  carriers, 47% and 76 years for heterozygote and 91% and 68 years for homozygote carriers of the  $\epsilon 4$  allele.

Homozygosity for the APOE allele  $\epsilon 2$  has been identified as the primary molecular cause of type III hyperlipidaemia (familial dysbetalipoproteinaemia), which leads to a greatly increased risk of arteriosclerosis.

Alongside its significance for differential diagnosis, the determination of APOE alleles has an increasing pharmacological significance in the development of new medications against Alzheimer's disease.

■ **Diagnostics:** The EUROArray APOE Direct was especially developed for specific determination of the APOE gene variants  $\epsilon 2$ ,  $\epsilon 3$  and  $\epsilon 4$  and enables fast and simple analysis of the APOE alleles in a single test. In the unique direct procedure, whole-blood samples can be used directly without the need for DNA isolation, which saves time and costs. Data analysis, data interpretation and archiving are done completely automated by means of the EUROArrayScan software. In the results it is exactly distinguished between homozygous and heterozygous presence of the different possible genotypes. In the context of Alzheimer's diagnostics, the EUROArray APOE Direct is a good complement to the antibody-based test systems offered by EUROIMMUN.



## Product overview

Parameter	Sample material	Application	Order number	Page
APOE Direct	Whole blood/ genomic DNA	Molecular biological in vitro determination of disease-associated APOE alleles in human genomic DNA for diagnosis of Alzheimer's disease, type III hyperlipoproteinaemia and other diseases associated with alleles $\epsilon 2$ , $\epsilon 3$ and/or $\epsilon 4$ of the APOE gene.	MN 5710-####-V	300



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q080** at [www.euroimmun.com](http://www.euroimmun.com)



# Molecular genetics

ApoE · F V / II / MTHFR · HLA-B27 · HLA-B57:01 · HLA-Cw6 · HLA-DQ2/8 · HFE · LCT



For more information on this subject scan the QR code or enter the Quick Link code **q135** at [www.euroimmun.com](http://www.euroimmun.com)

## Factor V / Factor II / MTHFR

■ **Clinical information:** Deep and superficial venous thrombosis and thromboembolism of the brain, lung and coronary vessels are among the most frequent causes of death in western industrialised countries. These conditions result from a combination of genetic and exogenous factors. More than half of all thromboembolic cases are caused by genetic risk factors, particularly if the disease occurs before the age of 45 without any noticeable external factors or at an atypical location. The most important and most frequent genetic risk factors are the factor V Leiden (1691G>A) and the factor II 20210G>A mutations. Furthermore, two polymorphisms in the methylene tetrahydrofolate reductase (MTHFR) gene are associated with an increase in the homocystein level (hyperhomocysteinemia), which is also a risk factor for thrombosis. An increased homocysteine level is also associated with an increased risk of neural tube defects, premature delivery, abortion and implantation failure in in vitro fertilisation.

The mutated factor V can be only insufficiently inactivated by activated protein C (APC). This so-called APC resistance results in an increased thrombosis tendency. The factor II (prothrombin) 20210G>A mutation leads to increased prothrombin plasma levels, resulting in an increased risk of thrombosis. If these mutations are present in both genes, the risk of venous thrombosis is 20 times higher. If these genetic risk factors are accompanied by other genetic predisposing gene variants such as mutations in the MTHFR gene, the total risk of thromboembolism is expected to be increased even further.

■ **Diagnostics:** The **EUROArray FV / FII+ / MTHFR Direct** has been designed to provide secure determination of the most important genetic thrombosis risk factors and is easy to perform. In the direct procedure, the blood sample is treated with two extraction reagents and can then be used directly in the PCR. The time-consuming and cost-intensive DNA isolation is no longer necessary. Data analysis, data interpretation and archiving are fully automated using the **EUROArrayScan software**. Due to integrated mutation controls, the EUROArray FV / FII+ / MTHFR Direct ensures the highest possible reliability of results, even for rare genotypes. The controls indicate whether the analysed DNA contains further known mutations in direct proximity to the investigated sequence variants that may affect the binding to the probes and, consequently, the test result. Different EUROArray test systems are available for the determination of the FV Leiden and FII 20210G>A mutations and the polymorphisms 677C>T and 1298A>C in the MTHFR gene. Thus, the determinations can be performed separately or together in one test run, depending on the analysis request.



## Product overview

Parameter	Sample material	Application	Order number	Page
FV/FII+/MTHFR Direct	Whole blood/ genomic DNA	Molecular biological in vitro determination of point mutations or single-nucleotide polymorphisms in the factor V gene (factor V Leiden, 1691G>A), factor II (prothrombin) gene (20210G>A) and/or MTHFR gene (677C>T and 1298A>C) in human genomic DNA to assess the genetic thrombosis risk	MN 5820-####-V	300
FV/FII+ Direct	Whole blood/ genomic DNA		MN 5821-####-V	301
FV Leiden Direct	Whole blood/ genomic DNA		MN 5822-####-V	301
FII+ Direct	Whole blood/ genomic DNA		MN 5823-####-V	301
MTHFR Direct	Whole blood/ genomic DNA		MN 5824-####-V	301



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g080** at [www.euroimmun.com](http://www.euroimmun.com)



# Molecular genetics

ApoE · F V / II / MTHFR · HLA-B27 · HLA-B57:01 · HLA-Cw6 · HLA-DQ2/8 · HFE · LCT



For more information on this subject scan the QR code or enter the Quick Link code **q130** at [www.euroimmun.com](http://www.euroimmun.com)

## HLA-B27

■ **Clinical information:** Human leukocyte antigens (HLA) are tissue antigens of the human major histocompatibility complex (MHC). HLA-B belongs to the HLA antigens of class I (also called MHC I antigens) which are present on all nucleus-containing cells of the body. Their function is the control of the T-cell-mediated immune response. Due to an extreme genetic polymorphism there are a large number of HLA phenotypes. For HLA-B over 1000 different alleles have been described. The HLA-B\*27 allele alone has 130 subtypes (B\*27:01 to B\*27:105), which differ only in a few bases. The membrane-bound HLA-B27 protein is associated with the occurrence of several autoimmune diseases, such as ankylosing spondylitis (Bechterew's disease). Around 3 to 6% of HLA-B\*27 carriers develop ankylosing spondylitis. Around 90% of ankylosing spondylitis patients are carriers of this tissue antigen, in particular subtypes B\*27:02, B\*27:04 and B\*27:05. The subtypes B\*27:06 and B\*27:09 on the other hand are not associated with ankylosing spondylitis. Therefore, subtype differentiation is necessary for confirmation of diagnosis in particular populations.

■ **Diagnostics:** HLA-B27 can be determined accurately and precisely with molecular biological methods via the detection of the corresponding allele (HLA-B\*27) in the genomic DNA of the patient. Due to the cross reactivity that occurs with antibodies (with e.g. HLA-B7) and possible false negative results in immunophenotyping when HLA-B\*27 expression is low, molecular genetic determination of HLA-B\*27 is more specific and sensitive than serological methods. Especially the PCR method using allele-specific primers has the potential to provide reliable results, particularly for the various HLA-B\*-27 subtypes.

The HLA-B\*27 primers for this test system have been chosen and optimised so that all currently known HLA-B\*27 subtypes are detected. Furthermore, when a positive result is obtained, it is indicated whether subtypes HLA-B\*27:06 or HLA-B\*27:09 could be involved. These two subtypes are not associated with ankylosing spondylitis. With the unique direct procedure, the DNA does not have to be isolated. The blood sample is treated with two extraction reagents and can then be used directly in the PCR. Data analysis, data interpretation and archiving are fully automated using the **EUROArrayScan software**. Numerous controls on the **EUROArray HLA-B27** verify the correctness of the results. For every reaction it is verified that human DNA was present in the PCR and that the primers for the amplification were functional, which is particularly relevant when negative HLA-B27 results are obtained. All of these controls ensure a reliable test result with just one PCR reaction.



## Product overview

Parameter	Sample material	Application	Order number	Page
HLA-B27 Direct	Whole blood/ genomic DNA	Molecular biological in vitro determination of disease-associated HLA-B*27 alleles in human genomic DNA in the diagnosis of rheumatic diseases, in particular ankylosing spondylitis (Bechterew's disease)	MN 5110-####-V	300



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q080** at [www.euroimmun.com](http://www.euroimmun.com)





# Molecular genetics

ApoE · F V / II / MTHFR · HLA-B27 · HLA-B57:01 · HLA-Cw6 · HLA-DQ2/8 · HFE · LCT



For more information on this subject scan the QR code or enter the Quick Link code **q131** at [www.euroimmun.com](http://www.euroimmun.com)

## HLA-B57:01

■ **Clinical significance:** Genetic testing for HLA-B\*57:01 is useful for preventing hypersensitivity reactions against the HIV chemo-pharmaceutical agent abacavir. All HIV-infected patients should be tested for the presence of the HLA-B\*57:01 allele before starting treatment with drugs containing abacavir sulphate.

Symptoms of a hypersensitivity reaction are fever, exanthema, pruritus, occasionally gastrointestinal and respiratory problems, joint pain and increased liver/kidney parameters with a progressive course up to death, especially with re-exposure. Depending on the ethnic group, a significant part of the treated patients are affected. Reactions have proven to occur in 8 to 16% of black Africans, 20 to 22% of Hispanics and 48 to 61% of Caucasians. Around 8% of people carry the HLA-B\*57:01 allele. The prevalence ranges between 0.1% (e.g. Japanese) and 19.6% (e.g. South Africans).

■ **Diagnostics:** The EUROArray HLA-B57:01 Direct enables fast and simple detection of HLA-B\*57:01 alleles – no in-depth knowledge of molecular biology is required. The primers and probes employed in this test system were selected and optimised such that all HLA-B\*57:01 alleles known worldwide can be sensitively and specifically detected in a single reaction. The direct method enables the direct use of whole blood samples. Therefore, a time- and cost-consuming DNA isolation is no longer required. The evaluation, generation and archiving of results are carried out fully automatically with the **EUROArrayScan software**.



## Product overview

Parameter	Sample material	Application	Order number	Page
HLA-B57:01 Direct	Whole blood/ genomic DNA	Molecular genetic in vitro determination of HLA-B*57:01 alleles in human genomic DNA, associated with hypersensitivity reactions during treatment with abacavir.	MN 5210-####-V	300



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q080** at [www.euroimmun.com](http://www.euroimmun.com)



# Molecular genetics

ApoE · F V / II / MTHFR · HLA-B27 · HLA-B57:01 · HLA-Cw6 · HLA-DQ2/8 · HFE · LCT



For more information on this subject scan the QR code or enter the Quick Link code **q132** at [www.euroimmun.com](http://www.euroimmun.com)

## HLA-Cw6

■ **Clinical information:** Human leukocyte antigens (HLA) are tissue antigens of the human major histocompatibility complex (MHC), which is localised on the short arm of chromosome 6. HLA-C belongs to the HLA antigens of class I (also called MHC I antigens), which are represented on all nucleus-containing cells of the body. Their function is the control of the T-cell-mediated immune response.

HLA-C\*06 alleles are the genetic component for the disposition to the autoimmune reactions that result in psoriasis. There is a strong genetic component to psoriasis; around 40% of cases are familial. Monozygotic twins show a concordance rate of 62 to 70% and dizygotic twins of 21 to 23%. Total-genome association studies have confirmed that of all gene sites HLA-C shows the highest association with psoriasis, and HLA-C\*06 can be considered as by far the most powerful genetic marker for the disease. Around 67% of psoriasis patients carry the HLA-C\*06 allele compared to a prevalence of around 10 to 20% for the HLA-Cw6 antigen in the general population. Caucasians with the HLA-C\*06 allele have a 10-fold increased risk of developing psoriasis. An association of psoriatic arthritis with HLA-Cw6 has also been described. The detection of the allele can therefore also be used to support the diagnosis. This can enable the differentiation from other arthritides especially in psoriatic arthritis patients with ambiguous skin changes or in patients with an unavailable family anamnesis.

■ **Diagnostics:** The **EUROArray HLA-Cw6 Direct** has been specifically designed for the determination of HLA-C\*06 alleles coding for HLA-Cw6. It is therefore particularly easy to perform compared to other molecular biological methods for the detection of HLA-C\*06. With the unique direct procedure, the DNA does not have to be isolated. The whole blood sample is merely treated with two extraction reagents and can then be used directly in the PCR.

In chronic inflammatory skin diseases the determination of HLA-C\*06 is of great significance for differential diagnostics, since the presence of the HLA-Cw6 antigen is associated in particular with type 1 psoriasis vulgaris (OR 16.0) and psoriasis guttata (OR 33.6), but is only comparatively weakly associated (OR 2.6) with type 2 psoriasis vulgaris. In type 1 psoriasis vulgaris around 83% of patients carry the HLA-C\*06 allele, whereas in type 2, which has a milder course, the proportion of HLA-Cw6-positive patients is only 44%. In the EUROArray HLA-Cw6 Direct the PCR primers have been chosen and optimised so that all relevant HLA-C\*06 subtypes are detected. Data analysis, data interpretation and archiving are fully automated using the **EUROArrayScan software**. For every reaction the presence of isolated human genomic DNA is verified. Moreover, the functionality of the primers for HLA-Cw6 is verified, providing additional security with negative results.



## Product overview

Parameter	Sample material	Application	Order number	Page
HLA-Cw6 Direct	Whole blood/ genomic DNA	Molecular genetic in vitro determination of disease-associated HLA-C*06 alleles in human genomic DNA in the diagnosis of psoriasis with skin manifestation (in particular type 1 psoriasis vulgaris, psoriasis guttata, type 2 psoriasis vulgaris), joint manifestation (in particular psoriatic arthritis) etc.	MN 5410-####-V	300



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q080** at [www.euroimmun.com](http://www.euroimmun.com)



# Molecular genetics

ApoE · F V / II / MTHFR · HLA-B27 · HLA-B57:01 · HLA-Cw6 · HLA-DQ2/8 · HFE · LCT



For more information on this subject scan the QR code or enter the Quick Link code **q133** at [www.euroimmun.com](http://www.euroimmun.com)

## HLA-DQ2/DQ8

■ **Clinical information:** The determination of HLA-DQ2/DQ8 is important to diagnostically exclude coeliac disease, an autoimmune disease which occurs in predisposed individuals as a reaction to gluten sensitivity. Almost 100% of coeliac disease patients possess the genetic risk factors HLA-DQ2 or HLA-DQ8. These are heterodimeric surface receptors consisting of an alpha and a beta chain, which are coded by the HLA-DQA1 and HLA-DQB1 alleles of human leukocyte antigens (HLA).

The determination of HLA-DQ2 and HLA-DQ8 is, above all, significant for the following: doubtful biopsy results, ambiguous serology (especially in children under 2 years old), patients on a gluten-free diet with inconclusive diagnosis, clarification of the genetic predisposition of first-degree relatives of coeliac disease patients, and differentiation from other intestinal diseases. Around 95% of coeliac disease patients have the HLA-DQ2 genotype, which is subdivided into HLA-DQ2.5 and HLA-DQ2.2. HLA-DQ2.5 is composed of the allele HLA-DQA1\*05:01 (or DQA1\*05:05) coding for the alpha chain and the allele HLA-DQB1\*02:01 (or DQB1\*02:02) coding for the beta chain. HLA-DQ2.2 consists of the allele HLA-DQA1\*02 coding for the alpha chain and the allele HLA-DQB1\*02:02 coding for the beta chain. Those patients who are not HLA-DQ2 positive exhibit the genotype HLA-DQ8, which, according to the ESPGHAN guidelines, is determined by the presence of the alleles HLA-DQA1\*03:01 and HLA-DQB1\*03:02. In many studies which investigated the relation between the presence of HLA-DQ and coeliac disease, the alleles HLA-DQA1\*03:01/02/03 are not differentiated and therefore all classed as alpha subunit of DQ8.

Moreover, the differentiation between homo- and heterozygous presence of the alleles coding for the alpha and beta subunits of HLA-DQ2.2 and -DQ2.5 enables an improved risk assessment.

■ **Diagnostics:** The detection of the two leukocyte antigens is important in the diagnosis of coeliac disease, since almost 100% of coeliac disease patients are positive for either DQ2 or DQ8. Although these markers are not particularly specific – around 50% of the healthy population also carries one of these two antigens – the absence of these risk factors is an important exclusion criterion as they possess a negative predictive value of near to 100%. If neither DQ2.2, DQ2.5, nor DQ8 are detected in a patient, then coeliac disease can be as good as excluded.

The **EUROArray HLA-DQ2/DQ8 Direct** has been specifically optimised for the determination of the disease-associated HLA-DQA1 and HLA-DQB1 alleles coding for the subunits of HLA-DQ2.2, -DQ2.5 and -DQ8. The test system **EUROArray HLA-DQ2/DQ8-h Direct** enables more comprehensive diagnostics since it includes the determination of the homo- and heterozygous presence of the alleles coding for HLA-DQ2.2 or -DQ2.5. Both analyses are extremely easy to perform. Owing to the unique direct procedure, the DNA no longer needs to be isolated. The blood sample is treated with two extraction reagents and can then be directly used in the PCR. The PCR primer and microarray probes are selected and optimised in such way that all relevant HLA-DQA1 and HLA-DQB1 alleles can be reliably detected. Data analysis, data interpretation and archiving are fully automated using the **EUROArrayScan Software**. The exact analysis of the alpha and beta subunits of the DQ2 and DQ8 molecules ensures reliable and unambiguous results. In combination with antibody diagnostics (see page 114): Anti-



Endomysium IIFT, Anti-Tissue Transglutaminase ELISA and the new highly specific tests Anti-Gliadin (GAF-3X) ELISA and EUROPLUS Anti-Gliadin (GAF-3X) IIFT, the EUROArray HLA-DQ2/DQ8 offers accurate and reliable diagnostics for coeliac disease and dermatitis herpetiformis.

## Product overview

Parameter	Sample material	Application	Order number	Page
HLA-DQ2/DQ8 -h Direct	Whole blood/ genomic DNA	Molecular genetic in vitro determination of disease-associated HLA-DQA1 and HLA-DQB1 alleles in human genomic DNA in the diagnosis of gluten-sensitive enteropathy (coeliac disease, sprue) and dermatitis herpetiformis.	MN 5320-####-V	300
HLA-DQ2/DQ8 Direct	Whole blood/ genomic DNA	Molecular genetic in vitro determination of disease-associated HLA-DQA1 and HLA-DQB1 alleles in human genomic DNA in the diagnosis of gluten-sensitive enteropathy (coeliac disease, sprue) and dermatitis herpetiformis.	MN 5321-####-V	300



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q080** at [www.euroimmun.com](http://www.euroimmun.com)



# Molecular genetics

ApoE · F V / II / MTHFR · HLA-B27 · HLA-B57:01 · HLA-Cw6 · HLA-DQ2/8 · HFE · LCT



For more information on this subject scan the QR code or enter the Quick Link code **q134** at [www.euroimmun.com](http://www.euroimmun.com)

## HFE gene (haemochromatosis)

■ **Clinical information:** Hereditary haemochromatosis is the most frequent autosomal, recessive inherited metabolic disorder and results from increased resorption of iron in the upper small intestine. In affected individuals the iron uptake from food leads to an increase in the total iron content in the body from approximately 2 to 6g (normal value) to up to 80g. The iron then deposits in the liver, pancreas, spleen, thyroid gland, pituitary gland, heart and joints. In untreated patients irreversible damage occurs, resulting in an increased risk of cardiomyopathy, arthropathy, diabetes mellitus, liver cirrhosis and liver and pancreas carcinoma. In Germany, it is estimated that more than 200,000 people suffer from hereditary haemochromatosis, which is one of the most common genetic diseases in northern Europe.

Two mutations in the HFE gene are directly associated with this disease. They lead to a loss or reduction of the physiological function of the Hfe protein. The two mutations result in the amino acid substitutions C282Y and H63D, which represent the most frequent haemochromatosis-associated mutations (90%). Besides C282Y and H63D, there are two further rare mutations in the HFE gene that are also associated with the development of haemochromatosis. These cause either a change in the amino acid sequence (S65C) of the Hfe protein or early termination of protein synthesis (E168X).

New studies show that 90 to 100% of haemochromatosis patients exhibit homozygous gene defects. However, even a mutation in one HFE allele is sufficient to cause at least minor abnormalities in iron metabolism. By determining the mutations in the HFE gene, the predisposition to hereditary haemochromatosis can already be detected in childhood, so that preventive measures can be taken at an early stage (e.g. reduced consumption of foods with a high iron content).

■ **Diagnostics:** The **EUROArray Haemochromatosis (2 SNP+) Direct** enables reliable determination of the two most common haemochromatosis-associated mutations, C282Y and H63D, in the HFE gene. A more comprehensive investigation, additionally encompassing the more rarely occurring mutations, is offered by the test system **EUROArray Haemochromatosis (4 SNP+) Direct**, which comprises the analysis of C282Y, H63D, S65C and E168X. With the unique direct procedure, the time-consuming and cost-intensive DNA isolation is no longer required. The blood sample is merely treated with two extraction reagents and can then be used directly in the PCR. The PCR primers and microarray probes in these test systems have been chosen so that the mutations in the HFE gene described above are clearly identified. Data analysis, data interpretation and archiving are fully automated using the **EUROArrayScan software**. When a positive result is obtained, the system differentiates between homozygous and heterozygous mutations. Unique integrated controls indicate whether the analysed DNA contains further known mutations in addition to the investigated sequence variants that may affect the binding to the probes and, consequently, the test result. Thus, the EUROArray Haemochromatosis (4 SNP+ or 2 SNP+) Direct ensures the highest possible reliability of results even for rare genotypes.





## Product overview

Parameter	Sample material	Application	Order number	Page
Haemochromatosis (4 SNP+) Direct	Whole blood/ genomic DNA	Molecular genetic in vitro determination of two or four mutations in the HFE (high iron) gene in human genomic DNA in the detection or exclusion of the genetically caused iron overload disorder hereditary haemochromatosis in cases of conspicuous patient or family anamnesis	MN 5520-####-V	300
Haemochromatosis (2 SNP+) Direct	Whole blood/ genomic DNA		MN 5521-####-V	300



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q080** at [www.euroimmun.com](http://www.euroimmun.com)



# Molecular genetics

ApoE · F V / II / MTHFR · HLA-B27 · HLA-B57:01 · HLA-Cw6 · HLA-DQ2/8 · HFE · LCT



For more information on this subject scan the QR code or enter the Quick Link code **q150** at [www.euroimmun.com](http://www.euroimmun.com)

## Lactose intolerance (LCT gene) and hereditary fructose intolerance

■ **Clinical information: Primary lactose intolerance** is based on a genetically caused deficiency in the intestinal enzyme lactase, which is responsible for breaking down lactose into glucose and galactose. Unbroken lactose is fermented by bacteria in the ileum and colon. The resulting fermentation products lead to digestive problems and typical symptoms of lactose intolerance. These include abdominal pain, nausea, meteorism and diarrhoea. In the long term, primary lactose intolerance can lead to deficiencies and, as a result, unspecific symptoms such as fatigue, chronic fatigue and depression. Around 20% of Europeans and almost 100% of the entire population in many parts of Asia and in southern Africa suffer from primary lactose intolerance. However, mutations leading to a constantly increased lactase production and thus to lactose tolerance (lactase persistence) have also been observed.

The two most frequent mutations associated with primary lactose intolerance are the polymorphisms 13910 C/T and 22018 G/A, which are located in the promotor region of the lactase (LCT) gene. According to the current state of knowledge, 13910 C/C and 22018 G/G homozygous carriers develop symptoms of lactose intolerance, while 13910 C/T and 22018 G/A heterozygous carriers only have symptoms in case of stress or intestinal infection. 13910 T/T and 22018 A/A homozygous carriers are lactase persistent and show no symptoms at all. In addition to genetic lifelong primary lactose intolerance (with a lactase activity of less than 50%), there is also secondary lactose intolerance, which generally disappears after several months. Differentiation and clarification of the exact cause of the disorders is essential for patients. Secure and exact diagnosis requires a genetic diagnostic test in addition to the evaluation of the clinical symptoms.

**Hereditary fructose intolerance (HFI)** is a rare, autosomal recessive inherited metabolic disorder that is caused by mutations in the aldolase B gene (ALDOB gene). The four most frequent mutations in Europe lead to the amino acid replacements A149P, A174D and N334K as well as to the formation of premature stop codons (del4E4). For manifest HFI both alleles must be affected. Aldolase B is an enzyme that is essential for fructose metabolism and is located predominantly in the liver cells. It catalyses the decomposition of fructose 1 phosphate (F-1-P) to dihydroxyacetone phosphate and glyceraldehyde. If the enzyme is defect, F-1-P accumulates and, due to its toxicity, causes nausea, vomiting and gastrointestinal complaints in combination with indigestion and, in the long term, liver damage. Indirectly, gluconeogenesis and glycogen decomposition are inhibited, which may result in severe hypoglycaemia with shaking, sweating, pallor, lethargy and cramps and, in the worst case, in death.

HFI should be clinically differentiated from the much more frequent intestinal fructose intolerance (also called fructose malabsorption; prevalence ~30%). Fructose malabsorption is generally diagnosed by means of the hydrogen breath test. First, a defined amount of fructose is taken up by the patient, then the H<sub>2</sub> concentration in



the breath is measured. However, in case of HFI, administration of fructose-containing food may lead to a severe hypoglycaemic reaction. There, before carrying out a hydrogen breath test, the patient should be investigated for HFI using a molecular genetic test.

■ **Diagnostics:** The **EUROArray Lactose/Fructose Intolerance Direct** test was designed specifically for reliable determination of the most important genetic risk factors of primary lactose intolerance and HFI and is extremely easy to perform. With the unique direct procedure, the DNA no longer needs to be isolated. The blood sample is treated with two extraction reagents and can then be used directly in the PCR. The PCR primers and microarray probes have been carefully selected so that the polymorphisms 13910 C/T and 22018 G/A or mutations A149P, A174D, N334K and del4E4 are clearly identified. Data analysis, data interpretation and archiving are fully automated using the **EUROArrayScan Software**. When a positive result is obtained, the system differentiates between homozygous and heterozygous mutations. The EUROArray Lactose/Fructose Intolerance Direct ensures a high result security even for rare genotypes. For this purpose, the test system comes with unique controls that indicate whether the investigated DNA contains further known mutations in direct proximity to the sequence variants being analysed which may affect the binding to the probes and compromise the detection.

## Product overview

Parameter	Sample material	Application	Order number	Page
Lactose/Fructose Intolerance Direct	Whole blood/ genomic DNA	Molecular genetic in vitro determination of the most relevant single nucleotide polymorphisms in the LCT gene or point mutations in the aldolase B gene in human genomic DNA for the diagnosis of primary lactose intolerance and/or hereditary fructose intolerance	MN 5350-####-V	300
Lactose Intolerance Direct	Whole blood/ genomic DNA		MN 5351-####-V	300
Fructose Intolerance Direct	Whole blood/ genomic DNA		MN 5352-####-V	300



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q080** at [www.euroimmun.com](http://www.euroimmun.com)



# Molecular infection diagnostics

Dermatophytosis · HPV · GynTect · STI · SARS-CoV-2 · Zika Virus · Tuberculosis



For more information on this subject scan the QR code or enter the Quick Link code **q158** at [www.euroimmun.com](http://www.euroimmun.com)

## Dermatophytosis

■ **Clinical information:** Dermatophytoses are infections of the skin, hair and nails, which are caused in most cases by dermatophytes, and in rarer cases by yeasts and moulds. The dermatophytes encompass fungi of the genera *Trichophyton*, *Epidermophyton*, *Nannizzia*, *Paraphyton*, *Lophophyton*, *Microsporum* and *Arthroderma*. Depending on the main host or transmission route, dermatophytes are divided into anthropophilic (humans), zoophilic (animals) and geophilic (soil) species. Human pathogenic yeasts and moulds include *Candida spec.*, *Scopulariopsis brevicaulis*, *Fusarium spec.* and *Aspergillus fumigatus*.

Fungal infections of the skin are the most frequently occurring infectious diseases with high relapse rates. Worldwide, approximately 20 to 25% of the population is affected by fungal skin diseases. Around 70% of all human dermatophyte infections are caused by anthropophilic species. Zoophilic dermatophytes often cause severe inflammatory reactions in humans. The transmission of zoophilic dermatophytes to humans occurs via close contact, especially with pets, which are often asymptomatic carriers. Geophilic dermatophytes less frequently cause disease in humans. Contact with e.g. *Nannizzia gypsea*, however, can lead to infections on the hands and arms in gardeners or farm workers.

The clinical image of dermatophytoses is very heterogeneous and cannot always be differentiated from other dermatoses, such as eczema, psoriasis, erysipelas, or autoimmune diseases. Further, a simultaneous bacterial infection, pretreatment with corticosteroid-containing preparations or secondary contact allergy can hinder identification of dermatophytoses. Dermatophytoses must always be treated. Before starting therapy, a positive pathogen detection result should be present. This allows the different activity spectra of antifungal drugs to be taken into account and the oftentimes lengthy therapy to be designed in the most effective way.

■ **Diagnostics:** Standard laboratory diagnostics of dermatophytoses encompass the microscopic detection of fungus and the attempt to culture the pathogen from clinical material. Culturing is generally time-consuming and may be hindered by antimycotic therapy started before taking the sample. Especially in mixed infections, false diagnoses are often made based on culture methods, since slowly growing species are overlooked or overgrown by other pathogens in the sample.

The EUROArray Dermatophytosis combines a multiplex PCR with a microarray and enables detection of up to 50 dermatophytes as well as clear species identification of up to 23 dermatophytes and 6 yeasts/moulds in one reaction. The detection is highly specific and sensitive, even after the start of therapy, and offers a huge time advantage over detection by culture. The EUROArray Dermatophytosis thus contributes significantly to improved identification of dermatophytosis pathogens and finding the respective specific treatment. It also aids quick determination of the infection source.



The EUROArray Dermatomycosis offers fast, reliable and precise detection of dermatophytes, yeasts and moulds. The test is very easy to perform – no in-depth molecular biology knowledge is required. Data analysis, data interpretation and archiving are fully automated using EUROArrayScan software.

## Product overview

Parameter	Sample material	Application	Order number	Page
Dermatomycosis	DNA	PCR-based molecular genetic direct detection of up to 50 dermatophytes and clear species identification of up to 23 dermatophytes and 6 yeasts/moulds	MN 2850-####	302



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g080** at [www.euroimmun.com](http://www.euroimmun.com)



# Molecular infection diagnostics

Dermatomycosis · HPV · GynTect · STI · SARS-CoV-2 · Zika Virus · Tuberculosis



For more information on this subject scan the QR code or enter the Quick Link code **q136** at [www.euroimmun.com](http://www.euroimmun.com)

## Human papillomavirus

■ **Clinical information:** Genital human papillomaviruses (HPV) are the most frequently sexually transmitted viruses. The prevalence of HPV in Europe amounts to 8% to 15%. Worldwide, it is estimated to be 2% to 45%, varying considerably between the different age and population groups in each country. HPV only infect epithelial cells, where they replicate in the cell nuclei. HPV can cause unregulated tumour-like growth of the host cells, which can be either benign, with warts forming at the site of infection, or malignant, especially resulting in cervical carcinoma.

So far, 30 genital HPV types have been described. They are divided into two groups according to their oncogenic potential: high-risk and low-risk HPV. While high-risk HPV are involved in the development of carcinoma and can be detected in over 99% of cervical carcinomas, low-risk HPV alone are only found in non-malignant tissue changes. The WHO has officially classified genotypes 16, 18, 31, 33, 35, 39, 45, 51, 52, 56, 58, 59 and 66 as oncogenic and thus as high-risk HPV. HPV 16 can be detected in 50 to 60% and HPV 18 in 10 to 20% of cervical carcinomas. However, other HPV, such as 26, 53, 68, 73 and 82 have also been found in cervical carcinoma and should therefore also be considered as high-risk HPV. Low-risk viruses include HPV 6 and 11, the main causative agents of genital warts (*Condylomata acuminata*, fig warts). Further low-risk types are 40, 42, 43, 44, 54, 61, 70, 72, 81 and 89 (CP6108). Although infections with low-risk HPV are not potentially lethal, the consequences of the infection, e.g. benign genital warts, can represent a physical and mental impairment for the patient. In Germany, around 1% of people between 15 and 49 years of age are affected.

For assessment of the course of HPV infection and the risks involved it is not only important to differentiate between high-risk and low-risk viruses but also to discriminate between the different viruses in the high-risk group.

■ **Diagnostics:** Alongside cytology (Pap smear), direct detection methods for HPV play a very important role in the early diagnosis of cervical carcinoma. They are based on the detection of viral DNA, mainly using PCR, or the detection of viral RNA produced by the host cells. Whereas the Pap smear is used to investigate cervical cells for pathological changes, a PCR-based test is able to detect an HPV infection before morphological cell changes have occurred.

While HPV tests based on conserved genes require only a few primer systems, the detection of the oncogenes E6/E7, which vary considerably in the different HPV, is much more complex. The disadvantage of using conserved genes for HPV detection is that the genes may be lost during integration of viral DNA into the host DNA. PCR systems based on these sequences can therefore lead to false negatives despite viral DNA being present. The **EUROArray HPV** is based on the detection of the oncogenes E6/E7 and thus provides the highest possible sensitivity even after integration of the virus DNA into the host DNA.



The use of subtype-specific primer systems and probes in the **EUROArray HPV** allows the detection and typing of all 30 relevant genital HPV in one test run – namely 18 high risk HPV (16, 18, 26, 31, 33, 35, 39, 45, 51, 52, 53, 56, 58, 59, 66, 68, 73, 82) and 12 low risk HPV (6, 11, 40, 42, 43, 44, 54, 61, 72, 81, 89, 70). The **EUROArray HPV** is easy to perform in comparison to other molecular biological methods – no in-depth molecular biology knowledge is required. Data analysis, data interpretation and archiving are fully automated using the **EUROArrayScan software**.

## Product overview

Parameter	Sample material	Application	Order number	Page
Human papillomavirus (HPV)	DNA	PCR-based direct detection of human papillomaviruses (HPV), which are involved in the development of neoplasms, in particular cervical carcinoma	MN 2540-####	302



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q080** at [www.euroimmun.com](http://www.euroimmun.com)





# Molecular infection diagnostics

Dermatomycosis · HPV · GynTect · STI · SARS-CoV-2 · Zika Virus · Tuberculosis



For more information on this subject scan the QR code or enter the Quick Link code **q174** at [www.euroimmun.com](http://www.euroimmun.com)

## GynTect<sup>®</sup> – cervical cancer test

■ **Clinical information:** An increasing number of countries are changing their **cervical cancer screening** from cytological examinations to HPV screening tests, or a combination of both, at longer intervals. However, only few HPV infections actually lead to lesions that develop into cancer. The majority are overcome by the immune system.

As a result of this new screening strategy, however, **more and more women are being confronted with a positive test result**, which in turn can cause great fear of having cancer. Since conventional screening methods have no prognostic value, there is no way to predict whether an HPV infection will develop into cancer. For this reason, standard screening often leads to unnecessary treatment, including costly surgical procedures that can cause preterm births or miscarriages in women of reproductive age during an existing or subsequent pregnancy. In addition, an inaccurate diagnosis leads to unnecessarily lengthy and intensive monitoring, which is often accompanied by psychological stress for the patient.

■ **Diagnostics:** The GynTect<sup>®</sup> test was developed for improved patient management in cervical cancer screening. It is used to specifically **detect changes in DNA methylation that affect six specific genes** (ASTN1, DLX1, ITGA4, RXFP3, SOX17, ZNF671) **and occur in the development of cervical cancer**. The test can therefore be used to distinguish HPV infections that cause cervical cancer from those that do not and therefore do not require treatment. Accordingly, the GynTect<sup>®</sup> test is much more specific for high-grade lesions than HPV tests and is an excellent way to determine whether a colposcopy or treatment is needed following a positive HPV test result.

**In general, the GynTect<sup>®</sup> test is particularly suitable for women with a positive (HPV) or abnormal (cytology) cervical cancer screening result who are**

- pregnant or would like to conceive
- prefer a non-invasive diagnostic procedure
- want to avoid long monitoring or waiting times for the result of a confirmatory test or
- prefer to continue treatment with their gynaecologist rather than being referred directly to a specialist.

**Sales restrictions:** This test is only available in Canada, Italy, Poland, Portugal and Turkey.



## Product overview

Method/Parameter	Sample material	Application	Order number	Page
GynTect® DNA Methylation test	Bisulphite-converted DNA	PCR-based detection of methylated DNA regions that occur specifically in cervical cancer and its precancerous stages, but not in healthy cervical tissue	MN 254a-####	302



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g080** at [www.euroimmun.com](http://www.euroimmun.com)



# Molecular infection diagnostics

Dermatomycosis · HPV · GynTect · STI · SARS-CoV-2 · Zika Virus · Tuberculosis



For more information on this subject scan the QR code or enter the Quick Link code **q143** at [www.euroimmun.com](http://www.euroimmun.com)

## STI – Sexually transmitted infections

■ **Clinical significance:** Infections with sexually transmitted pathogens, in particular Chlamydia, Neisseria, Mycoplasma, Ureaplasma and Trichomonas, often lead to inflammation of the urogenital tract. Untreated, they may ascend and eventually lead to infertility. Some pathogens, e.g. *Treponema pallidum*, can spread in the whole body and eventually lead to death. Infections with sexually transmitted pathogens often proceed asymptotically in the early stage, so that they may remain undetected and only become obvious when they have turned chronic. Infections with the herpes simplex viruses (HSV) -1 and -2 persist lifelong, but only show in acute breakouts by formation of blisters in the facial/labial or genital area. In severe courses they may even lead to encephalitis or meningitis.

In addition to the direct consequences for the patient, infections with most of the above pathogens during pregnancy can lead to intrauterine death, premature birth or damage to the foetus. Moreover, many pathogens can be transmitted to the newborn during birth, causing severe postnatal infections. Herpes virus infections in newborns may lead to neonatal herpes encephalitis or disseminated forms which are associated with high mortality rates.

■ **Diagnostics:** The methods which are commonly used for detection of infections with sexually transmitted pathogens encompass culturing, indirect detection by determination of pathogen-specific antibodies and direct detection, in which the pathogen itself is detected immunologically or by means of PCR. Since detection by culturing is especially time-consuming or even impossible for Chlamydia, Mycoplasma, Ureaplasma and Treponema, use of other detection methods, e.g. PCR-based procedures, is generally recommended or required.

The **EUROArray STI-11** enables simultaneous detection of 11 sexually transmitted pathogens in one reaction: *Chlamydia trachomatis*, *Neisseria gonorrhoeae*, HSV-1 and -2, *Haemophilus ducreyi*, *Mycoplasma genitalium* and *hominis*, *Treponema pallidum*, *Trichomonas vaginalis*, and *Ureaplasma parvum* and *urealyticum*. Timely detection of these pathogens and subsequent targeted treatment can prevent consequential damage, which can lead to severe chronic diseases or infertility. The detection using the EUROArray STI-11 is highly specific and sensitive and significantly faster than determination by culture. Moreover, the combined detection of these pathogens with the EUROArray STI-11 is especially useful for clarifying ambiguous clinical findings, identifying asymptomatic infections in pregnancy care, and identifying multiple infections with different sexually transmitted pathogens. The EUROArray STI-11 therefore contributes substantially to improving diagnosis of sexually transmitted infections.

The data analysis, interpretation and archiving for the EUROArray STI-11 are fully automated by the **EUROArrayScan software**. There are different EUROArray STI test systems available for the detection of different pathogen combinations, also of smaller pathogen ranges, so that the determination can be performed according to the individual requirements (see table).



The **EURORealTime HSV-1/2** test allows highly specific and sensitive detection of HSV-1 and/or HSV-2 as well as quantification of viral DNA by means of real-time PCR. It is suitable both for early diagnosis of HSV-1 and HSV-2 infections and differentiation of the two virus types. Analysis of raw data, evaluation, report generation and archiving are fully automated by means of the **EURORealTime Analysis Software**. The standard curves used for automatic quantification of the viral load can be saved in the software and, if required, used again in future runs.

## Product overview

Method / Parameter	Sample material	Application	Order number	Page
EUROArray STI - 11	DNA	PCR-based direct detection of <i>C. trachomatis</i> , <i>N. gonorrhoeae</i> , HSV-1, HSV-2, <i>H. ducreyi</i> , <i>M. genitalium</i> , <i>M. hominis</i> , <i>T. pallidum</i> , <i>T. vaginalis</i> , <i>U. parvum</i> and <i>U. urealyticum</i>	MN 2830-####	302
EUROArray STI - 7	DNA	PCR-based direct detection of <i>H. ducreyi</i> , <i>M. genitalium</i> , <i>M. hominis</i> , <i>T. pallidum</i> , <i>T. vaginalis</i> , <i>U. parvum</i> and <i>U. urealyticum</i>	MN 2830-####-1	302
EUROArray STI - CT/NG	DNA	PCR-based direct detection of <i>C. trachomatis</i> and <i>N. gonorrhoeae</i>	MN 2830-####-2	302
EUROArray HSV1/2 VZV	DNA	PCR-based direct detection of HSV-1, HSV-2 and varicella zoster virus	MN 2530-####-1	302
EURORealTime HSV-1/2	DNA	Real-time PCR-based quantitative direct detection of HSV-1 and HSV-2	MP 2530-0125	303



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g080** at [www.euroimmun.com](http://www.euroimmun.com)



# Molecular infection diagnostics

Dermatomycosis · HPV · GynTect · STI · SARS-CoV-2 · Zika Virus · Tuberculosis



For more information on this subject scan the QR code or enter the Quick Link code **q168** at [www.euroimmun.com](http://www.euroimmun.com)

## SARS-CoV-2

■ **Clinical significance:** Severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2, previously called 2019-nCoV) belongs to the family of coronaviruses and, like SARS-CoV, is classified in the genus *Betacoronavirus*. At the end of 2019, SARS-CoV-2 caused an infection wave which quickly spread worldwide and was declared a pandemic by the WHO in March 2020. Just a few days after the first report about patients with pneumonia of unclear origin, SARS-CoV-2 was identified as the causative pathogen and the associated disease named COVID-19.

SARS-CoV-2 is mainly transmitted via aerosols during speaking, breathing, coughing or sneezing or at close contact with an infected person. The incubation period is usually three to seven, maximally 14 days. The symptoms and severity of SARS-CoV-19 infection can vary significantly. The most common symptoms encompass fever, coughing, breathing difficulties and fatigue. Therefore, in the majority of patients, the infection resembles a cold with light fever, with irregular lung infiltrates. Some patients, especially older and chronically ill persons, develop severe acute respiratory distress syndrome.

■ **Diagnostics:** Suitable methods for the diagnosis of SARS-CoV-2 infections are the detection of viral RNA by reverse transcriptase polymerase chain reaction (RT-PCR) or of virus protein by means primarily in sample material from the upper (nasopharyngeal or oropharyngeal swab) or lower respiratory tract (bronchoalveolar lavage fluid, tracheal secretion, sputum, etc.). The RT-PCR allows detection of the pathogen even in subclinical or asymptomatic courses already few days after virus contact and up to 14 days after onset of possible symptoms.

The EURORealTime-SARS-CoV-2 test enables highly specific and sensitive direct detection of SARS-CoV-2 by reverse-transcriptase real-time PCR. Reverse transcription, amplification and detection of the SARS-CoV-2 cDNA are performed in a single test. For differential diagnostics of symptoms which can be associated with COVID-19 as well as influenza, EUROIMMUN offers a combined tests for the parameters SARS-CoV-2, influenza virus type A and influenza virus type B: EURORealTime SARS-CoV-2/Influenza A/B. Optionally, the analysis of raw data, interpretation of data, generation of result reports and archiving of results including all internal and external controls, can be completely automated via the EURORealTime Analysis software. The required data processing steps are thus significantly simplified and accelerated. The software also provides convenient guidance through the entire work procedure, thus preventing errors. The software also provides convenient guidance through the entire work procedure, thus preventing the occurrence of errors.

Moreover, EUROIMMUN's product portfolio for COVID-19 diagnostics encompasses serological tests for differentiated detection of antibodies of different immunoglobulin classes and against different SARS-CoV-2 antigens, an antigen ELISA for acute diagnostics and an interferon gamma release assay (IGRA) to measure the cellular immune response.



## Product overview

Method / parameter	Sample material	Application	Order number	Page
EURORealTime SARS-CoV-2	RNA from throat swabs or saliva	Real-time PCR-based direct detection of SARS-CoV-2	MP 2606-####	303
EURORealTime SARS-CoV-2/Influenza A/B	RNA from throat swabs	Real-time PCR-based direct detection of SARS-CoV-2, influenza virus type A and influenza virus type B	MP 2606-20-####	303

Further serological products see page 177



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q168** at [www.euroimmun.com](http://www.euroimmun.com)



# Molecular infection diagnostics

Dermatomycosis · HPV · GynTect · STI · SARS-CoV-2 · Zika Virus · Tuberculosis



For more information on this subject scan the QR code or enter the Quick Link code **q147** at [www.euroimmun.com](http://www.euroimmun.com)

## Zika Virus

■ **Clinical significance:** Zika virus (ZIKV) is an arbovirus of the *Flaviviridae* family. The virus is generally transmitted by mosquitos of the genus *Aedes*. Transmission via sexual intercourse has also been reported in individual cases. The virus was first observed in African countries. In recent years, however, large outbreaks also occurred in tropical and subtropical regions in Asia, on islands in the Pacific and in Latin America.

The disease course is usually mild. The symptoms are near-to identical to those of dengue or chikungunya virus infections. After an incubation time of five to ten days a flu-like illness develops with fever, rash, arthralgia, myalgia, headache and conjunctivitis. Moreover, an increase in neurological diseases such as Guillain-Barré syndrome was registered following infections with ZIKV. Furthermore, pregnant women infected with ZIKV can transmit the virus to the foetus. In this case, the virus may impair the brain development and cause severe malformations of the brain as well as microcephaly. There is no specific treatment for ZIKV infections as yet. Protection from mosquito bites serves as a preventative measure. A vaccine is not available.

■ **Diagnostics:** The RNA genome of ZIKV can be directly detected in serum approximately five days after the onset of symptoms and in urine up to ten days by means of polymerase chain reaction (PCR). Specific antibodies against ZIKV, in contrast, are first detected several days after onset of symptoms. Therefore, direct detection of ZIKV RNA plays an important role especially in early stages of the infection, while serological antibody detection is especially relevant for the diagnosis of infections at later stages. By using RNA-based detection, ZIKV infections can be clearly distinguished from infections with related viruses, such as dengue or chikungunya virus, which cause similar symptoms and are endemic in the same regions.

The **EURORealTime Zika Virus** test provides highly specific and sensitive direct detection of ZIKV by means of reverse transcriptase real-time PCR. Reverse transcription, amplification, and detection of ZIKV cDNA take place in a single reaction. As an option, raw data analysis, interpretation of data, creation of reports and archiving of results, taking into account all internal and external controls, can also be performed fully automatically by the **EURORealTime Analysis Software**. The required data processing steps are thus significantly simplified and accelerated. Moreover, the software conveniently guides the user through the entire workflow, helping to prevent mistakes.

EUROIMMUN offers the complete range of test systems for specific detection of ZIKV infections, both for direct detection by real-time PCR and serological detection of specific antibodies.





## Product overview

Method/parameter	Sample material	Application	Order number	Page
EURORealTime Zika Virus	RNA from serum and urine	Real-time PCR-based direct detection of Zika virus	MP 2668-####	303
<b>Further serological products</b>				
Method	Substrate	Application	Order number	Page
ELISA	Recombinant non- structural protein (NS1) from Zika virus	Highly specific detection of Zika virus infections	EI 2668-9601 A/G/M	201
IFT	Arbovirus Fever Mosaic 2: Zika virus, chikungunya virus, dengue virus	For differential diagnosis of arbovirus infections, in parti- cular ZIKV, DENV and CHIKV	FI2668-####-1 G/M	211



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **g080** at [www.euroimmun.com](http://www.euroimmun.com)



# Molecular infection diagnostics

Dermatomycosis · HPV · GynTect · STI · SARS-CoV-2 · Zika Virus · Tuberculosis



For more information on this subject scan the QR code or enter the Quick Link code **q167** at [www.euroimmun.com](http://www.euroimmun.com)

## Tuberculosis

■ **Clinical significance:** Tuberculosis is among the most frequent infectious diseases worldwide alongside malaria and AIDS. According to estimations of the WHO, there are 10 million new infections and 1.8 million deaths each year.

Tuberculosis is caused by bacteria of the *Mycobacterium tuberculosis* complex (MTBC). This complex encompasses eight different mycobacteria, of which seven have been described to cause tuberculosis in humans and animals. Most of the cases are caused by *M. tuberculosis*.

Tuberculosis bacteria are transmitted primarily by inhalation of infectious droplets, which are emitted into the air as aerosols by patients with open pulmonary tuberculosis through coughing and speaking. Therefore, primary infections in most cases lead to pulmonary tuberculosis. In rare cases, primary tuberculosis also affects other organs such as the skin or the digestive tract. Only 5 to 10% of the infected persons develop active tuberculosis; in immunocompetent persons, a large share of the infections is asymptomatic. Latent infections may persist over decades and be reactivated when the immune system is weakened.

■ **Diagnostics:** Microbiological tuberculosis diagnostics are often challenging, especially in the initial stage. Therefore, it is particularly important to apply all available diagnostic methods if there is a suspicion of tuberculosis in order to recognise it, heal it, and break the reaction chain. Fast and sensitive direct detection of tuberculosis pathogen DNA in sputum, bronchoalveolar lavage fluid and bronchial secretion optimally supplements microscopy and time-intensive detection by culture (six to eight weeks).

The EURORealTime MTB test enables highly specific and reliable detection of MTBC by real-time PCR. The detection of a total of three MTBC-specific target regions ensures particularly sensitive diagnostics. Optionally, analysis of raw data, data interpretation, generation of result reports and archiving of results, taking into account all internal and external controls, can be completely automated using the EURORealTime Analysis software. In this way, the required data processing steps are significantly simplified and accelerated. The software also provides convenient guidance through the entire work procedure, thus preventing errors.



## Product overview

Method/parameter	Sample material	Application	Order number	Page
EURORealTime MTB	DNA from sputum, bronchial lavage fluid or bronchial secretion	Real-Time PCR-based direct detection of the <i>M. tuberculosis</i> complex	MP 2145-####	303



To view all EUROIMMUN products for this subject scan the QR code or enter the Quick Link code **q167** at [www.euroimmun.com](http://www.euroimmun.com)



# Products for molecular genetic diagnostics

Molecular genetic  
diagnostics





### Format

- 0803: 8 slides with 3 fields each
- 0505: 5 slides with 5 fields each
- 1005: 10 slides with 5 fields each
- 2005: 20 slides with 5 fields each

**MN** **5110** - **2005** - **V**

### Sample material

V: Whole blood

### Product code

### Product classification

- MN: Test system EUROArray (molecular genetic determinations)..... page 300
- MN: Test system EUROArray (molecular infectious diagnostics)..... page 302
- MC: Control EUROArray (molecular infectious diagnostics)..... page 302
- MP: Test system EURORealTime PCR (molecular infectious diagnostics) ..... page 303

Molecular genetic diagnostics

For product orders the amount, product code and test name are required. **Test kits** comprise all reagents needed to perform the investigation.


**EUROArray for Molecular Genetic Determinations (Test Systems)**

Order No.	Description	Format
MN 5110-0803-V MN 5110-0505-V MN 5110-1005-V MN 5110-2005-V	<b>EUROArray HLA-B27 Direct</b>	08 x 03 05 x 05 10 x 05 20 x 05
MN 5150-0803 * MN 5150-0505 * MN 5150-1005 * MN 5150-2005 *	<b>EUROArray HLA-DRB1 Shared Epitope</b>	08 x 03 05 x 05 10 x 05 20 x 05
MN 5210-0803-V MN 5210-0505-V MN 5210-1005-V MN 5210-2005-V	<b>EUROArray HLA-B57:01 Direct</b>	08 x 03 05 x 05 10 x 05 20 x 05
MN 5320-0803-V MN 5320-0505-V MN 5320-1005-V MN 5320-2005-V	<b>EUROArray HLA-DQ2/DQ8-h Direct</b>	08 x 03 05 x 05 10 x 05 20 x 05
MN 5321-0803-V MN 5321-0505-V MN 5321-1005-V MN 5321-2005-V	<b>EUROArray HLA-DQ2/DQ8 Direct</b>	08 x 03 05 x 05 10 x 05 20 x 05
MN 5350-0803-V MN 5350-0505-V MN 5350-1005-V MN 5350-2005-V	<b>EUROArray Lactose/Fructose Intolerance Direct</b>	08 x 03 05 x 05 10 x 05 20 x 05
MN 5351-0803-V MN 5351-0505-V MN 5351-1005-V MN 5351-2005-V	<b>EUROArray Lactose Intolerance Direct</b>	08 x 03 05 x 05 10 x 05 20 x 05
MN 5352-0803-V MN 5352-0505-V MN 5352-1005-V MN 5352-2005-V	<b>EUROArray Fructose Intolerance Direct</b>	08 x 03 05 x 05 10 x 05 20 x 05
MN 5410-0803-V MN 5410-0505-V MN 5410-1005-V MN 5410-2005-V	<b>EUROArray HLA-Cw6 Direct</b>	08 x 03 05 x 05 10 x 05 20 x 05
MN 5520-0803-V MN 5520-0505-V MN 5520-1005-V MN 5520-2005-V	<b>EUROArray Haemochromatosis (4 SNP+) Direct</b>	08 x 03 05 x 05 10 x 05 20 x 05
MN 5521-0803-V MN 5521-0505-V MN 5521-1005-V MN 5521-2005-V	<b>EUROArray Haemochromatosis (2 SNP+) Direct</b>	08 x 03 05 x 05 10 x 05 20 x 05
MN 5710-0803-V MN 5710-0505-V MN 5710-1005-V MN 5710-2005-V	<b>EUROArray APOE Direct</b>	08 x 03 05 x 05 10 x 05 20 x 05
MN 5820-0803-V MN 5820-0505-V MN 5820-1005-V MN 5820-2005-V	<b>EUROArray FV / FII+ / MTHFR Direct</b>	08 x 03 05 x 05 10 x 05 20 x 05

\* For research use only, not for in vitro diagnostic use in the sense of EU directive 98/79/EC.



## EUROArray for Molecular Genetic Determinations (Test Systems)

Order No.	Description	Format
MN 5821-0803-V	EUROArray FV / FII+ Direct	08 x 03
MN 5821-0505-V		05 x 05
MN 5821-1005-V		10 x 05
MN 5821-2005-V		20 x 05
MN 5822-0803-V	EUROArray FV Leiden Direct	08 x 03
MN 5822-0505-V		05 x 05
MN 5822-1005-V		10 x 05
MN 5822-2005-V		20 x 05
MN 5823-0803-V	EUROArray FII+ Direct	08 x 03
MN 5823-0505-V		05 x 05
MN 5823-1005-V		10 x 05
MN 5823-2005-V		20 x 05
MN 5824-0803-V	EUROArray MTHFR Direct	08 x 03
MN 5824-0505-V		05 x 05
MN 5824-1005-V		10 x 05
MN 5824-2005-V		20 x 05




**EUROArray for Molecular Infectious Diagnostics (Test Systems)**

Order No.	Description	Format
MN 2530-0803-1	<b>EUROArray HSV1/2 VZV</b>	08 x 03
MN 2530-0505-1		05 x 05
MN 2530-1005-1		10 x 05
MN 2530-2005-1		20 x 05
MN 2540-0803	<b>EUROArray HPV</b>	08 x 03
MN 2540-0505		05 x 05
MN 2540-1005		10 x 05
MN 2540-2005		20 x 05
MN 2830-0803	<b>EUROArray STI - 11</b>	08 x 03
MN 2830-0505		05 x 05
MN 2830-1005		10 x 05
MN 2830-2005		20 x 05
MN 2830-0803-1	<b>EUROArray STI - 7</b>	08 x 03
MN 2830-0505-1		05 x 05
MN 2830-1005-1		10 x 05
MN 2830-2005-1		20 x 05
MN 2830-0803-2	<b>EUROArray STI - CT/NG</b>	08 x 03
MN 2830-0505-2		05 x 05
MN 2830-1005-2		10 x 05
MN 2830-2005-2		20 x 05
MN 2830-0803-3	<b>EUROArray STI - CT/NG/TP/TV</b>	08 x 03
MN 2830-0505-3		05 x 05
MN 2830-1005-3		10 x 05
MN 2830-2005-3		20 x 05
MN 2830-0803-4	<b>EUROArray STI - 6</b>	08 x 03
MN 2830-0505-4		05 x 05
MN 2830-1005-4		10 x 05
MN 2830-2005-4		20 x 05
MN 2830-0803-5	<b>EUROArray STI - HSV-1/2</b>	08 x 03
MN 2830-0505-5		05 x 05
MN 2830-1005-5		10 x 05
MN 2830-2005-5		20 x 05
MN 2850-0803	<b>EUROArray Dermatomycosis</b>	08 x 03
MN 2850-0505		05 x 05
MN 2850-1005		10 x 05
MN 2850-2005		20 x 05

**EUROArray for Molecular Infectious Diagnostics (Controls)**

Order No.	Description	Format
MC 2540-0506	<b>EUROArray HPV positive control</b>	5 x 0.06 ml (0.3 ml)


**EURORealTime PCR for Molecular Infectious Diagnostics (Test Systems)**

Order No.	Description	Format
MP 2145-0125 MP 2145-0225 MP 2145-0425	<b>EURORealTime MTB</b>	25 reactions 50 reactions 100 reactions
MP 2530-0125 MP 2530-0225 MP 2530-0425	<b>EURORealTime HSV-1/2</b>	25 reactions 50 reactions 100 reactions
MP 2606-0125 MP 2606-0225 MP 2606-0100 MP 2606-0425 MP 2606-0200 MP 2606-1000	<b>EURORealTime SARS-CoV-2</b>	25 reactions 50 reactions 100 reactions 100 reactions 200 reactions 1000 reactions
MP 2606-0125-20 MP 2606-0225-20 MP 2606-0100-20 MP 2606-0425-20 MP 2606-0200-20 MP 2606-1000-20	<b>EURORealTime SARS-CoV-2/Influenza A/B</b>	25 reactions 50 reactions 100 reactions 100 reactions 200 reactions 1000 reactions
MP 2668-0125 MP 2668-0225 MP 2668-0425	<b>EURORealTime Zika Virus</b>	25 reactions 50 reactions 100 reactions



# Additional reagents and material



ZF 1020 - 0125 -2

Product code

**Product classification**

- ZD: Reagents and other items for EUROIMMUN Westernblot and EUROLINE..... page 306
- ZM: Reagents and other items for EUROArray..... page 307


**Reagents and Other Items for EUROIMMUN Westernblot and EUROLINE**

Order No.	Item	Format
ZD 1129-0101 A	secondary reagents EUROLINE/Westernblot IgA	1 reagent kit
ZD 1129-0101 E	secondary reagents EUROLINE allergy IgE	1 reagent kit
ZD 1129-0101 G	secondary reagents EUROLINE/Westernblot IgG	1 reagent kit
ZD 1129-0101 M	secondary reagents EUROLINE/Westernblot IgM	1 reagent kit
ZD 3001-0101 ZD 3001-0401	anti-CCD absorbent	lyophilisate, for 40 µg 4 x lyophilisate, for 40 µg
ZD 9880-0101 ZD 9880-01500	Green paper (EUROLiScan)	
ZD 9885-0116 ZD 9885-0130	adhesive foil	1 piece á 7,5 x 12,5 cm 1 piece á 12,5 x 19,9 cm
ZD 9895-0130 ZD 9895-20030	incubation tray, black	1 piece, 30 channels 200 pieces, 30 channels
ZD 9897-0130 ZD 9897-0144 ZD 9897-12044 ZD 9897-20030 ZD 9897-70010	incubation tray, black for the volume-reduced incubation of allergy EUROLINE test strips	1 piece, 30 channels 1 piece, 44 channels 120 pieces, 44 channels 200 pieces, 30 channels 700 pieces, 10 channels
ZD 9898-0144 ZD 9898-0148 ZD 9898-3044 ZD 9898-20048	incubation tray, black	1 piece, 44 channels 1 piece, 48 channels 30 pieces, 44 channels 200 pieces, 48 channels
ZD 9899-0108 ZD 9899-10508	incubation tray, white	1 piece, 8 channels 1050 pieces, 8 channels



<b>Reagents and Other Items for EUROArray</b>		
<b>Order No.</b>	<b>Item</b>	<b>Format</b>
ZM 0121-0050	WASH REAGENT 1	500 ml concentrate
ZM 0122-0012	WASH REAGENT 2	125 ml concentrate
ZM 0123-0101	EUROArray wash buffer set	1 set
ZM 0201-0150-Q	QIAamp DSP Blood Mini Kit	50 reactions
ZM 0202-0150-Q *	QIAamp Viral RNA Mini Kit	50 reactions
ZM 0203-0150-Q *	QIAamp DNA Mini Kit	50 reactions
ZM 0204-0110-Q *	EpiTect Fast Bisulfite Kit (QIAGEN) for 10 patient samples	10 samples
ZM 0210-1000-Q *	Qiagen Collection Tubes	1000 tubes
ZM 0221-0126-Q *	Qiagen Buffer AL	264 ml
ZM 0222-0450-Q *	Qiagen Buffer ATL	4 x 50 ml
ZM 0281-5001	Copan regular FLOQSwab with 1 ml eNAT transport and conservation medium (608CS01R)	50 Swabs
ZM 0282-5002	Copan L-shape FLOQSwab with 2 ml eNAT transport and conservation medium (606CS01L)	50 Swabs
ZM 0283-5001	Buccal hDNAfree FLOQSwab, Regular size tip, 20 mm Breaking Point, in tube with Active Drying System (50E010D01)	50 Swabs
ZM 9101-0168 *	Prepito NA EU Kit	168 reactions in one kit
ZM 9102-0960 *	Pre-NAT II NA EU Kit	960 reactions in one kit
ZM 9106-1100	chemagic Low Well Plates	100 plates per packaging unit
ZM 9107-1096	900 µL Cond Filter Tips	10 packs with 96 tips
ZM 9108-1096	175 µl Conduc Filter Tip	10 packs with 96 tips
ZM 9113-0101	chemagic Stands	1 piece
ZM 9999-0105	TITERPLANE reagent tray for EUROArray slides	1 piece

\* For research use only, not for in vitro diagnostic use in the sense of EU directive 98/79/EC.



# Index

1,25-Dihydroxy Vitamin D.....	256, 257, 262, 264, 265	BACE-1.....	245, 261
17-OH-progesterone.....	260	BAP.....	255, 262, 264, 265
25-OH vitamin D.....	256, 257, 260	Barmah forest virus.....	211
3alpha-adiol G.....	260	Bartonella.....	94, 209
ACE.....	264	Bechterew's disease.....	272, 273
Acetylcholine receptor.....	17, 129, 143, 150, 158	Beta-amyloid.....	244, 245, 260, 263
AChR.....	128, 129, 150, 158	BFV.....	211
ACTH.....	264, 265	Bile canaliculi.....	112
Adalimumab.....	146	Biliary ducts.....	112
Additional reagents and material.....	304	Bone metabolism.....	254
Adenovirus.....	201, 202	BoneTRAP.....	255, 262, 264, 265
Adiponectin.....	260	Bordetella.....	168, 192, 194, 197, 209
Adrenal cortex.....	90, 151	Borrelia.....	9, 20, 170, 171, 184, 185, 192, 193, 195-197, 204-206, 209
AIH.....	110, 111, 113	Borreliosis.....	170
Aldosterone.....	260, 264, 265	BP180.....	134
Allergy diagnostics.....	9, 26, 64, 66, 68, 82, 216, 224, 226, 227, 230-241	BP230.....	134
Alzheimer's disease.....	244, 268, 269	BPI.....	105, 143
AMA.....	30, 88, 89, 91-93, 96, 97, 111-113, 139-142, 145, 148, 156, 157, 160, 162-164	Brain.....	14, 126, 128, 151, 182, 184, 244, 270, 294
AMA M1.....	145	Brucella abortus.....	198
AMA M2.....	30, 88, 89, 139-142, 148		
AMPA.....	126, 127	Calcitonin.....	150, 256, 260
AMPA1.....	90, 153	Calprotectin.....	15, 116, 117, 252, 253, 261, 263-265
AMPA2.....	153	Campylobacter.....	197
Amphiphysin.....	88, 90, 96, 124-126, 128, 140, 151, 152	cANCA.....	90, 91, 96, 104, 143, 154-156
ANA..	14, 15, 54, 88, 91-93, 96-97, 100-103, 107, 110-113, 141, 144, 148, 149, 152, 154-157, 160-164	Candida.....	183, 284
ANA global test.....	96, 160	Cardiolipin.....	108, 109, 145, 148, 172, 173, 195
ANCA.....	54, 104, 105, 132, 133, 143, 149, 157	CartiLaps.....	262
Androstenedione.....	260	CASPR2.....	90, 91, 96, 126, 127, 153, 158
ANDV.....	95, 213	Cathepsin G.....	104, 105, 143
Ankylosing spondylitis.....	272, 273	CCP.....	20, 106, 107, 144, 147-149
ANNA.....	124	Cell nuclei.....	91-93, 96, 97, 100, 110, 152, 154-156, 160-164, 286
Anti-phospholipid syndrome.....	108	CENP A.....	88, 101, 111, 113, 140, 141
APS.....	108, 109, 149	CENP B.....	30, 88, 101, 111, 113, 140, 141
AQP4.....	128	Centromere.....	148
Aquaporin-4.....	90, 128, 129, 152	CEP-1.....	106, 107, 144
Arbovirus.....	94, 189, 211, 212, 214, 294, 295	Cerebellum.....	90, 96, 124, 125, 127, 151, 152
ASMA.....	91, 93, 97, 110, 111, 113, 156, 157, 162-164	Chemiluminescence .	14-15, 62-63, 87, 137, 147-149, 171, 191, 204-206, 231, 239-241, 259, 263-265
Aspergillus.....	15, 182, 183, 207, 240, 261, 284	Chikungunya virus.....	94, 95, 188, 189, 203, 211, 212, 214, 294, 295
Atopy.....	20, 222, 223, 232, 236-238	Chlamydia.....	94, 173-175, 186, 194, 196, 198, 209, 290
ATP4B.....	119, 143	ChLIA.....	11, 26, 62, 63, 104-107, 114, 115, 130-133, 147, 170, 171, 179, 187, 204, 245, 253, 263, 264
Autoimmune dermatoses.....	134, 135	Cholangitis.....	112
Autoimmune encephalitis.....	90, 126, 153	Chronic inflammatory bowel diseases.....	104, 116, 252
Autoimmune gastritis.....	15, 115, 117-119	Churg-Strauss syndrome.....	104
Autoimmune hepatitis.....	102, 110, 112	CIC.....	145
Automation.....	6, 8, 10, 20, 22, 40, 45, 48, 60, 61, 64, 74, 82, 86, 185	Circulating immune complexes.....	145
Avidity.....	178, 179, 187, 198-202, 205, 206, 213	cLED.....	50, 51
Avidity determination.....	179, 198-202	CMV.....	185, 186, 194, 199, 205, 206
		cN-1A.....	15, 88, 101, 141, 145





You can also search online at  
[www.euroimmun.com](http://www.euroimmun.com)



Coeliac disease.....	15, 93, 114, 115, 117, 119, 142, 164, 278, 279	Eastern equine encephalitis virus.....	211
Collagen.....	105, 132-135, 143, 145, 255	EBV.....	89, 178, 179, 184, 193, 195, 196, 205, 206, 213
Collagen type VII.....	134, 135, 143, 145	Echinococcus.....	188, 189, 193, 196, 198
Collagenosis.....	102	EEEV.....	211
COMP.....	262	EJ.....	88, 89, 101, 141, 142
Connective tissue diseases.....	100	Elastase.....	104, 105, 143
Cortisol.....	260, 264, 265	ENA.....	101, 148
CoV.....	188	Encephalitis.....	14, 15, 90, 126, 127, 153, 184, 185, 188, 201, 211, 212, 214, 290
COVID-19.....	11, 15, 176, 205, 206, 292	Endocrinopathies.....	118, 244
Coxiella burnetii.....	15, 198	Endomysium.....	88, 93, 97, 114, 115, 134, 140, 142, 145, 147, 164, 165, 279
Coxsackie virus.....	94, 212	Endothelial cells.....	165
Crimean Congo fever virus.....	188, 202, 203, 213	Enterovirus.....	202
Crithidia.....	52, 54, 93, 97, 102, 103, 161, 162	Envoplakin.....	134, 135, 143
CRMP5.....	124	Eonis.....	78, 79
Crohn's disease.....	104, 115, 116, 119, 252	Epidermis.....	92, 134, 158, 159, 170
CrossLaps.....	255, 262, 264, 265	Epstein-Barr virus.....	95, 178, 185, 193, 202, 204, 213
CSF.....	84, 85, 126, 170, 184, 185, 191, 197-202, 207, 208, 244-247, 259-261, 263	Estrone.....	260
CSQ pair of controls.....	208	EUROArray.....	11, 34, 74-78, 173, 175, 183, 268, 270-280, 283-287, 290, 291, 299-302, 305, 307
CSQrel.....	84, 184	EUROArrayProcessor.....	74-76
CTX-I.....	255, 262, 264, 265	EUROArrayScanner.....	10, 74, 76, 77
CTX-II.....	262	EUROASSAY.....	28, 137, 139, 231, 232
CUZD1.....	116, 117, 157	EUROBlotMaster.....	30, 32, 60, 61, 64, 65
CV2.....	88, 90, 96, 124-126, 140, 151, 152	EUROBlotOne.....	10, 30, 32, 60, 61, 68, 69, 138, 192
CXCL13.....	184, 207, 261	EUROBlotScanner.....	66, 67
Cyclic citrullinated peptide.....	107	EUROIMMUN Analyzer I.....	56, 57, 60, 61, 70, 84
Cytomegalovirus.....	14, 185-187, 199	EUROIMMUN Analyzer I-2P.....	56, 57, 61
		EUROIMMUN CSF Software.....	84, 85, 184, 185
dp-uc MGP.....	264, 265	EUROLabOffice.....	11, 30, 32, 44, 48, 52, 54, 60, 66, 68, 82, 83
DBS.....	20, 60, 61	EUROLabWorkstation ELISA.....	11, 58-61, 70, 84
Dehydroepiandrosterone.....	260	EUROLabWorkstation IFA.....	11, 46, 47, 96, 97
Dehydroepiandrosterone sulfate.....	260	EUROLINE....	30-33, 64, 87-89, 102, 111-119, 124, 129, 137-138, 140-142, 191-195, 218-238, 305-306
Dengue virus.....	15, 94, 188, 189, 201, 207, 211, 212, 214, 260, 295	EUROLineScan.....	30, 32, 66-68, 70, 306
Dermatitis herpetiformis.....	114, 134, 279	EUROLINE-WB.....	32, 33, 64, 66, 191, 193, 195, 196
Dermatomycosis.....	11, 183, 284, 285, 302	EUROPattern.....	10, 52-55, 87, 90-97, 137, 151-164, 175, 191, 209-214
Dermatophytes.....	183, 284, 285	EUROPattern Microscope Live.....	52, 53
Desmoglein.....	9, 92, 134, 135, 143, 159	EUROPLUS.....	10, 91-92, 96, 101, 104-105, 113-115, 133, 151, 155-161, 162, 164, 179, 209, 213, 279
Desmosomes.....	92, 134, 158	EURORealTime.....	11, 36, 78, 80, 81, 177, 185, 291-297, 299, 303
Diabetes.....	14, 120-122, 280	EURORealTime Analysis.....	36, 78, 80, 81, 291, 292, 294, 296
DFS70.....	88, 101, 141, 142, 144	EUROSORB.....	191
DHEA.....	260	EUROStar III Plus.....	50, 51
DHEA-S.....	260	Exanthema.....	178, 274
DNER.....	88, 124, 125, 140, 152	Eye.....	154, 174
DOBV.....	94, 195, 212	Eye antigens.....	154
DPA-Dx.....	10, 226-229, 232, 234, 236, 238	F-actin.....	91, 93, 110, 111, 156, 157, 162
DPPX.....	90, 126, 127, 153	Factor V / Factor II.....	270
Dried blood spots.....	14, 15, 20, 60	Farr.....	102, 103
dsDNA.....	30, 88, 93, 97, 101-103, 141, 144, 148, 150, 161, 162	Fibrillarlin.....	88, 101, 141
		Flavivirus.....	189, 211



Food.....	6, 14, 180, 220-223, 226, 227, 232, 234-236, 280, 283
Free estriol.....	260
Free testosterone.....	260, 264, 265
Free thyroxine.....	123, 150, 260
Free triiodothyronine.....	123, 150, 260
Fructose intolerance.....	282, 283, 300
FT3.....	122, 123, 150, 260
FT4.....	122, 123, 150, 260
Fungal infections.....	11, 284
FV/FII.....	270, 271, 300, 301
GABA B.....	90, 126, 127, 153
GAD.....	121, 125, 128, 129, 143, 151
GAF-3X.....	9, 11, 88, 115, 117, 119, 134, 140, 142, 146, 147, 164, 279
Gangliosides.....	128, 129, 140
GBM.....	91, 104, 105, 132, 133, 140, 143, 147-149, 155, 156
GD1b.....	128, 129, 140
Gliadin.....	20, 114, 115, 117, 119, 134, 146-148, 164
Glomerular basement membrane.....	91, 104, 130, 132, 133, 140, 143, 155, 156
Glomeruli.....	91, 130, 132, 156, 251
Glomerulonephritis.....	104, 130, 132, 250, 251
Glutamic acid decarboxylase.....	120, 121, 129, 151
Gluten-sensitive enteropathy.....	114, 279
GM1.....	128, 129, 140
GM2.....	129, 140
GM3.....	129, 140
Goblet cells.....	116, 117, 157
Goodpasture's syndrome.....	132
GP2.....	14, 116, 117, 157
GQ1b.....	128, 129, 140
Granulocytes.....	52, 90, 91, 96, 104, 105, 117, 118, 133, 154-157, 252
Grasses.....	218, 226
Graves' disease.....	122, 123
Growth hormone.....	264
GT1b.....	129, 140
Guillain-Barré syndrome.....	128, 294
Haemochromatosis.....	280, 281, 300
Hantavirus.....	94, 95, 188, 195, 202, 212, 213
Hashimoto's thyroiditis.....	122, 123
Heart muscle.....	158
Helicobacter pylori.....	14, 193, 195, 197
HEp-2.....	23, 52, 91-93, 96, 97, 100, 101, 103-105, 107, 111, 113, 133, 152, 154-156, 160-163
HEp-20-10.....	92, 93, 96, 97, 101, 160, 161, 163, 164
Hepatitis.....	14, 89, 102, 108, 110, 112, 172, 180, 194, 199
Hepatitis E virus.....	14, 89, 180, 194, 199
Hereditary haemochromatosis.....	280, 281
Herpes.....	185, 186, 193, 196, 199, 204, 290
Herpes simplex.....	185, 186, 193, 196, 199, 204, 290
HEV.....	180, 181, 199
HFE gene.....	280
hGH.....	264
HHV-6.....	94, 210
Hippocampus.....	127, 152
Histones.....	30, 88, 101, 103, 139, 141, 144
HIV.....	178, 182, 184, 274
HLA-B27.....	272, 273, 300
HLA-B57.....	274, 275, 300
HLA-Cw6.....	276, 277, 300
HLA-DQ2/DQ8.....	278, 279, 300
Hormones.....	122, 259-264
House dust.....	218, 239
HPV.....	286-288, 302
HSV-1.....	173, 175, 185, 187, 194, 196, 199, 204, 205, 290, 291, 302, 303
HSV-2.....	9, 173, 175, 187, 194, 196, 199, 204, 205, 290, 291
HTNV.....	94, 195, 212
Hu.....	88, 90, 96, 124-126, 140, 151, 152
Human papillomavirus.....	286, 287
HUVEC.....	185
IA2.....	120, 121, 143
ICAP.....	100, 101
IDS-iSYS.....	62, 63, 89
IDS-i10.....	62, 63
IgE.....	14, 146, 218-226, 228, 229, 231-241, 306
IGFBP-3.....	264, 265
IGF-I.....	264, 265
IgLON5.....	127, 153, 154
Immunofluorescence 6-9, 15, 22-23, 32, 42-54, 87, 90-97, 100-104, 124, 134, 137, 151-165, 209-214	
InaKtif MGP.....	264, 265
Infectious mononucleosis.....	178
Infliximab.....	146
Influenza virus.....	202, 292, 293
Inhalation.....	182, 218, 219, 222, 223, 226, 232-234, 296
Insect venoms.....	227-229, 232, 237, 238
Insulin.....	120, 121, 150
Insulin-like Growth Factor-I.....	264, 265
Insulin-like Growth Factor Binding Protein-3.....	264, 265
Intact PINP.....	255, 264, 265
Intact parathyroid hormone.....	257
Intact PTH.....	257, 260, 264, 265
Intestinal goblet cells.....	116, 117, 157
Intestinal mucosa.....	116
Intestinal tissue.....	90, 96, 125, 151, 152
Intrinsic factor.....	88, 115, 117-119, 140, 143, 157
iPTH.....	257



You can also search online at  
[www.euroimmun.com](http://www.euroimmun.com)



IRMA .....	38, 150	Microarray.....	35, 278, 280, 283, 284
Islet cells .....	90, 120, 121, 151	Microscopic polyangiitis .....	104
Japanese encephalitis virus .....	15, 188, 201, 211, 212, 214	Microscopy .....	6, 15, 17, 48, 50-55, 130, 182, 296
Jo-1.....	28, 30, 88, 89, 101, 139, 141, 142, 144, 145, 148, 161	Microtiter ELISA.....	24, 56
Ku.....	88, 101, 141, 142	Miller-Fisher syndrome.....	128
La crosse virus.....	211	Mites .....	218
Lactoferrin.....	104, 105, 143, 157	Mitochondria.....	91-93, 96, 97, 156, 157, 160, 162-164
Lactose intolerance.....	282, 283, 300	MOG .....	14, 90, 128, 129, 152, 154
Lambert-Eaton myasthenic syndrome.....	128	Molecular diagnostics .....	9
Laminin.....	15, 134, 135, 159	Molecular infectious diagnostics.....	299, 302, 303
LC-1.....	88, 110, 111, 113, 139, 140, 143	MOMP.....	174, 175
LCT gene.....	282, 283	Moulds .....	182, 183, 284, 285
Legionella.....	197	MPO.....	91, 96, 104, 105, 133, 140, 143, 147, 148, 155, 156
Leishmania .....	210	MRZ .....	14, 184
LEMS .....	128	MTB .....	296, 297, 303
Leptin.....	260	MTHFR .....	270, 271, 300, 301
Leydig cells .....	151	Multifocal motor neuropathy .....	128
LG11.....	90, 91, 96, 126, 127, 153, 158	Multiple sclerosis.....	14, 128, 184
Limbic encephalitis.....	15, 126	Mumps virus .....	14, 20, 185, 200
Listeria .....	209	Murray Valley encephalitis virus .....	211
Liver. 14-15, 88, 91-93, 96-97, 110-115, 139-140, 143, 149, 156-157, 160-165, 178, 180, 182, 280-282		Myasthenia gravis .....	91, 128, 158
Liver antigens .....	156	Mycoplasma.....	94, 173, 198, 210, 290
Liver diseases.....	15, 88, 91, 111, 113, 140, 157	Myelin .....	128, 129
Liver-kidney microsomes.....	110, 111, 143, 156	Myelin-associated glycoprotein.....	128
LKM .....	91, 93, 97, 111, 156, 157, 163, 164	Myeloperoxidase.....	91, 96, 104, 140, 143, 155, 156
LKM-1.....	88, 110, 111, 113, 139, 140, 143, 148	Myositis .....	14, 15, 100, 101, 141
Lupus anticoagulant.....	108	N-MID .....	255, 262, 264, 265
Lyme borreliosis .....	170	Nerves.....	90, 96, 128, 129, 151, 152
M2.....	30, 88, 89, 112, 113, 139-142, 148, 162, 219, 223, 228, 232-234, 236-238, 251	Neurofilament.....	246, 247, 261
M4.....	139, 142, 233	Neurogranin.....	14, 245, 261
M9.....	139, 142	Neurology.....	9, 90, 96, 124, 125, 151-153
Ma2.....	124, 126	Neuromyelitis optica .....	128
Ma2/Ta.....	124	Neuronal antigens .....	140
MAb.....	151	Neuropathy.....	128
MAG .....	128, 129	NMDAR.....	9, 14, 127
Malaria.....	296	NOR90 .....	88, 101, 141
Mayaro-Viren.....	203	nRNP/Sm .....	28, 30, 88, 101, 103, 139, 141, 144, 161
Measles virus .....	20, 184, 185, 200	Nuclear membrane .....	113
Membranous nephropathy.....	10, 14, 15, 130, 131, 156	Nucleosomes.....	30, 88, 101-103, 141, 144
Meningitis.....	184, 290	Oesophagus .....	92, 114-116, 134, 135, 158, 159
Meningoencephalitis.....	184	OJ.....	88, 89, 101, 141, 142
MERGITE!.....	11, 42, 43, 46, 74	Optical nerve.....	128
MERS-CoV .....	188	OspC .....	89, 171, 194, 197, 209
Mi-2 .....	88, 101, 141	Ostase .....	255, 262, 264, 265
		Osteocalcin .....	255, 262, 264, 265
		Ovarian antigens .....	151



Ovary.....	151	RA Analyzer 10.....	11, 147, 171, 204, 263
pANCA.....	90, 91, 96, 104, 143, 154-157	Random access.....	11, 26, 62, 63, 107, 171
Pancreas.....	90, 96, 112, 116, 117, 120, 121, 125, 151, 152, 157, 280	RC-IFT.....	9
Pancreas islets.....	90, 96, 151, 152	Real-time PCR.....	17, 36, 37, 78, 79, 81, 291, 292, 294, 296
Parainfluenza virus.....	202	Recoverin.....	88, 125, 140
Paraneoplastic neurological syndromes.....	124	Renal glomeruli.....	91, 156
Parasites.....	184	Renal glomeruli (GBM).....	91, 156
Parathyroid hormone.....	256, 257	Renin.....	261, 264, 265
Parietal cells.....	115, 117-119, 143, 151, 157	Respiratory syncytial virus (RSV).....	201
Parotid gland.....	158	Retina.....	154
Parvovirus.....	14, 108, 186, 194, 199, 204-206	Reverse triiodothyronine.....	260
PBC.....	111-113	Rheumatoid arthritis.....	14, 106
PCA.....	88, 115, 117-119, 140, 143, 151, 157	Rheumatoid factors.....	106
PCNA.....	30, 88, 101, 141, 144	Ri.....	88, 90, 96, 124, 125, 140, 151, 152
PCR.....	14-17, 34-37, 72-74, 78-81, 168, 174-180, 270-280, 283-284, 286, 290-292, 294, 296, 299, 303	RIA.....	9, 38, 102, 103, 121, 123, 129, 150
PDGFR.....	88, 101, 141	Ribosomal P-proteins.....	88, 89, 101, 139, 141, 142, 144, 145
Pemphigoid.....	15, 92, 134, 135, 159	Rift Valley fever virus.....	188, 213
Pemphigus.....	14, 134	Ro-52.....	30, 88, 89, 101, 111, 113, 139-142, 144
Pernicious anaemia.....	117-119	Ross River virus.....	211
PGDH.....	15, 111, 113, 140	RP11.....	88, 101, 141
Phosphatidylserine.....	108, 109, 145	rPAg1.....	116, 117, 157
Phospholipase A2 receptor.....	14, 15, 91, 130, 143, 147, 156	rPAg2.....	116, 117, 157
Phospho-Tau.....	245	RT3.....	260
Pituitary gland.....	280	Rubella virus.....	20, 185-187, 194, 196, 199
PL-12.....	88, 89, 101, 141, 142	Sa.....	14, 106, 144
PL-7.....	88, 89, 101, 141, 142	Saccharomyces cerevisiae.....	115-117, 119, 146, 157, 165
PLA2R.....	10, 91, 130, 131, 143, 147, 156	Saliva.....	259, 260, 264, 265, 293
Placenta.....	178	Salt-split skin.....	92, 134, 135, 159
Plakins.....	134	Sandfly fever virus.....	94, 188, 212
Plasma Renin Activity.....	261	SARS coronavirus.....	210
Plasmodium.....	188, 189, 198	SARS-CoV.....	176, 292
PML.....	88, 101, 111-113, 140, 141	SARS-CoV-2.....	11, 14, 15, 17, 20, 176, 177, 200, 204, 207, 260, 292, 293, 303
pMN.....	130, 131	sCD163.....	250, 251, 261
PM-Scl.....	30, 88, 141, 144	Schistosoma.....	188, 198, 210
PNMA2.....	88, 124, 125, 140	Scl-70.....	28, 30, 88, 101-103, 111, 113, 139-141, 144, 148, 161
PNS.....	124, 125	SEOV.....	94, 212
PR3.....	91, 96, 104, 105, 133, 140, 147, 155, 156	sex hormone-binding globulin.....	260
PRA.....	261	Sexually transmitted infections.....	290
Pregnenolone.....	260	SHBG.....	260, 264, 265
Pre-NAT II.....	72-74, 80, 307	Sindbis virus.....	188, 214
PreQ.....	88, 89, 142	Sjögren's syndrome.....	100
progesterone.....	264, 265	Skeletal muscle.....	91, 158
Proteinase 3.....	91, 96, 104, 105, 140, 143, 147, 155, 156	SLA/LP.....	88, 110, 111, 113, 139, 140, 143, 157
Psoriasis.....	276, 277, 284	SLE.....	100, 102, 109, 144
Purkinje cell cytoplasm.....	151	Sm.....	14, 28, 30, 88, 91, 101, 103, 139, 141, 144, 148, 157, 161
PUUV.....	94, 195, 212	Smooth muscles.....	91, 93, 97, 110, 156, 157, 162-164
		SNV.....	94, 95, 212, 213



You can also search online at  
[www.euroimmun.com](http://www.euroimmun.com)



soluble CD163 .....	250
SOX1 .....	88, 125, 140
Sp100 .....	88, 101, 111-113, 140, 141
Spermatozoa .....	151
Sprinter .....	10, 44, 45, 60, 61
Sprinter XL .....	10, 44, 45, 60, 61
SRP .....	88, 89, 101, 141, 142
SS-A .....	28, 30, 88, 101, 103, 111, 113, 139-141, 144, 148, 161
SS-B .....	28, 30, 88, 101, 103, 139, 141, 144, 148, 161
ssDNA .....	144
St. Louis encephalitis virus .....	211
STI .....	173, 175, 290, 291, 302
Stiff-person syndrome .....	128, 129, 151
Stomach .....	91, 93, 97, 111, 113, 118, 119, 151, 156, 157, 162-164
Stool dosage tubes .....	253
Stress .....	14, 282, 288
Strongyloides .....	188, 198
Syphilis .....	108, 172
Systemic lupus erythematosus .....	100, 102
Systemic sclerosis .....	14, 15, 88, 100, 141
Ta .....	14, 88, 124, 125, 140
TAb .....	151
TBE virus .....	20, 184, 189, 200, 201, 210-212
Testis .....	151
Testosterone .....	260, 264, 265
TG .....	122, 123, 143, 150, 151
Th/To .....	88, 101, 141
Thrombocyte antigens .....	156
Thrombosis .....	108, 270, 271
Thrombospondin type-1 domain-containing protein 7A .....	130, 131
THSD7A .....	14, 130, 131, 156
Thyroglobulin .....	122, 123, 143, 150, 151
Thyroid diseases .....	122
Thyroid gland .....	123, 151, 280
Thyroid peroxidase .....	123, 143, 150
Thyroid stimulating hormone .....	122
Thyrotropin .....	122, 123, 143, 150
Tick-borne encephalitis .....	185
Tissue transglutaminase .....	15, 88, 114, 115, 117, 119, 140, 142, 145, 147
Titin .....	88, 125, 128, 129, 140
Tongue .....	228
TORCH .....	14, 15, 186, 187
Toscana virus .....	202
Total IgE .....	146, 218-223, 228, 229, 241
Total tau .....	244, 245, 260, 263
Total testosterone .....	260, 264, 265
Toxocara .....	15, 196, 198
Toxoplasma gondii .....	184-187, 194, 198
TPO .....	122, 123, 143, 150
Tr .....	88, 124, 125, 140
TRAcP 5b .....	255, 262, 264, 265
TRAb .....	122, 123
Transglutaminase .....	15, 88, 114, 115, 117, 119, 134, 140, 142, 145, 147, 279
Trees .....	218, 234
Treponema pallidum .....	172, 173, 184-186, 192-195, 197, 209, 290
Tropical diseases .....	188
Trypanosoma cruzi .....	198
TSH .....	122, 123, 143, 150
TSH receptor .....	122, 123, 143, 150
tTG .....	114, 115, 117, 119, 147
Tuberculosis .....	182, 296, 297
Tyrosine phosphatase .....	121
Ulcerative colitis .....	104, 116, 252
UNIQO 160 .....	48, 49
Ureaplasma urealyticum .....	94, 173, 210
Uromodulin .....	248, 249, 261
Usutu virus .....	201
Validation .....	24, 66, 88, 89, 140, 194
Varicella zoster virus .....	185, 186, 200, 210, 291
Vasculitis .....	104, 132, 172
VGKC .....	126
Vimentin .....	106
Vitamin D .....	20, 256, 257, 260, 262, 264, 265
VisE .....	9, 11, 89, 171, 194, 195, 197, 209
Voltage-gated potassium channels (VGKC) .....	126
VSM47 .....	91, 93, 110, 111, 156, 157, 162
VZV .....	184-186, 194, 200, 205, 210, 291, 302
WEEV .....	211
West Nile virus .....	188, 201, 211, 212
Western equine encephalitis virus .....	211
Western blot .....	32, 33, 64, 66, 110, 191, 193, 195, 196, 305, 306
Whooping cough .....	168
Yellow fever virus .....	94, 188, 189, 211, 212
Yersinia enterocolitica .....	193, 194, 196, 198
Yo .....	88, 90, 96, 124, 125, 140, 151, 152
Zic4 .....	88, 124, 125, 140
Zika virus .....	14, 15, 20, 94, 188, 189, 201, 211, 212, 294, 295, 303







